

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
 Data File : BF115181.D
 Acq On : 25 Jun 2019 11:10
 Operator : HP/JU
 Sample : PB120870BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120870BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5330952	6235955	74.06%	9.450%
2	6.254	727	734	737	rBV	5362465	6417633	76.22%	9.726%
3	6.384	750	756	759	rBV	6182826	6570781	78.04%	9.958%
4	6.613	791	795	798	rBV	2026101	1728978	20.53%	2.620%
5	6.772	817	822	825	rBV	5386562	5381486	63.92%	8.155%
6	7.172	884	890	893	rBV	4035933	4259751	50.59%	6.455%
7	7.889	1007	1012	1016	rBV	2536536	2247606	26.69%	3.406%
8	8.972	1190	1196	1199	rBV	7295334	7936059	94.26%	12.027%
9	9.636	1304	1309	1325	rBV2	2836631	2661276	31.61%	4.033%
10	10.419	1437	1442	1465	rBV	4649260	5124795	60.87%	7.766%
11	11.107	1555	1559	1563	rBV	3176134	2890530	34.33%	4.380%
12	12.701	1824	1830	1833	rBV	7479958	8419738	100.00%	12.760%
13	13.724	2000	2004	2015	rBV	2749065	2700726	32.08%	4.093%
14	14.830	2187	2192	2196	rBV	111878	124521	1.48%	0.189%
15	15.089	2231	2236	2245	rBV	1977383	2512165	29.84%	3.807%
16	15.165	2245	2249	2255	rVB	163175	206889	2.46%	0.314%
17	15.548	2309	2314	2319	rBV	142488	193951	2.30%	0.294%
18	15.989	2384	2389	2395	rVB	111518	171785	2.04%	0.260%
19	16.506	2471	2477	2483	rBV	59125	114433	1.36%	0.173%
20	17.112	2574	2580	2587	rVB2	40307	87841	1.04%	0.133%


Sum of corrected areas: 65986899

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115181.D
Acq On : 25 Jun 2019 11:10
Operator : HP/JU
Sample : PB120870BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120870BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

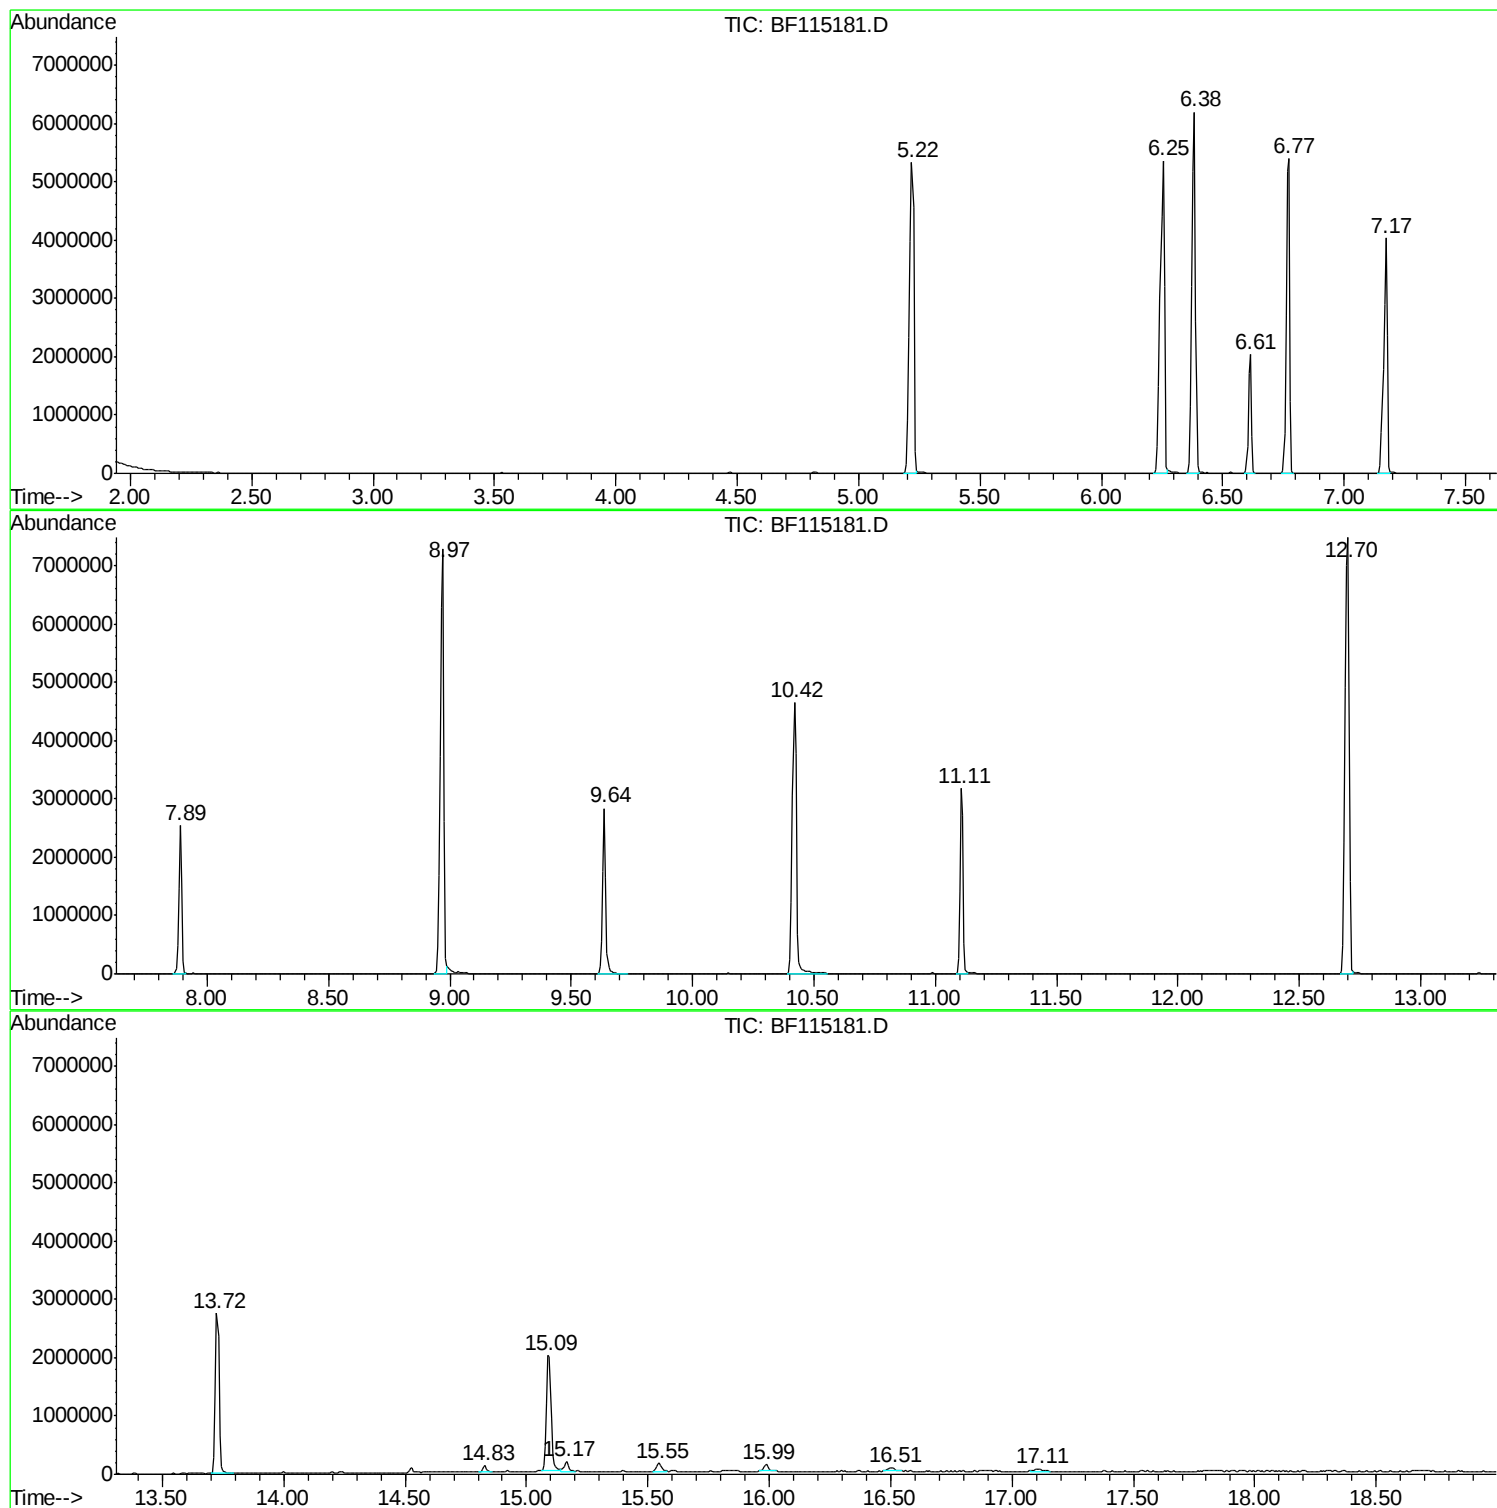

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115181.D
Acq On : 25 Jun 2019 11:10
Operator : HP/JU
Sample : PB120870BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120870BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	76.01 ng	6570780	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		2H-Cyclopenta[d]pyridazine, 2-methyl-	132	C8H8N2	022291-85-6	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

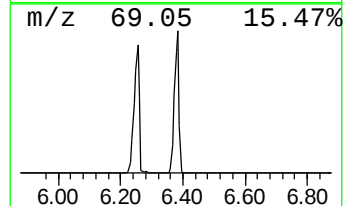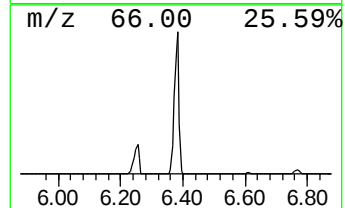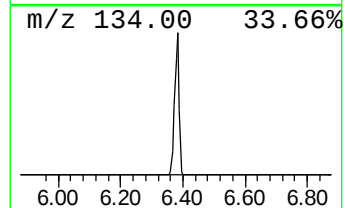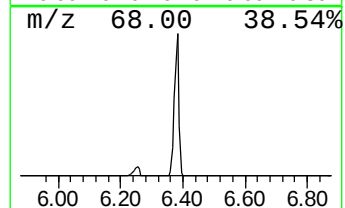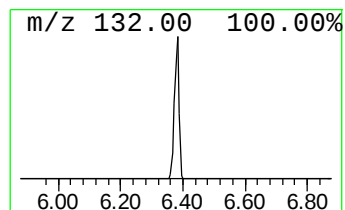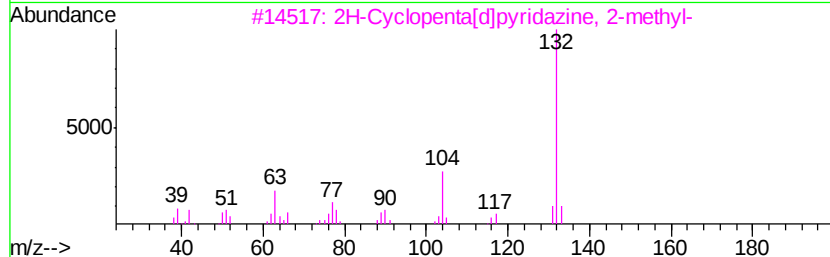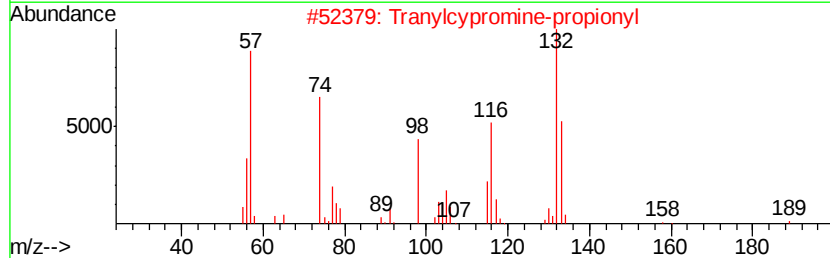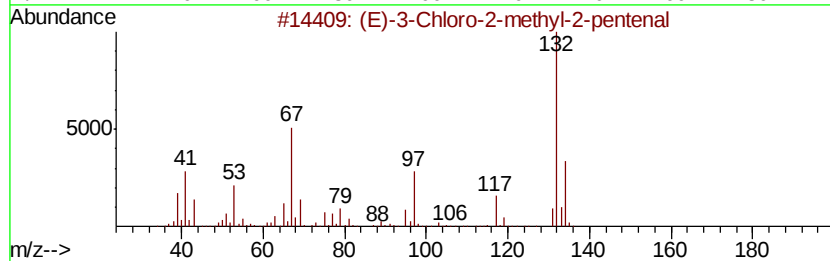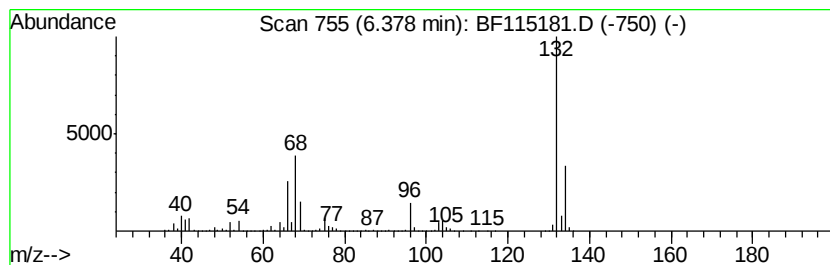

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
Data File : BF115181.D
Acq On : 25 Jun 2019 11:10
Operator : HP/JU
Sample : PB120870BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120870BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	76.0	ng	6570780	1	6.61	1728980	20.0