

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115187.D
Acq On : 25 Jun 2019 15:07
Operator : HP/JU
Sample : PB120785BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120785BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5319661	5688868	71.88%	9.535%
2	6.254	727	734	737	rBV	5175602	5795512	73.23%	9.714%
3	6.378	750	755	759	rBV	5501547	6077498	76.79%	10.187%
4	6.613	791	795	798	rBV	1750954	1611769	20.36%	2.702%
5	6.766	817	821	824	rBV	5273381	4988149	63.03%	8.361%
6	7.172	884	890	893	rBV	3786181	3893516	49.20%	6.526%
7	7.889	1007	1012	1015	rBV	2349179	2089120	26.40%	3.502%
8	8.972	1190	1196	1199	rBV	6702333	7329530	92.61%	12.285%
9	9.636	1303	1309	1329	rBV	2520166	2482452	31.37%	4.161%
10	10.419	1437	1442	1463	rBV	4396408	4533895	57.29%	7.599%
11	11.107	1555	1559	1563	rBV	3091802	2662131	33.64%	4.462%
12	12.695	1824	1829	1832	rBV2	7196745	7914453	100.00%	13.266%
13	13.724	2000	2004	2017	rBV	2437105	2438184	30.81%	4.087%
14	15.095	2231	2237	2247	rBV	1508041	2155560	27.24%	3.613%


Sum of corrected areas: 59660637

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115187.D
Acq On : 25 Jun 2019 15:07
Operator : HP/JU
Sample : PB120785BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120785BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

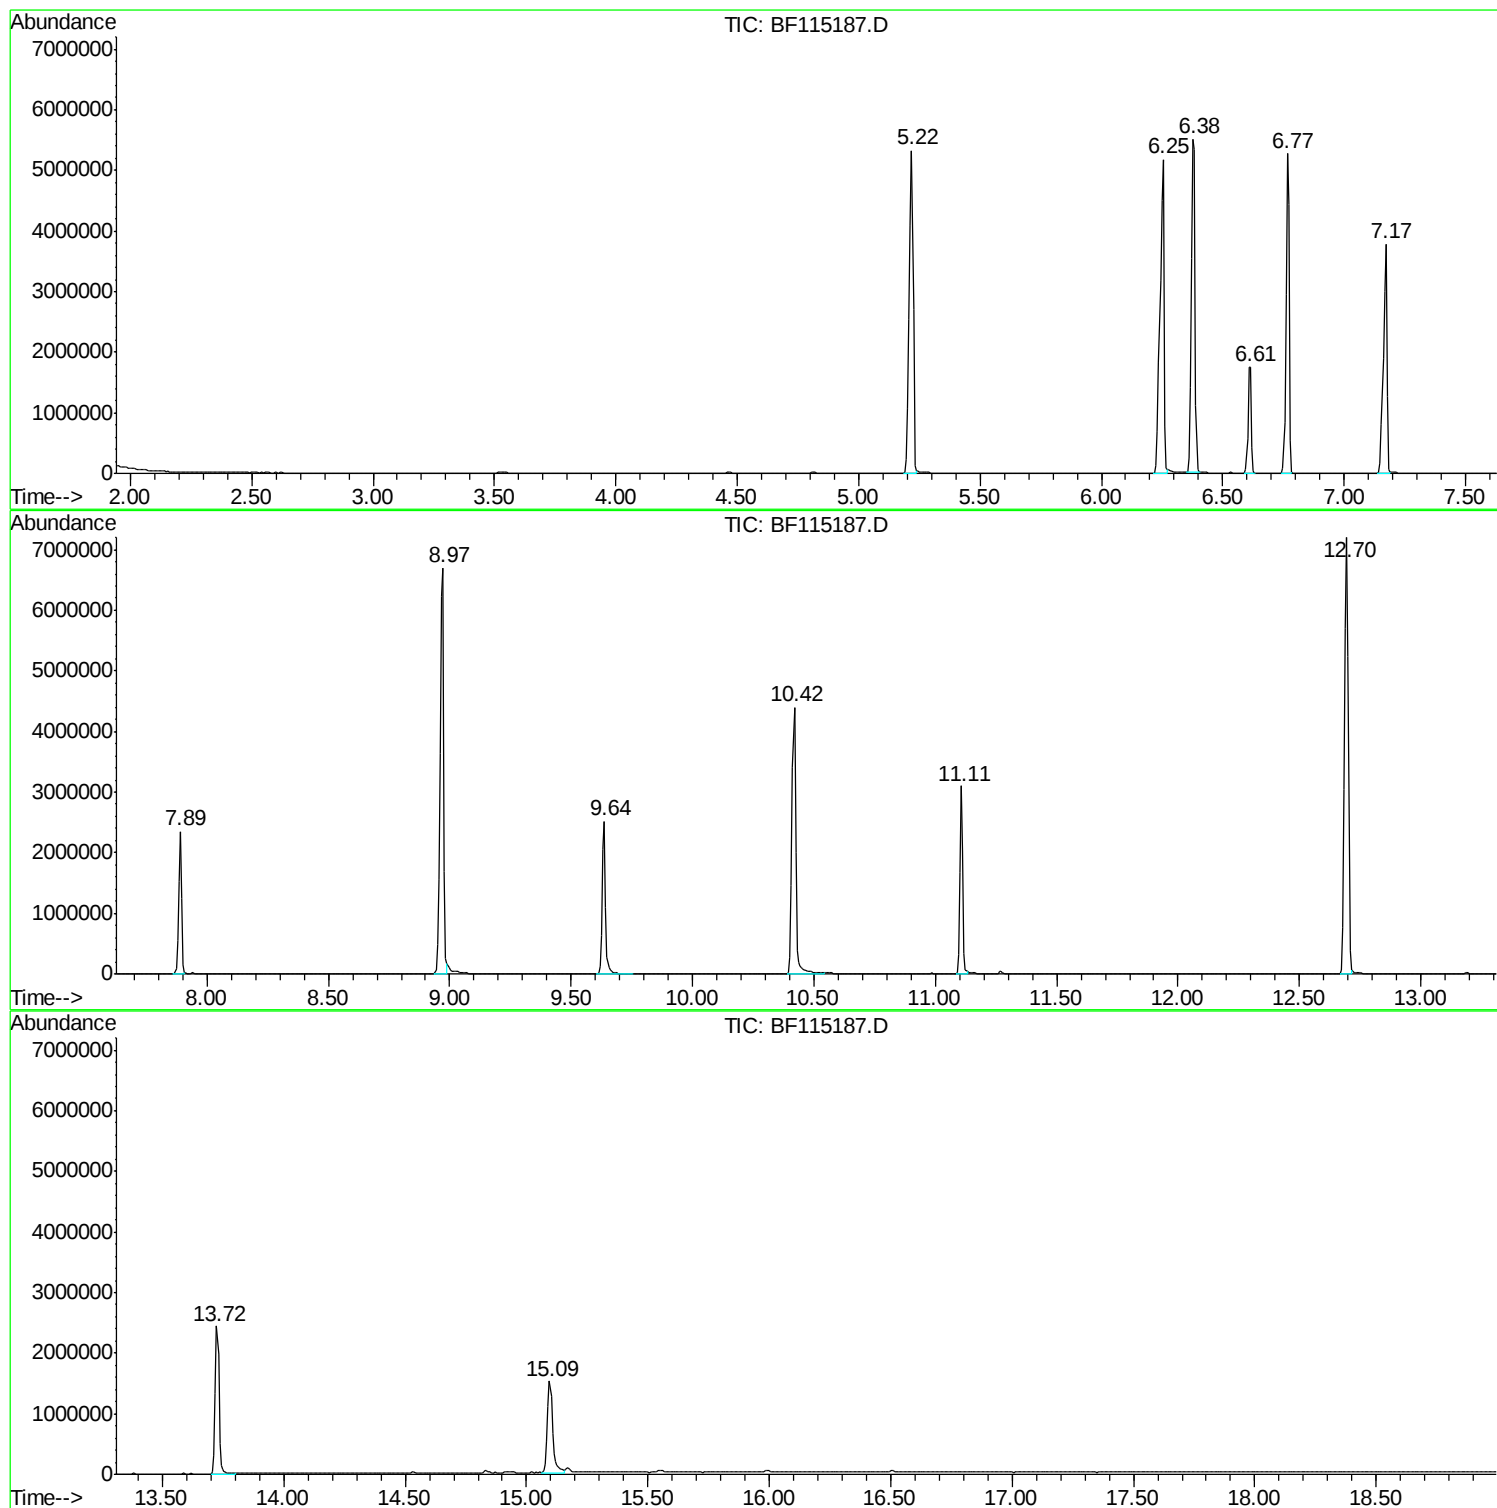

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115187.D
Acq On : 25 Jun 2019 15:07
Operator : HP/JU
Sample : PB120785BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120785BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	75.41 ng	6077500	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

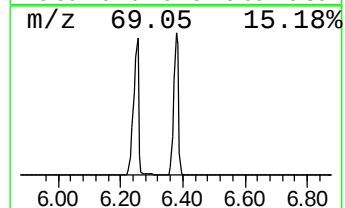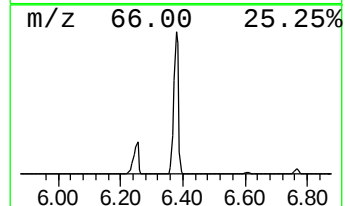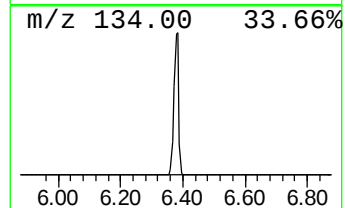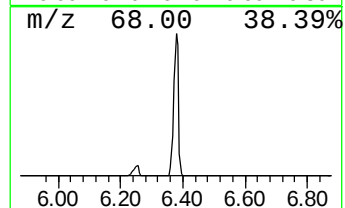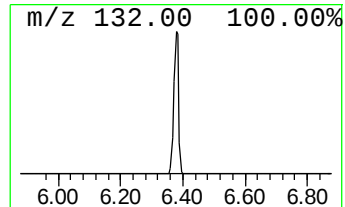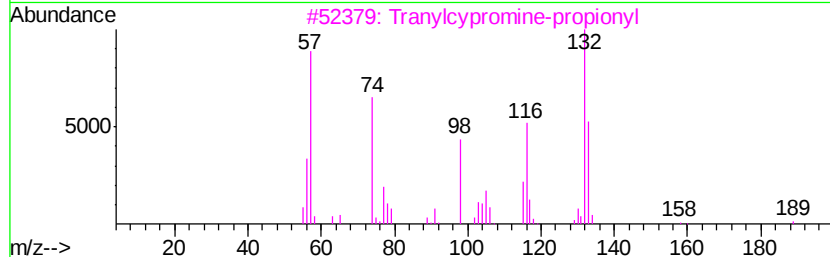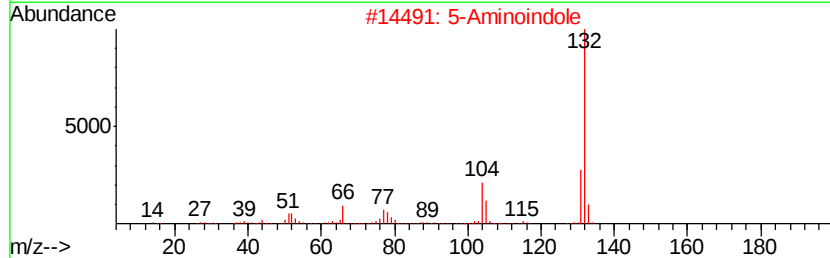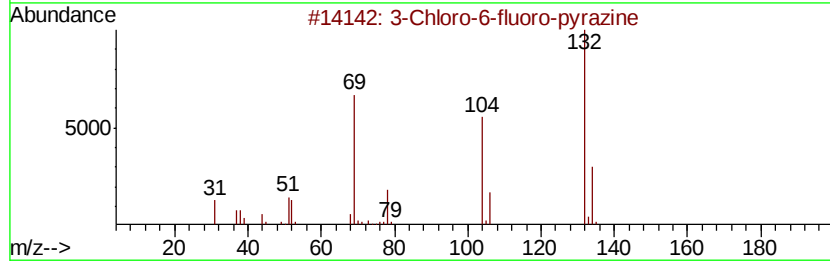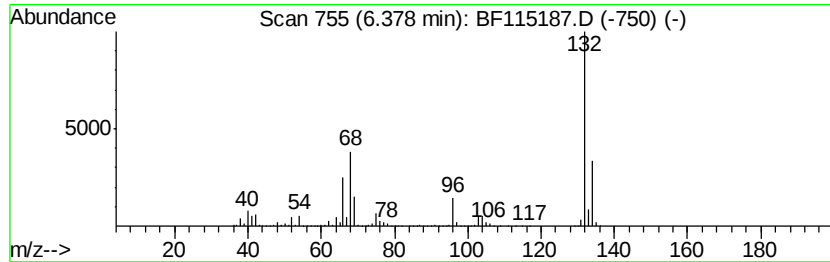

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
Data File : BF115187.D
Acq On : 25 Jun 2019 15:07
Operator : HP/JU
Sample : PB120785BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120785BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	75.4	ng	6077500	1	6.61	1611770	20.0