

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
 Data File : BF115188.D
 Acq On : 25 Jun 2019 15:34
 Operator : HP/JU
 Sample : PB120785TB
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120785TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5296367	5846477	73.04%	9.581%
2	6.254	727	734	737	rBV	5319233	5912244	73.86%	9.689%
3	6.378	750	755	759	rBV	5476039	6233058	77.87%	10.215%
4	6.607	791	794	798	rBV	1842100	1650382	20.62%	2.705%
5	6.766	817	821	824	rBV	5463488	5112334	63.87%	8.378%
6	7.172	884	890	893	rBV	3889619	3982181	49.75%	6.526%
7	7.889	1007	1012	1015	rBV	2354016	2147482	26.83%	3.519%
8	8.972	1190	1196	1199	rBV	6630436	7503970	93.74%	12.298%
9	9.636	1303	1309	1322	rBV	2595292	2535782	31.68%	4.156%
10	10.419	1437	1442	1458	rBV	4389332	4589082	57.33%	7.521%
11	11.107	1555	1559	1566	rBV	3284489	2748907	34.34%	4.505%
12	12.695	1824	1829	1832	rBV	7284458	8004730	100.00%	13.118%
13	13.724	2000	2004	2025	rBV	2589779	2500594	31.24%	4.098%
14	15.095	2232	2237	2247	rBV	1588807	2157306	26.95%	3.535%
15	15.165	2247	2249	2259	rVB	63968	95549	1.19%	0.157%


Sum of corrected areas: 61020078

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115188.D
Acq On : 25 Jun 2019 15:34
Operator : HP/JU
Sample : PB120785TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120785TB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

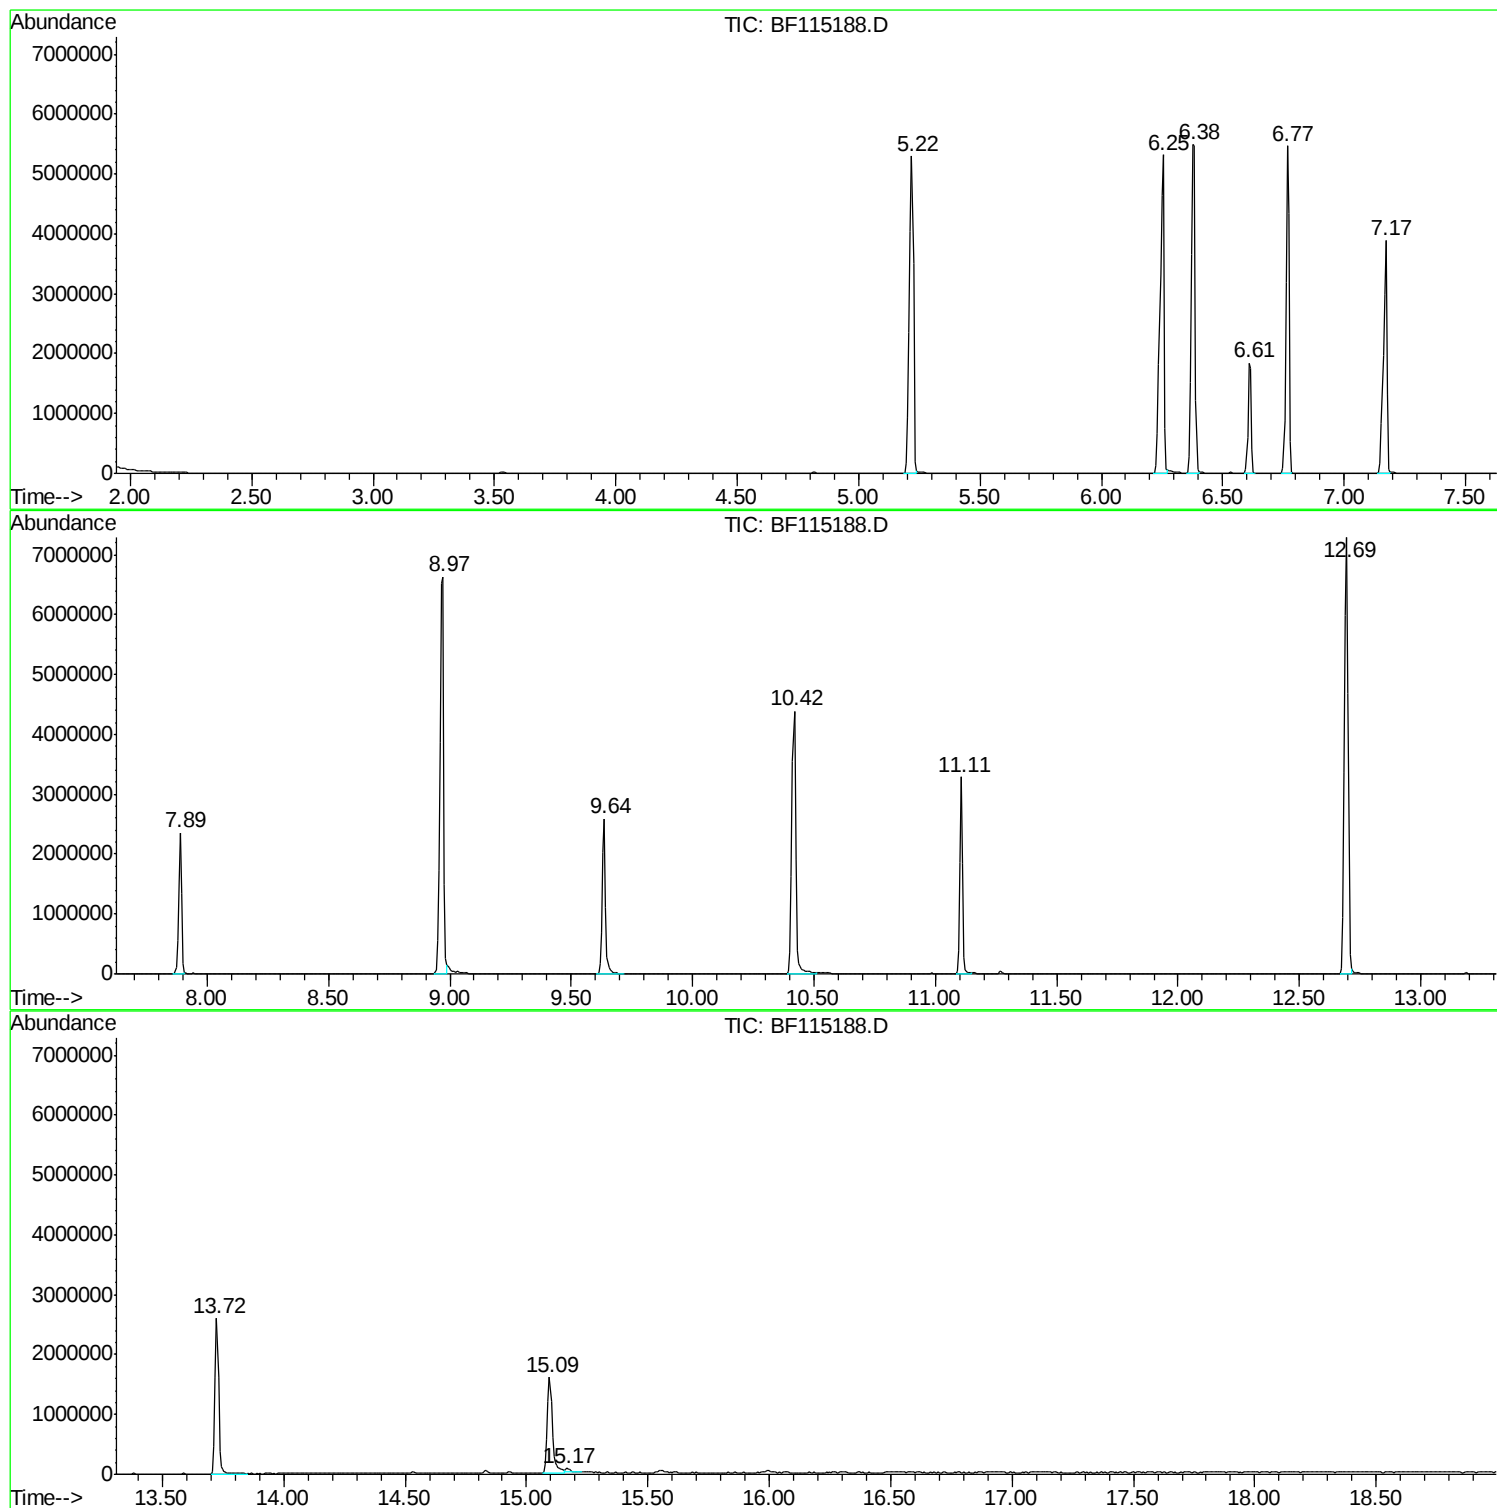

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115188.D
Acq On : 25 Jun 2019 15:34
Operator : HP/JU
Sample : PB120785TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120785TB









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	75.53 ng	6233060	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Amphetaminil	250	C17H18N2	017590-01-1	12

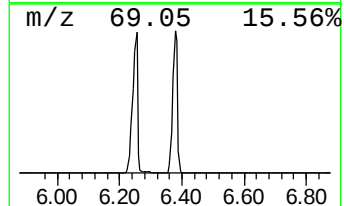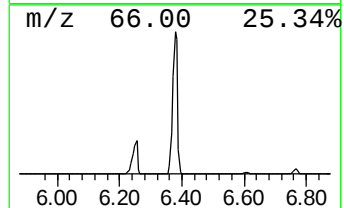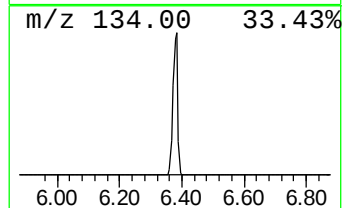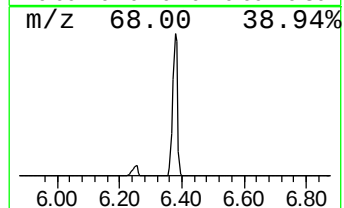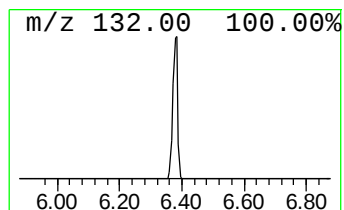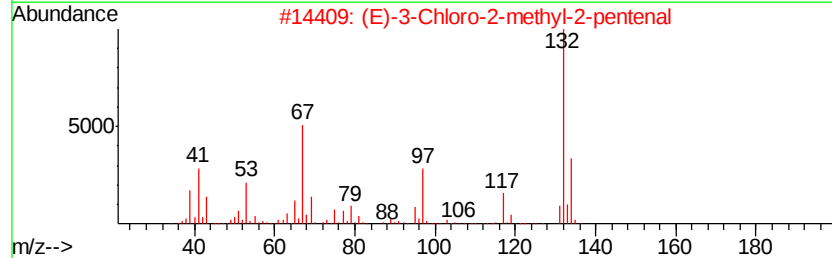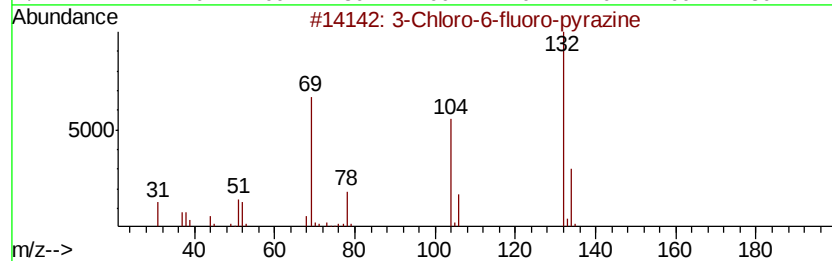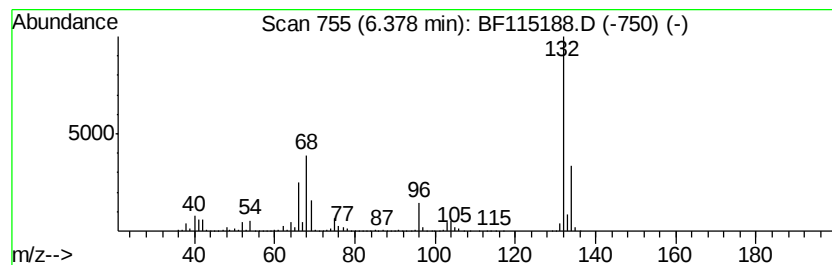

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
Data File : BF115188.D
Acq On : 25 Jun 2019 15:34
Operator : HP/JU
Sample : PB120785TB
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120785TB

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.38	6.38	75.5	ng	6233060	1	6.61	1650380	20.0