

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
 Data File : BF115190.D
 Acq On : 25 Jun 2019 16:27
 Operator : HP/JU
 Sample : PB120652BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120652BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.219	552	558	561	rBV	5357758	5745668	72.85%	9.439%
2	6.254	727	734	736	rBV	5192825	5821550	73.81%	9.563%
3	6.378	750	755	759	rBV	5455791	6136878	77.81%	10.081%
4	6.607	791	794	798	rBV	1774177	1630209	20.67%	2.678%
5	6.766	817	821	824	rBV	5296620	5072341	64.31%	8.333%
6	7.172	884	890	893	rBV	3831534	3916023	49.65%	6.433%
7	7.889	1007	1012	1015	rBV	2432369	2112511	26.79%	3.470%
8	8.972	1189	1196	1199	rBV	6651773	7409745	93.95%	12.172%
9	9.636	1303	1309	1326	rBV	2607209	2508814	31.81%	4.121%
10	10.419	1437	1442	1467	rBV	4410447	4548784	57.68%	7.473%
11	11.107	1555	1559	1566	rBV	3188247	2700644	34.24%	4.436%
12	12.695	1824	1829	1832	rBV	7298610	7886844	100.00%	12.956%
13	13.724	2000	2004	2020	rBV	2694924	2464240	31.24%	4.048%
14	15.089	2231	2236	2245	rBV	1628564	2187971	27.74%	3.594%
15	15.165	2245	2249	2261	rVB	117816	173937	2.21%	0.286%
16	15.548	2309	2314	2319	rBV	102656	149128	1.89%	0.245%
17	15.983	2382	2388	2397	rVB	98823	168150	2.13%	0.276%
18	16.501	2469	2476	2482	rBV2	65652	130453	1.65%	0.214%
19	17.106	2573	2579	2592	rVB2	46269	109522	1.39%	0.180%


Sum of corrected areas: 60873412

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115190.D
Acq On : 25 Jun 2019 16:27
Operator : HP/JU
Sample : PB120652BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120652BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

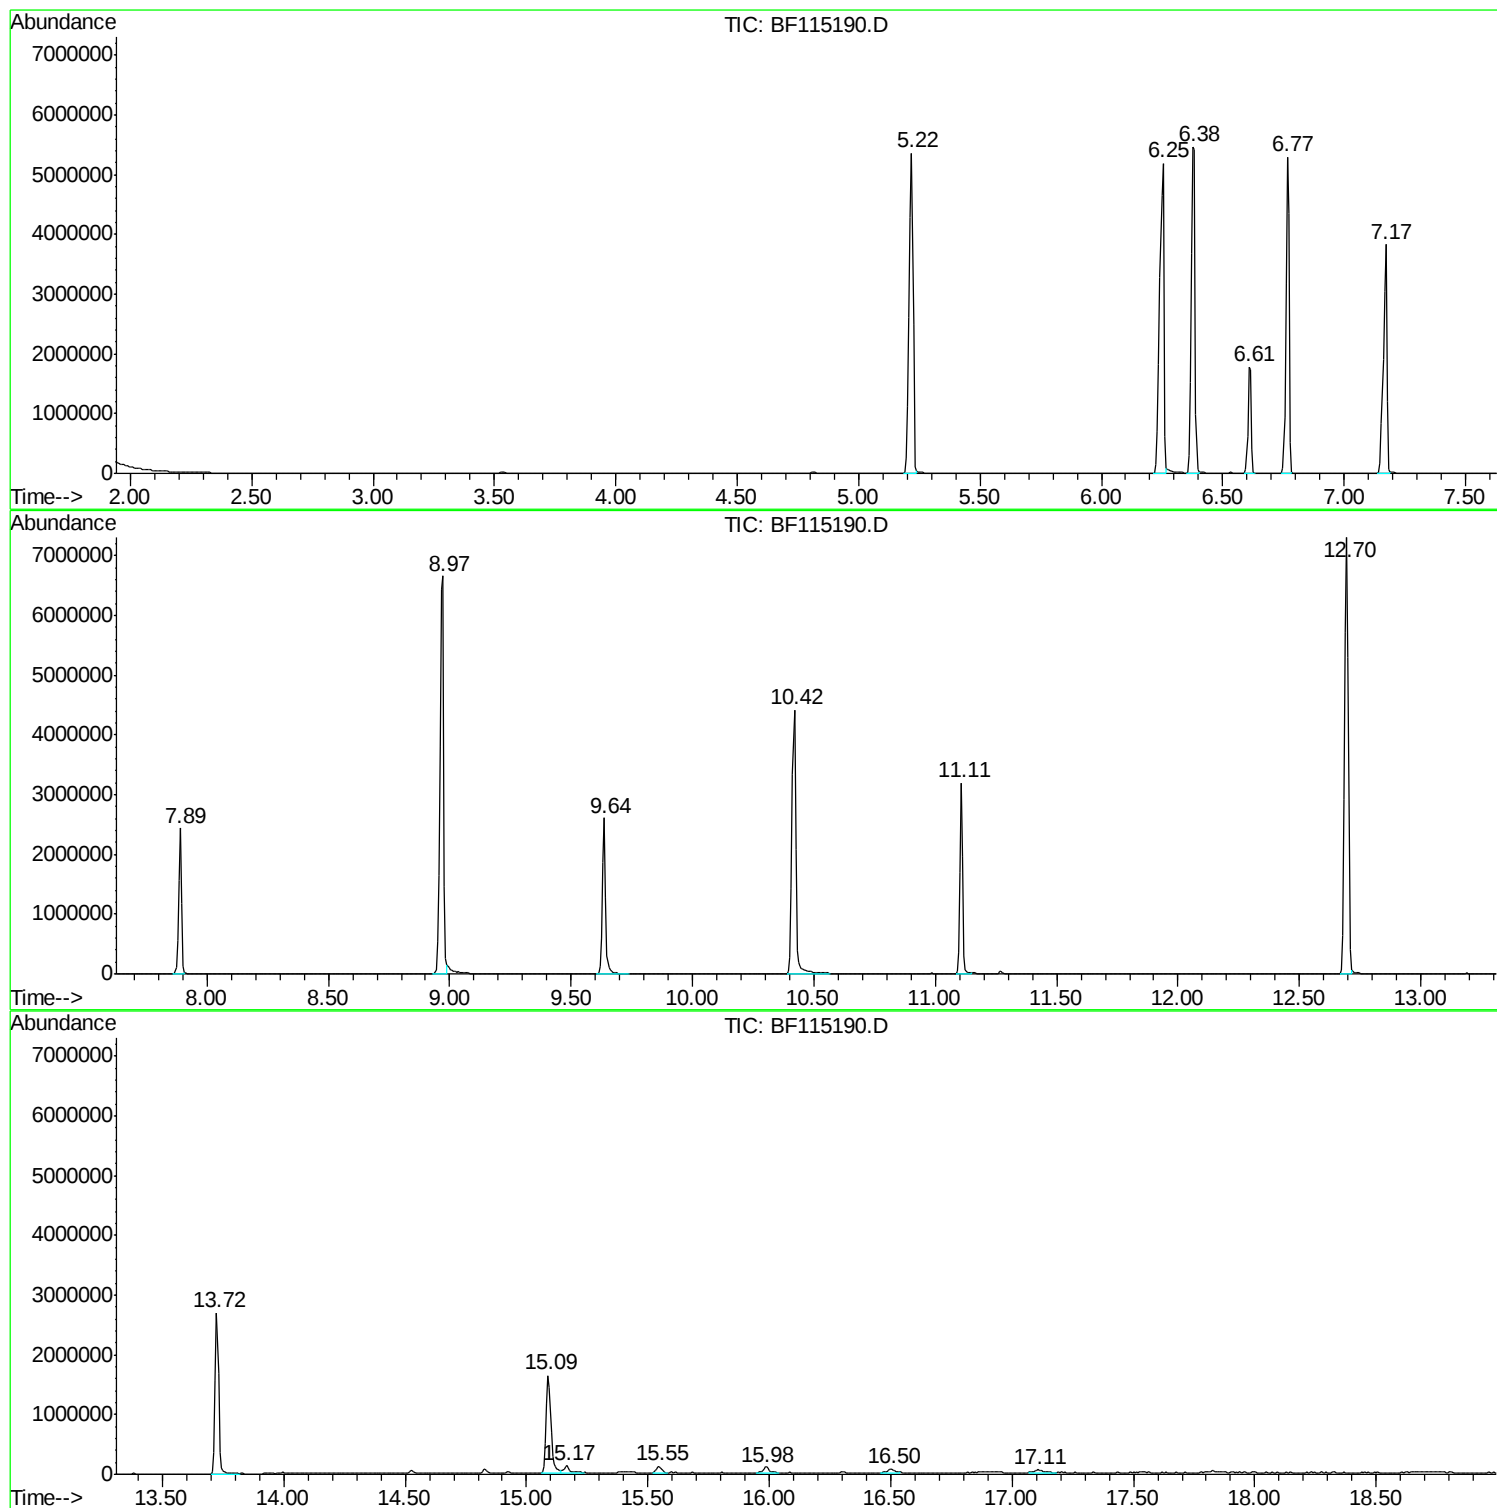

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062519\
Data File : BF115190.D
Acq On : 25 Jun 2019 16:27
Operator : HP/JU
Sample : PB120652BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120652BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.38 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	75.29 ng	6136880	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Xenon	132	Xe	007440-63-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

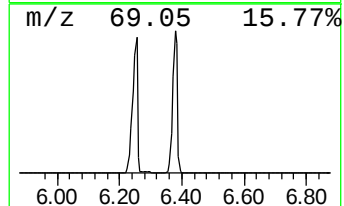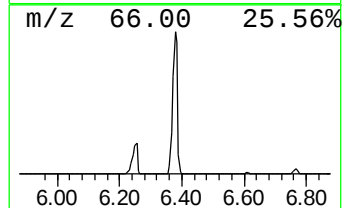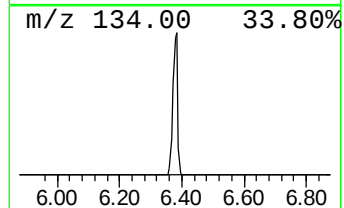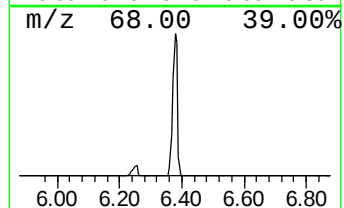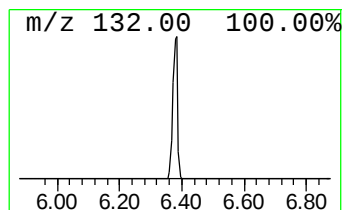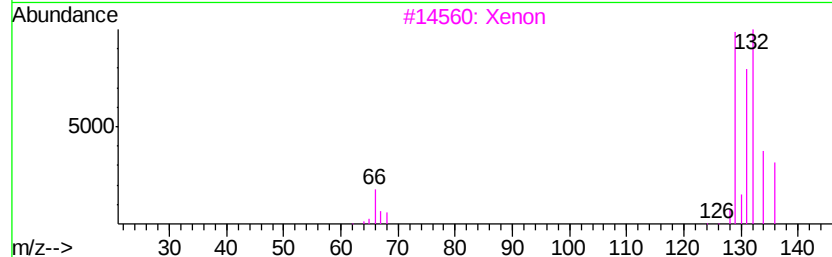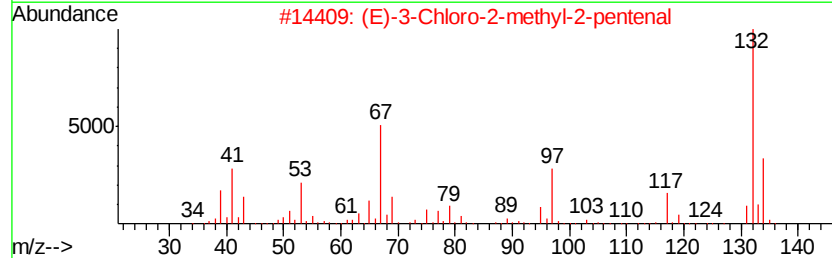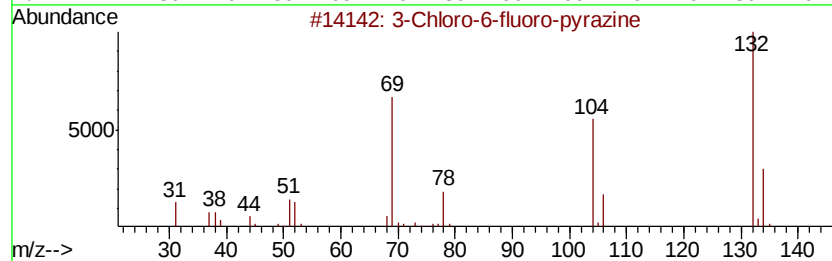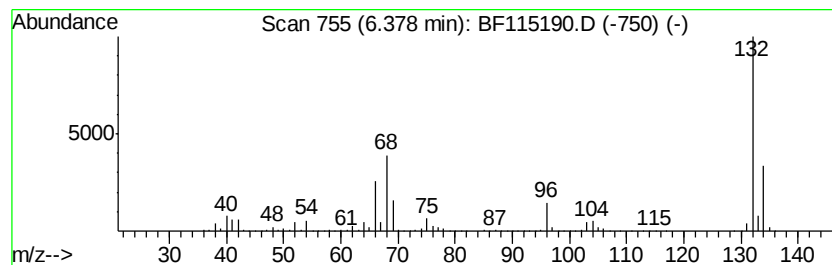

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
Data File : BF115190.D
Acq On : 25 Jun 2019 16:27
Operator : HP/JU
Sample : PB120652BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120652BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.38	6.38	75.3	ng	6136880	1	6.61	1630210	20.0