


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062519\
Data File : BF115191.D
Acq On : 25 Jun 2019 17:00
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 26 12:16:21 2019

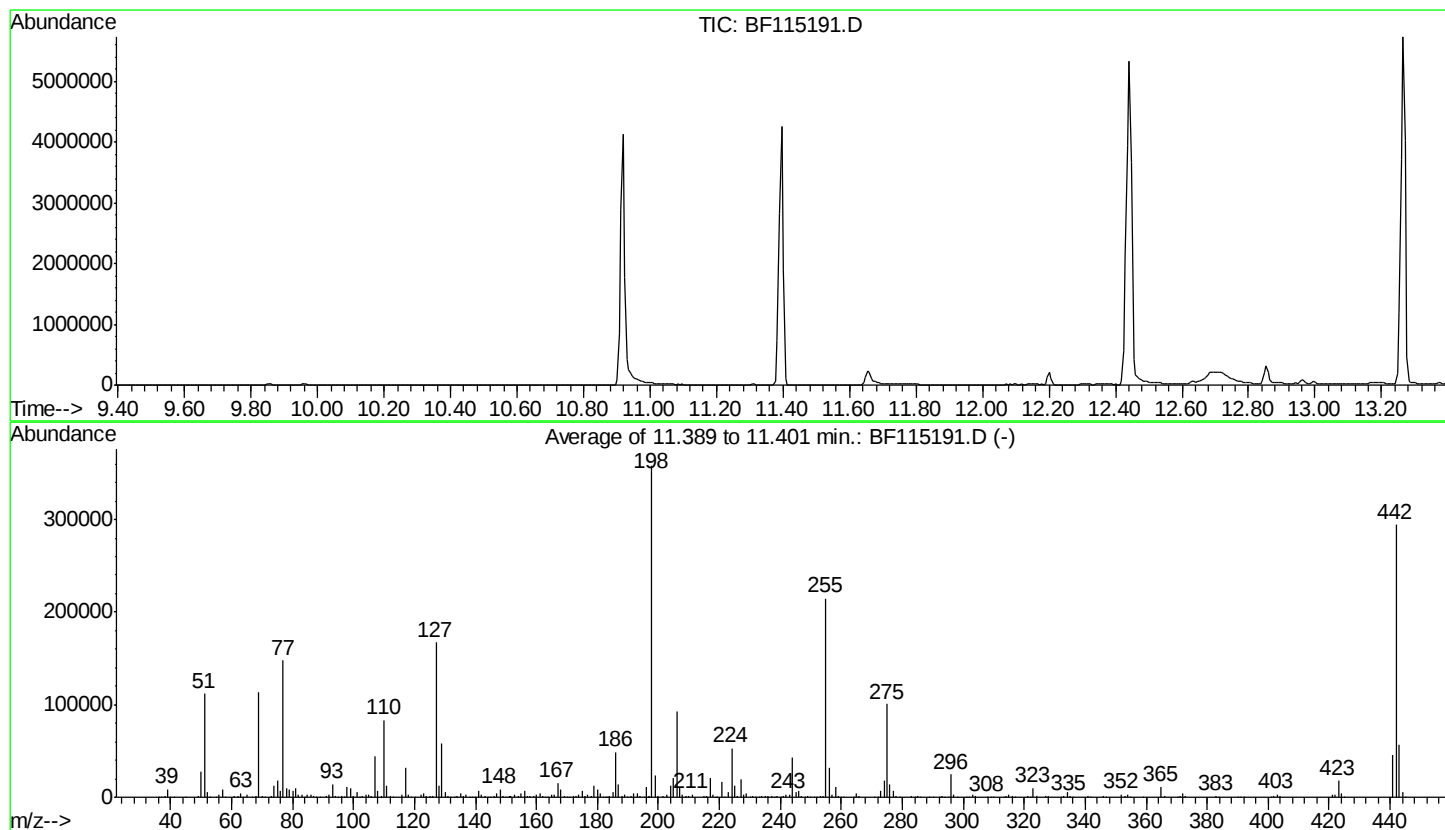

AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	111829	PASS
68	69	0.00	2	1.8	1988	PASS
69	198	0.00	100	31.5	112744	PASS
70	69	0.00	2	0.7	744	PASS
127	198	10	80	46.6	167010	PASS
197	198	0.00	2	0.5	1793	PASS
198	198	100	100	100.0	358144	PASS
199	198	5	9	6.7	23978	PASS
275	198	10	60	28.2	100821	PASS
365	198	1	100	3.2	11456	PASS
441	198	0.01	100	12.9	46280	PASS
442	198	50	100	82.1	293952	PASS
443	442	15	24	19.3	56698	PASS