

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062618\
 Data File : BF106843.D
 Acq On : 27 Jun 2018 1:10
 Operator : JU/SJ
 Sample : J3639-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062018-DBRI-E-D-M

Quant Time: Jun 27 04:39:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 25 18:50:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	40491	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	142867	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	62942	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	122727	20.00	ng	0.00
75) Chrysene-d12	14.14	240	123364	20.00	ng	-0.02
86) Perylene-d12	15.68	264	83471	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	94074	39.34	ng	0.00
7) Phenol-d6	6.60	99	80327	26.90	ng	-0.02
23) Nitrobenzene-d5	7.52	82	210032	81.70	ng	-0.01
41) 2,4,6-Tribromophenol	10.80	330	53918	73.91	ng	0.00
44) 2-Fluorobiphenyl	9.31	172	397132	111.37	ng	-0.01
78) Terphenyl-d14	13.08	244	480846	94.42	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.52	70	26879	13.655	ng	# 72
25) Isophorone	7.52	82	210030	46.363	ng	# 64
49) Dimethylphthalate	9.71	163	13671	2.896	ng	# 98
50) 2,6-Dinitrotoluene	10.00	165	7744	7.747	ng	# 24
56) 2,4-Dinitrotoluene	10.00	165	7744	5.935	ng	# 21
66) 4-Bromophenyl-phenylether	10.80	248	3288	2.245	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062618\
Data File : BF106843.D
Acq On : 27 Jun 2018 1:10
Operator : JU/SJ
Sample : J3639-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062018-DBRI-E-D-M

Quant Time: Jun 27 04:39:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 25 18:50:17 2018
Response via : Initial Calibration

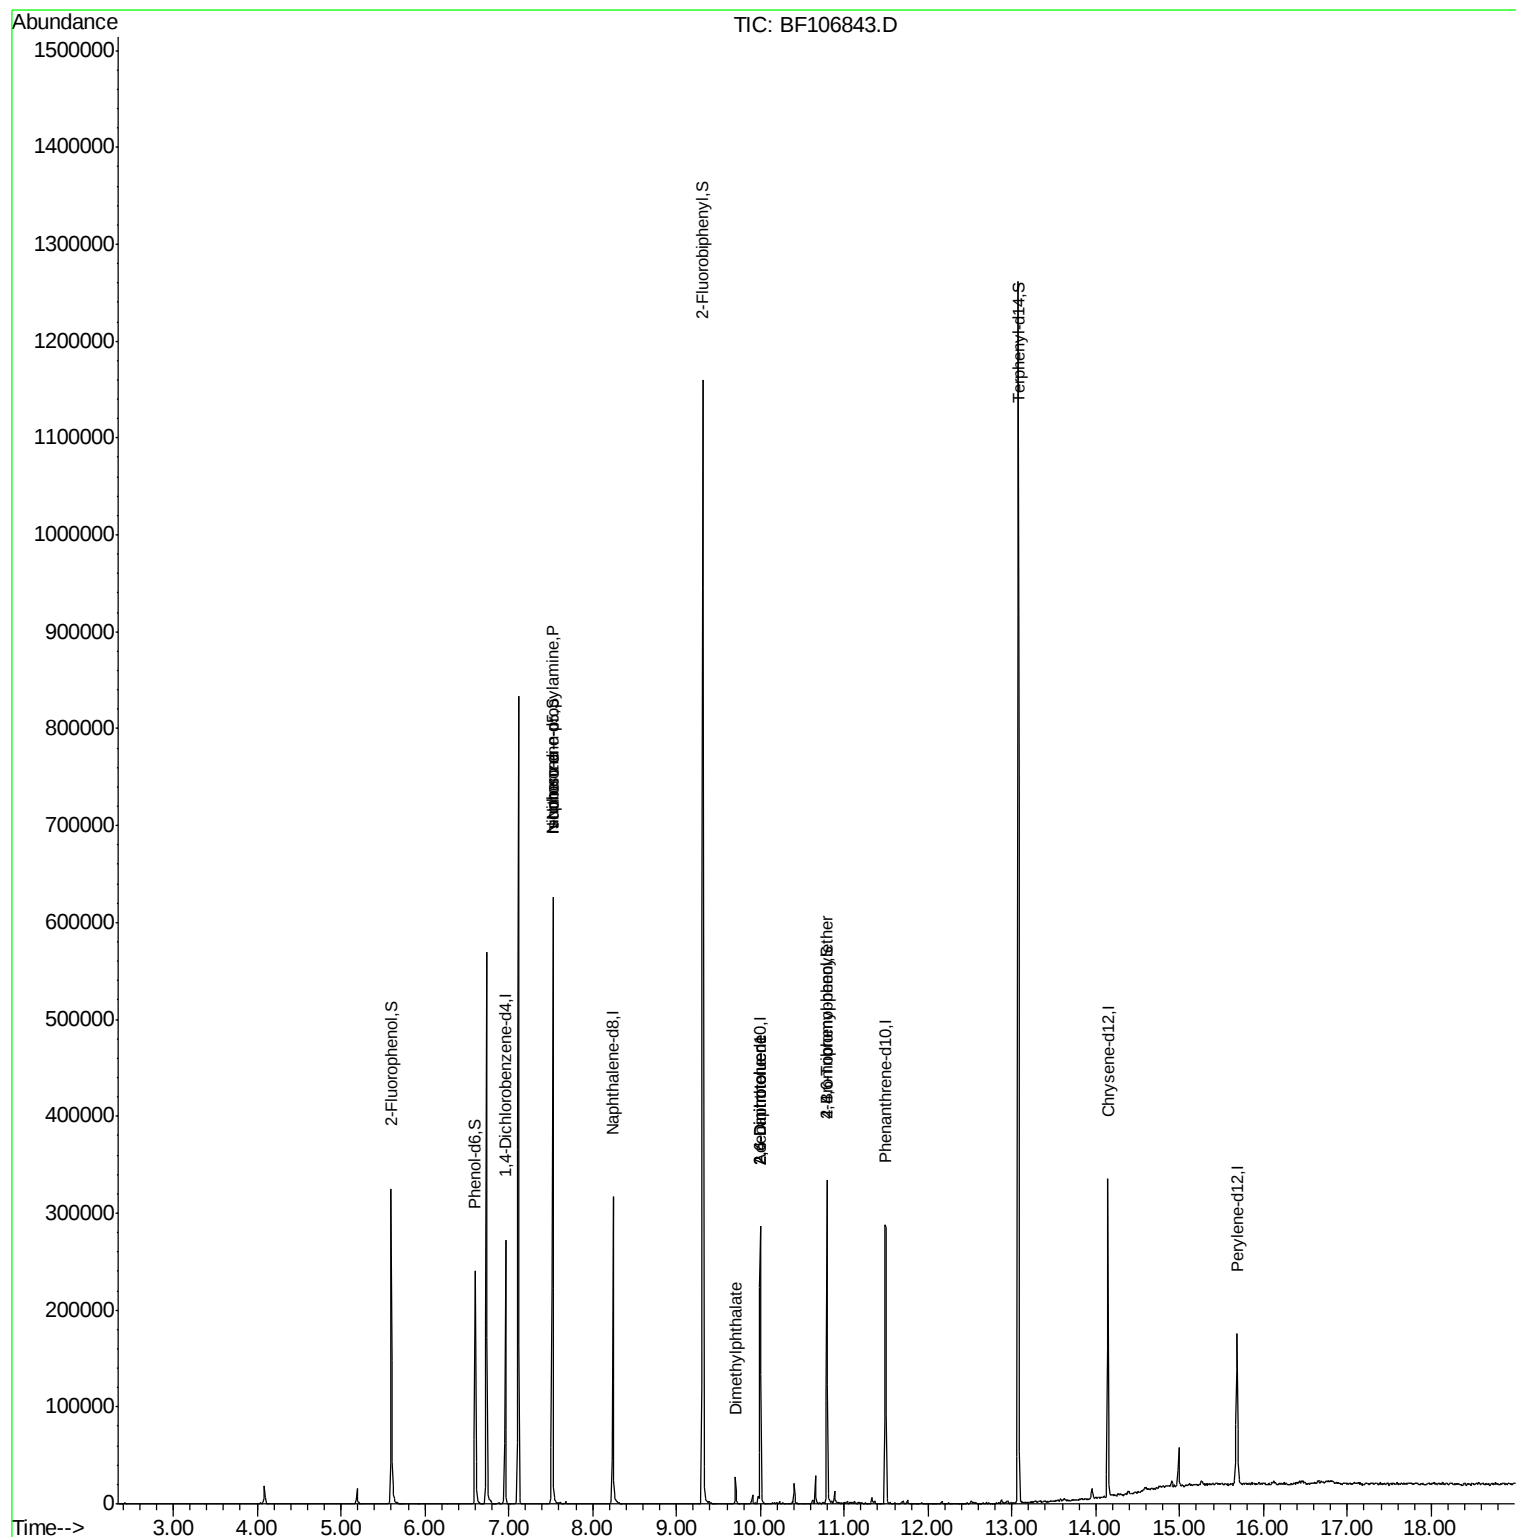




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.96 min Scan# 786
Delta R.T. -0.00 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Instrument :
BNA_F
ClientSampleId :
062018-DBRI-E-D-M

Tgt Ion:152 Resp: 40491
Ion Ratio Lower Upper
152 100
150 159.8 124.6 186.8
115 57.7 50.1 75.1

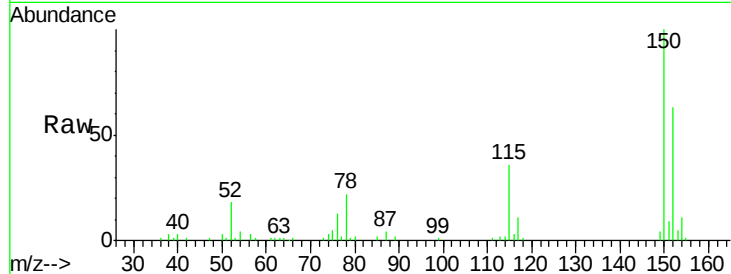


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

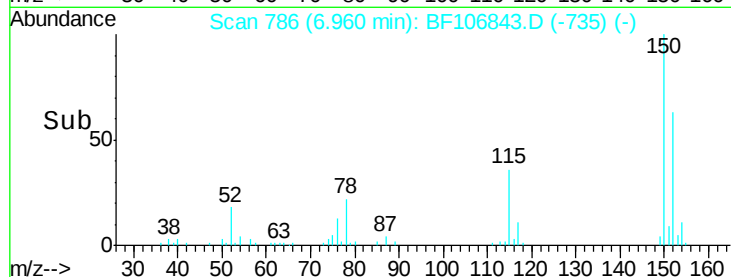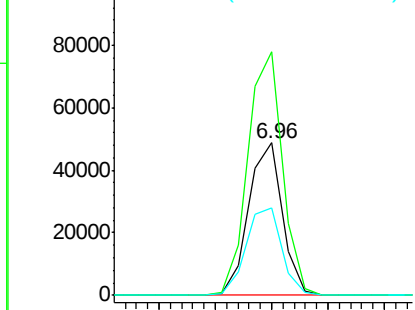



#5

2-Fluorophenol
Concen: 39.341 ng
RT: 5.60 min Scan# 555
Delta R.T. -0.00 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Tgt Ion:112 Resp: 94074
Ion Ratio Lower Upper
112 100
64 56.0 47.9 71.9
63 26.8 23.7 35.5

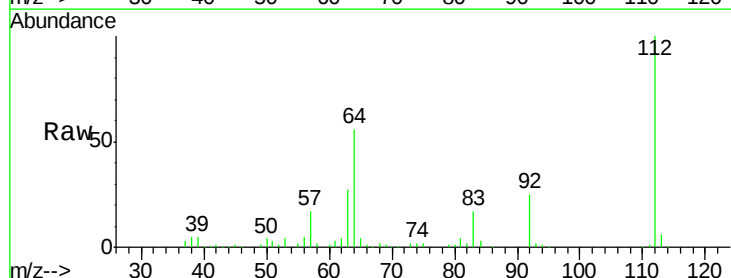

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

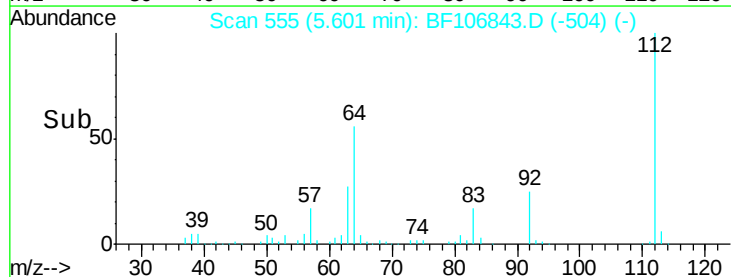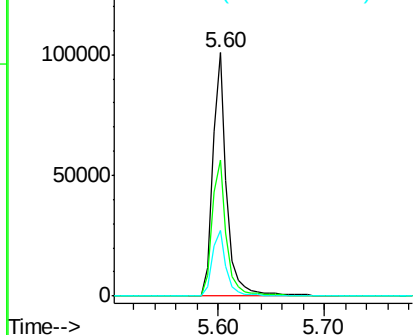



#7

Phenol-d6

Concen: 26.900 ng

RT: 6.60 min Scan# 724

Delta R.T. -0.02 min

Lab File: BF106843.D

Acq: 27 Jun 2018 1:10

Instrument :

BNA_F

ClientSampleId :

062018-DBRI-E-D-M


Tgt Ion: 99 Resp: 80327

Ion Ratio Lower Upper

99 100

42 18.2 14.5 21.7



71 34.5 25.4 38.0

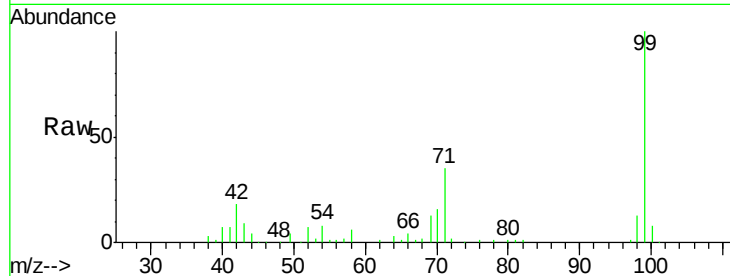

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

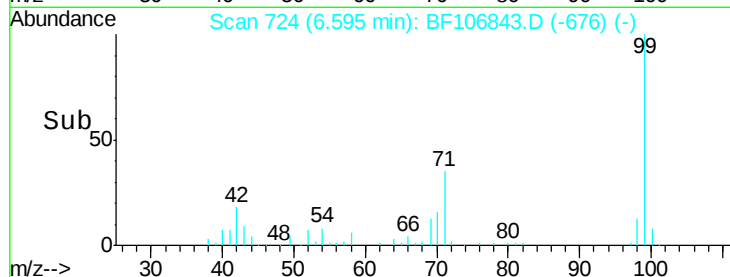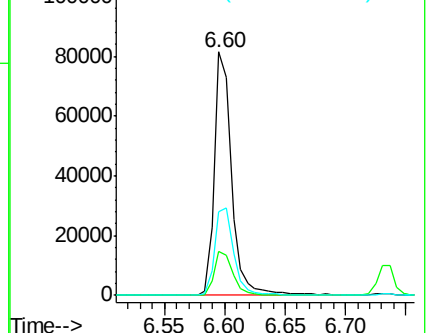

#19

n-Nitroso-di-n-propylamine

Concen: 13.655 ng

RT: 7.52 min Scan# 882

Delta R.T. 0.14 min

Lab File: BF106843.D

Acq: 27 Jun 2018 1:10

Tgt Ion: 70 Resp: 26879


Ion Ratio Lower Upper

70 100

42 41.4 47.5 71.3#

101 0.0 7.4 11.2#

130 2.2 16.6 25.0#


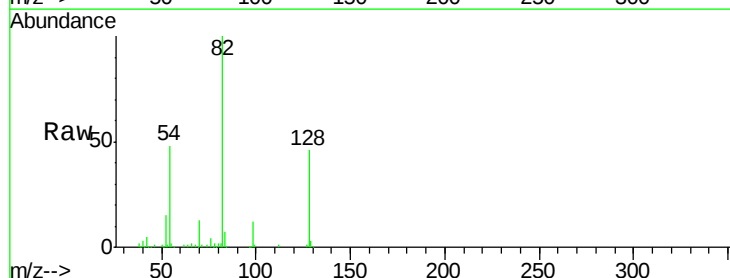


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1



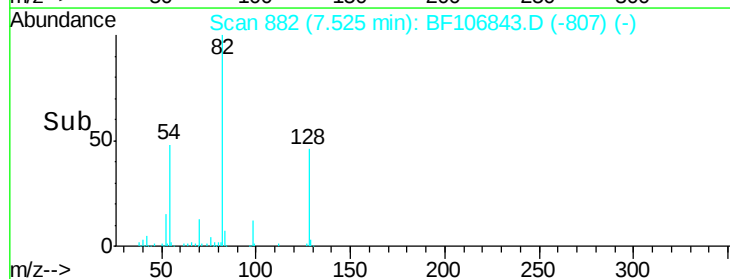
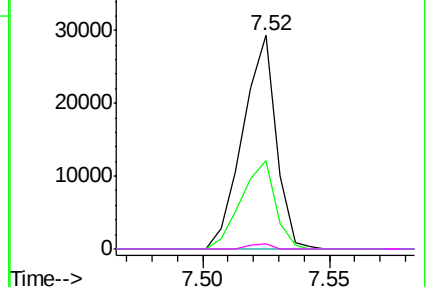




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.24 min Scan# 1004
Delta R.T. -0.01 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10




Instrument :
BNA_F
ClientSampleId :
062018-DBRI-E-D-M

Tgt Ion:	136	Resp:	142867
Ion	Ratio	Lower	Upper
136	100		
137	10.2	8.9	13.3
54	7.3	6.6	9.8
68	5.6	5.0	7.4

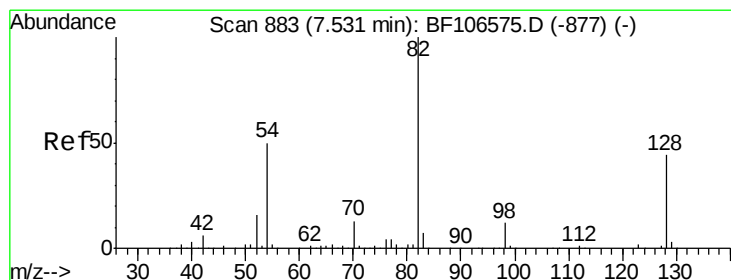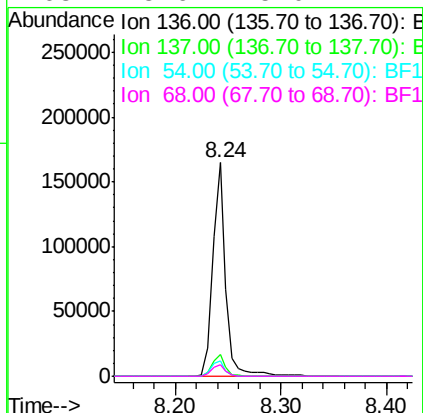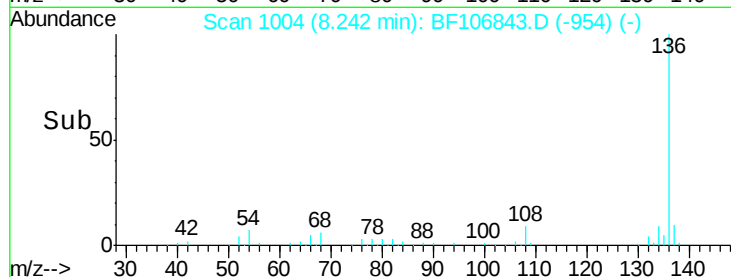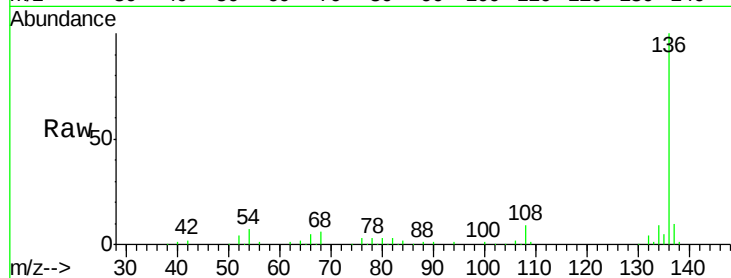

#23
Nitrobenzene-d5
Concen: 81.700 ng
RT: 7.52 min Scan# 882
Delta R.T. -0.01 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Tgt Ion:	82	Resp:	210032
Ion	Ratio	Lower	Upper
82	100		
128	46.5	36.1	54.1
54	47.9	41.4	62.2

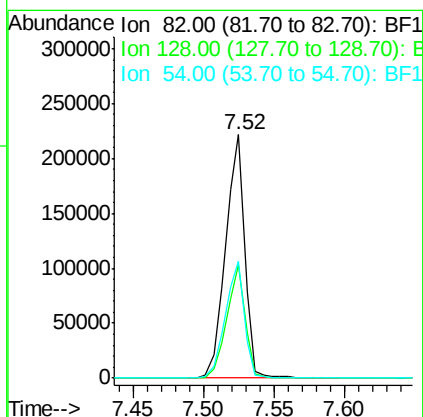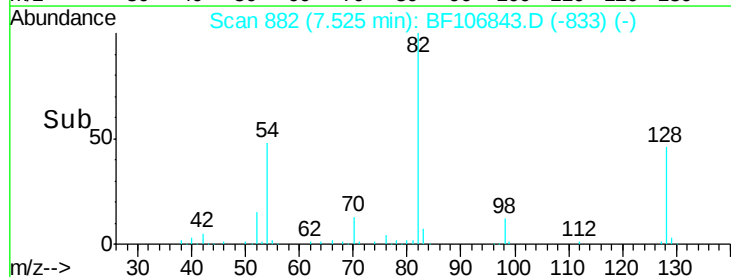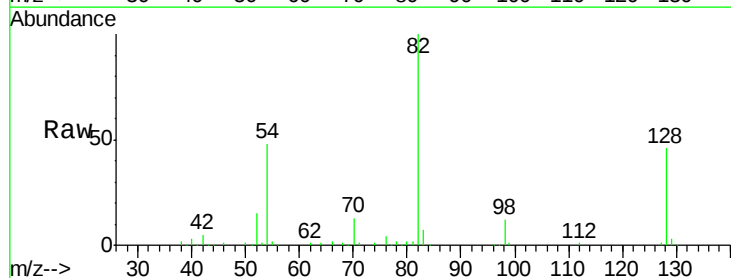



#25

Isophorone

Concen: 46.363 ng

RT: 7.52 min Scan# 882

Delta R.T. -0.26 min

Lab File: BF106843.D

Acq: 27 Jun 2018 1:10

Instrument :

BNA_F

ClientSampleId :

062018-DBRI-E-D-M


Tgt Ion: 82 Resp: 210030

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

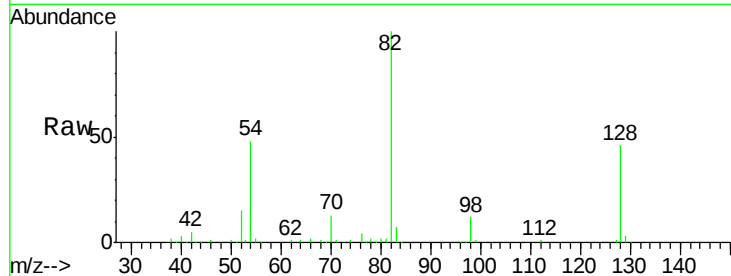

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

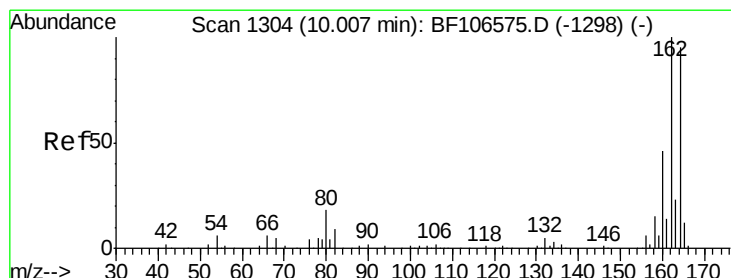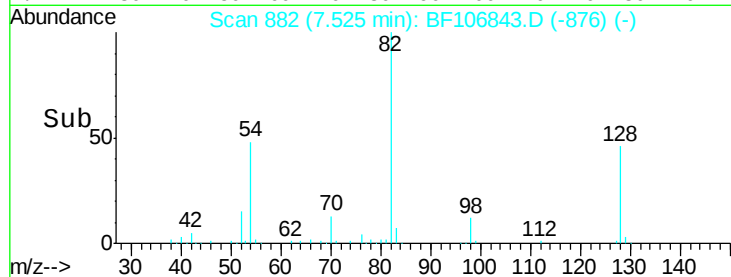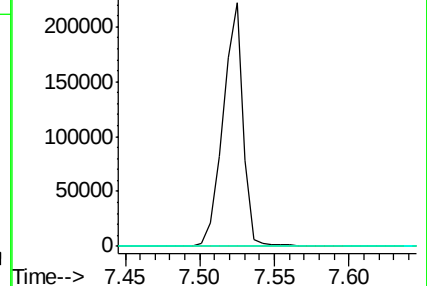

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.00 min Scan# 1303

Delta R.T. -0.01 min

Lab File: BF106843.D

Acq: 27 Jun 2018 1:10


Tgt Ion: 164 Resp: 62942

Ion Ratio Lower Upper

164 100

162 97.8 86.1 129.1



160 45.8 38.3 57.5

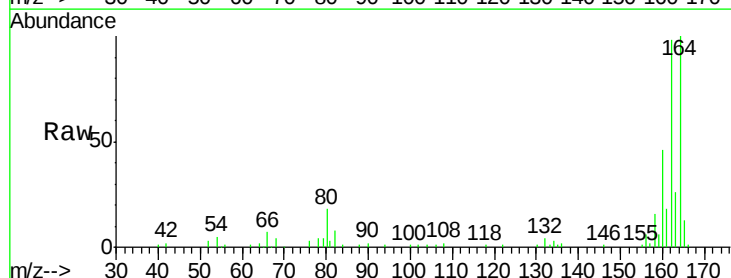

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



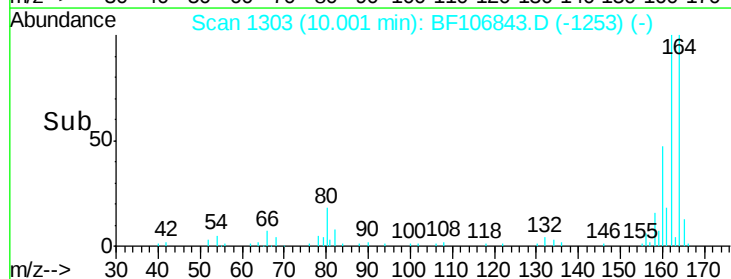
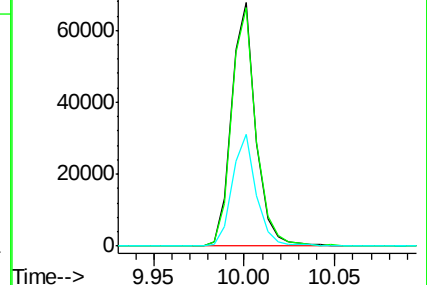




#41
 2,4,6-Tribromophenol
 Concen: 73.909 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF106843.D
 Acq: 27 Jun 2018 1:10




Instrument :
 BNA_F
 ClientSampleId :
 062018-DBRI-E-D-M

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.2	77.0	115.6
141	22.9	29.9	44.9#

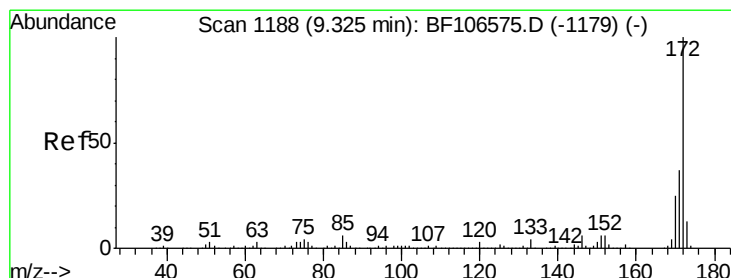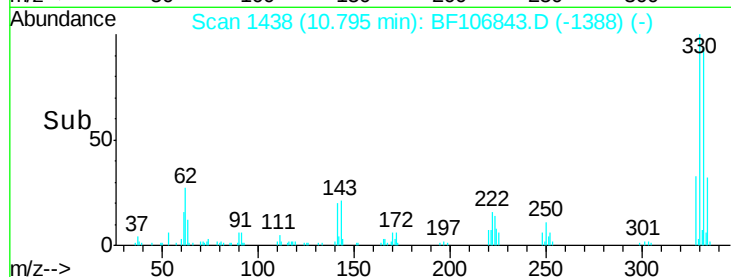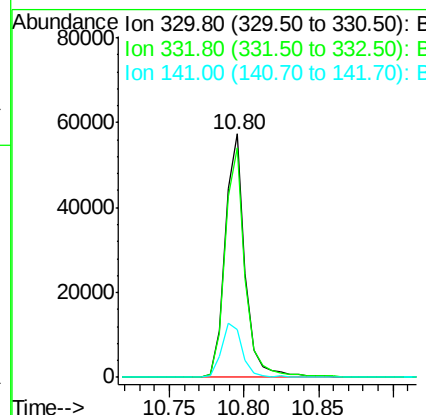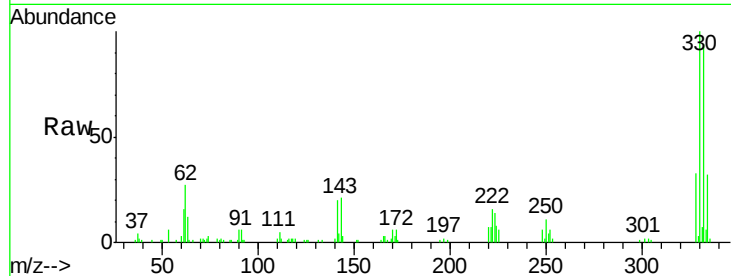

#44
 2-Fluorobiphenyl
 Concen: 111.373 ng
 RT: 9.31 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF106843.D
 Acq: 27 Jun 2018 1:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	29.7	44.5
170	24.1	19.6	29.4

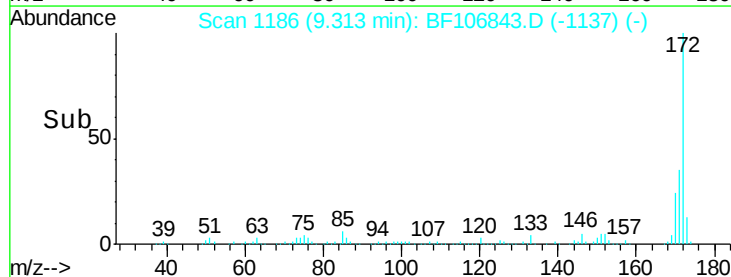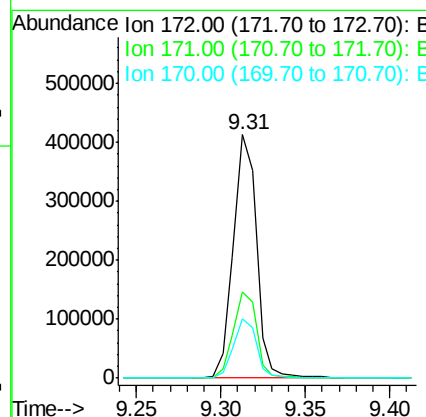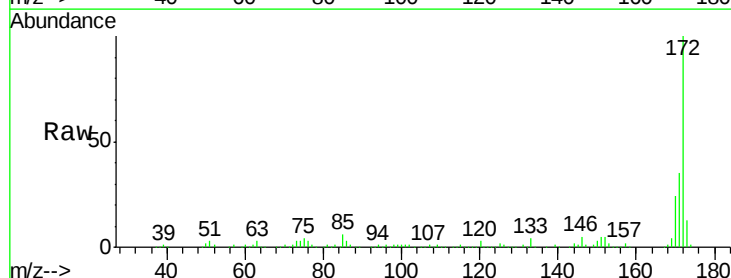







#49
Dimethylphthalate
Concen: 2.896 ng
RT: 9.71 min Scan# 1253
Delta R.T. -0.02 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Instrument :
BNA_F
ClientSampleId :
062018-DBRI-E-D-M

Tgt Ion:163 Resp: 13671
Ion Ratio Lower Upper
163 100
194 4.0 2.7 4.1
164 10.8 8.2 12.2

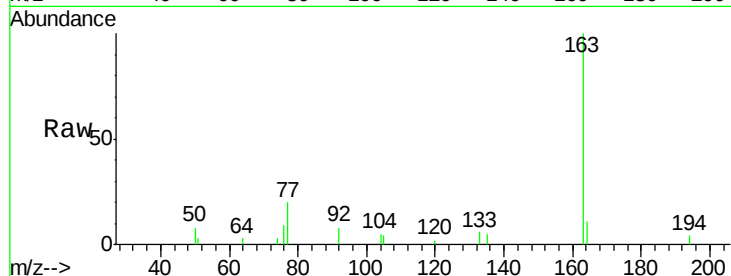


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

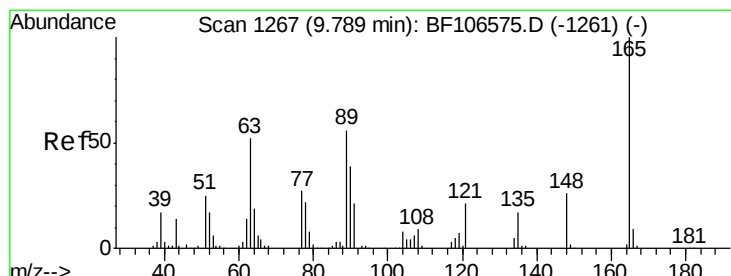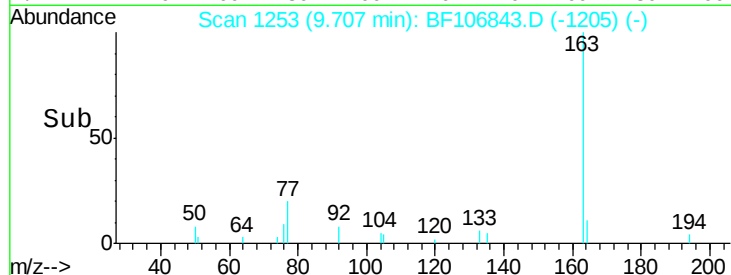
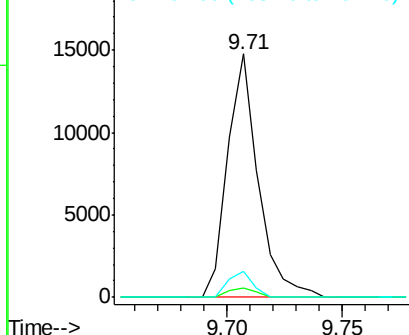


#50
2,6-Dinitrotoluene
Concen: 7.747 ng
RT: 10.00 min Scan# 1303
Delta R.T. 0.21 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Tgt Ion:165 Resp: 7744
Ion Ratio Lower Upper
165 100
63 0.0 44.7 67.1#
89 0.0 44.0 66.0#

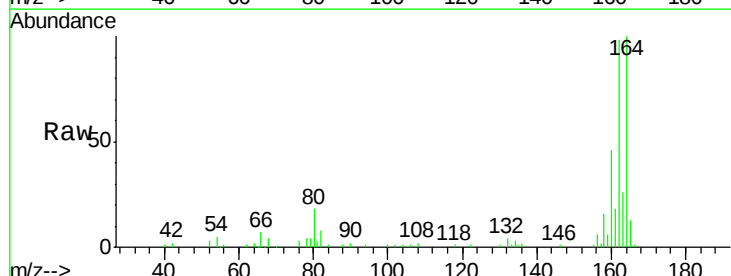

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1


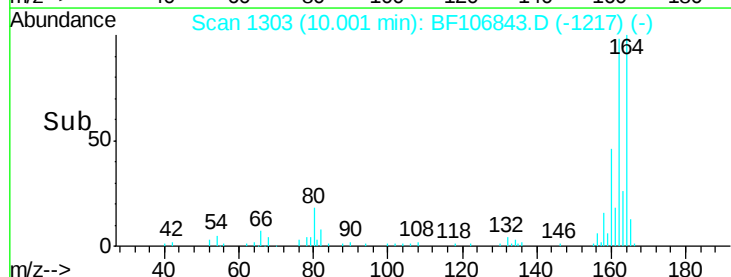
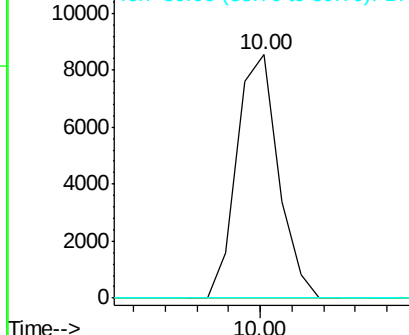




#56
2,4-Dinitrotoluene
Concen: 5.935 ng
RT: 10.00 min Scan# 1303
Delta R.T. -0.20 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10




Instrument :
BNA_F
ClientSampleId :
062018-DBRI-E-D-M

Tgt Ion:	165	Resp:	7744
Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#

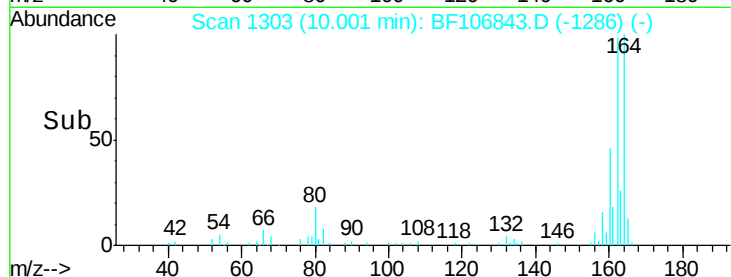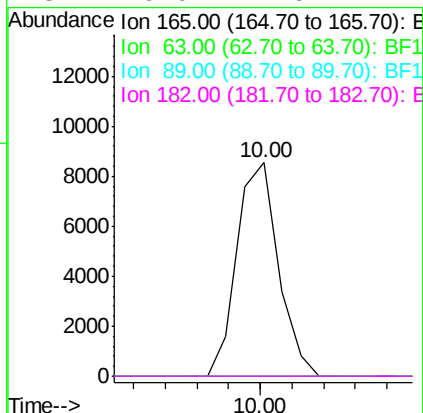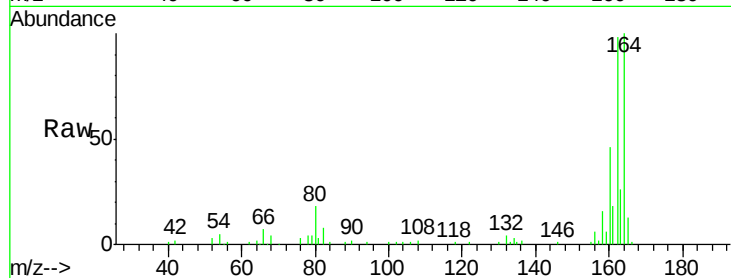

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1557
Delta R.T. -0.01 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Tgt Ion:	188	Resp:	122727
Ion	Ratio	Lower	Upper
188	100		
94	7.9	8.5	12.7#
80	7.8	9.2	13.8#

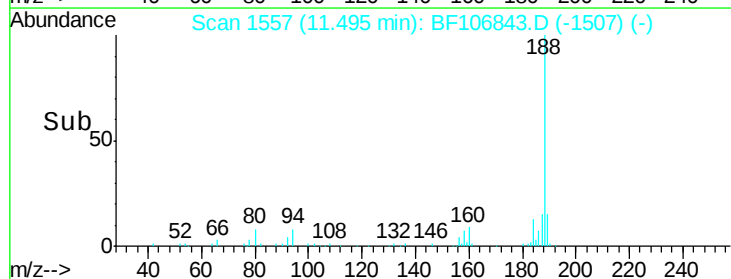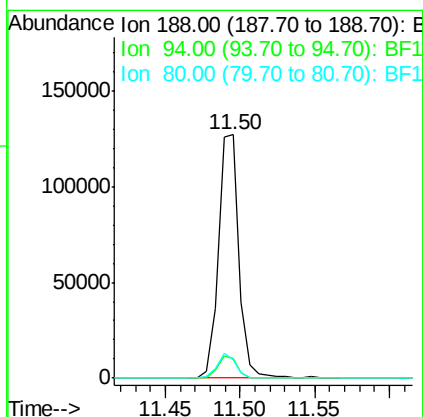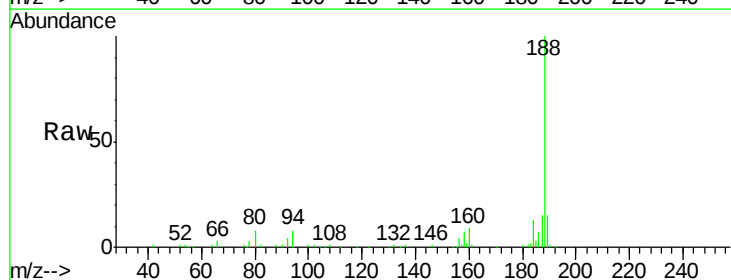







#66
4-Bromophenyl-phenylether
Concen: 2.245 ng
RT: 10.80 min Scan# 1438
Delta R.T. -0.24 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Instrument :
BNA_F
ClientSampleId :
062018-DBRI-E-D-M

Tgt Ion:248 Resp: 3288
Ion Ratio Lower Upper
248 100
250 190.5 76.9 115.3#
141 325.7 74.4 111.6#

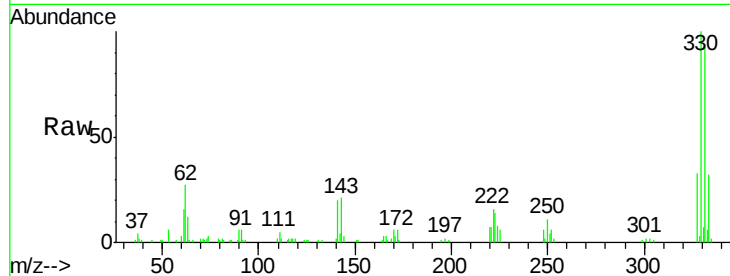


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

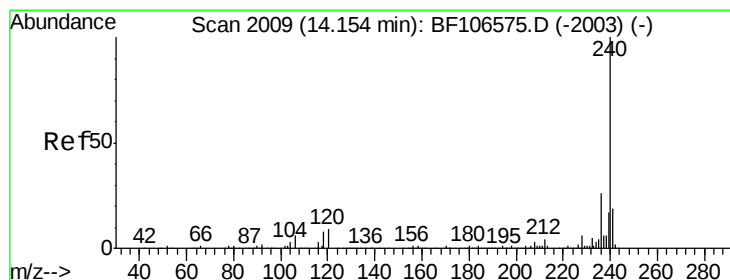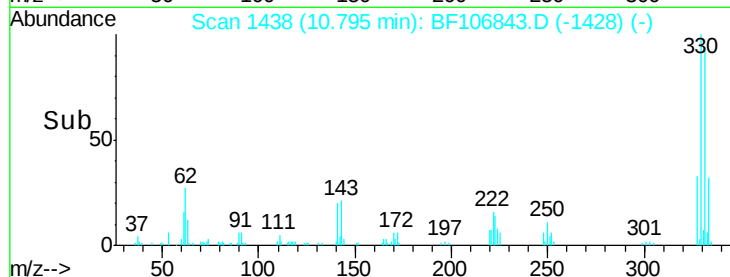
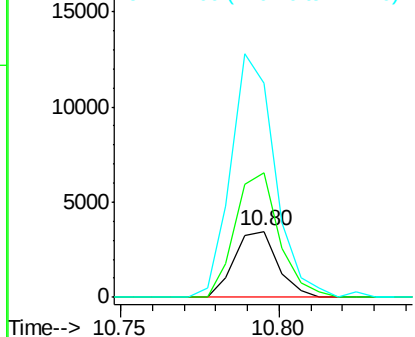


#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.14 min Scan# 2007
Delta R.T. -0.02 min
Lab File: BF106843.D
Acq: 27 Jun 2018 1:10

Tgt Ion:240 Resp: 123364
Ion Ratio Lower Upper
240 100
120 9.3 9.5 14.3#
236 25.1 20.7 31.1

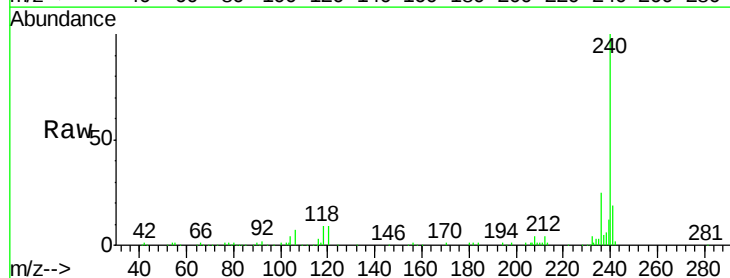

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



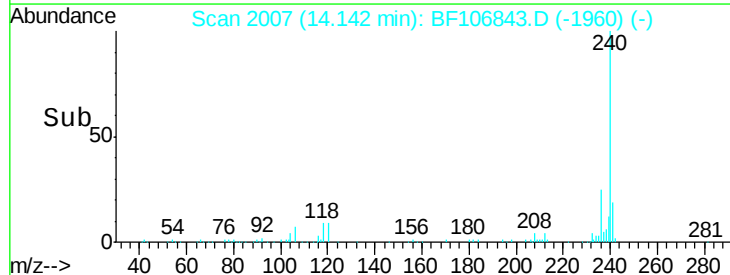
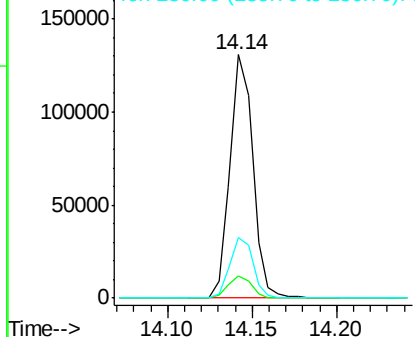




#78
 Terphenyl-d14
 Concen: 94.416 ng
 RT: 13.08 min Scan# 1826
 Delta R.T. -0.01 min
 Lab File: BF106843.D
 Acq: 27 Jun 2018 1:10

Instrument :
 BNA_F
 ClientSampleId :
 062018-DBRI-E-D-M

Tgt Ion: 244 Resp: 480846
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.4 8.0
 122 8.9 11.0 16.4#

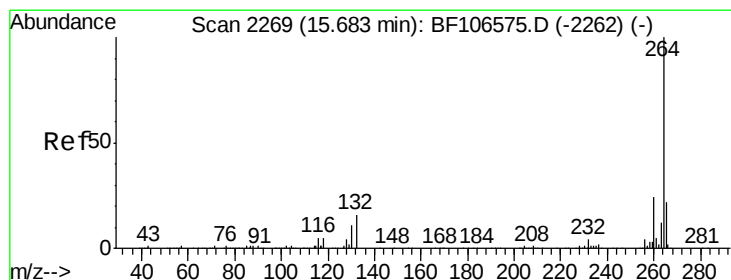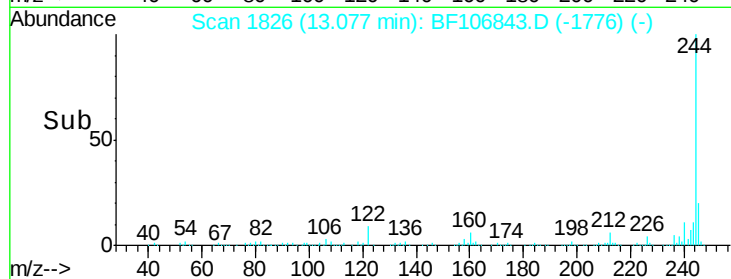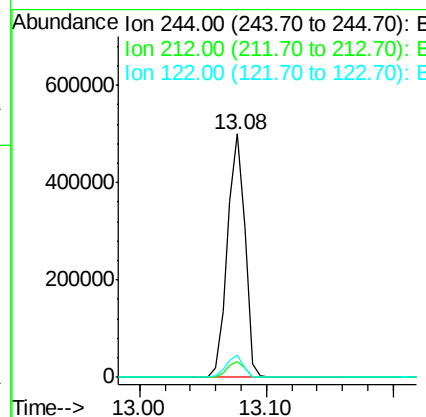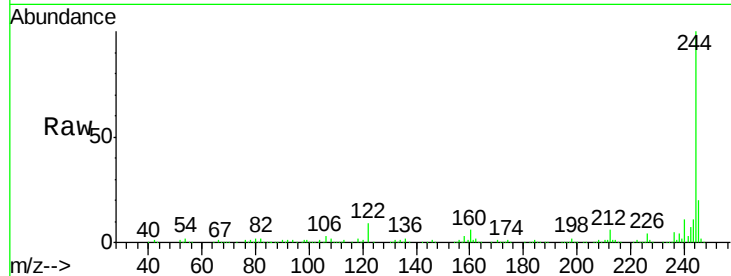

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.68 min Scan# 2269
 Delta R.T. -0.04 min
 Lab File: BF106843.D
 Acq: 27 Jun 2018 1:10

Tgt Ion: 264 Resp: 83471
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.2 28.8
 265 22.2 17.5 26.3

