

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062618\
 Data File : BF106850.D
 Acq On : 27 Jun 2018 4:14
 Operator : JU/SJ
 Sample : PB110514BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB110514BL

Quant Time: Jun 27 05:09:17 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 25 18:50:17 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.96	152	42158	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	151199	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	67732	20.00	ng	0.00
63) Phenanthrene-d10	11.49	188	128807	20.00	ng	-0.01
75) Chrysene-d12	14.14	240	125384	20.00	ng	-0.02
86) Perylene-d12	15.68	264	85264	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	205775	82.65	ng	0.00
7) Phenol-d6	6.60	99	256043	82.35	ng	-0.01
23) Nitrobenzene-d5	7.52	82	229601	84.39	ng	-0.01
41) 2,4,6-Tribromophenol	10.80	330	57581	73.35	ng	0.00
44) 2-Fluorobiphenyl	9.31	172	443278	116.19	ng	-0.01
78) Terphenyl-d14	13.08	244	494770	95.58	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062618\
Data File : BF106850.D
Acq On : 27 Jun 2018 4:14
Operator : JU/SJ
Sample : PB110514BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB110514BL

Quant Time: Jun 27 05:09:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 25 18:50:17 2018
Response via : Initial Calibration

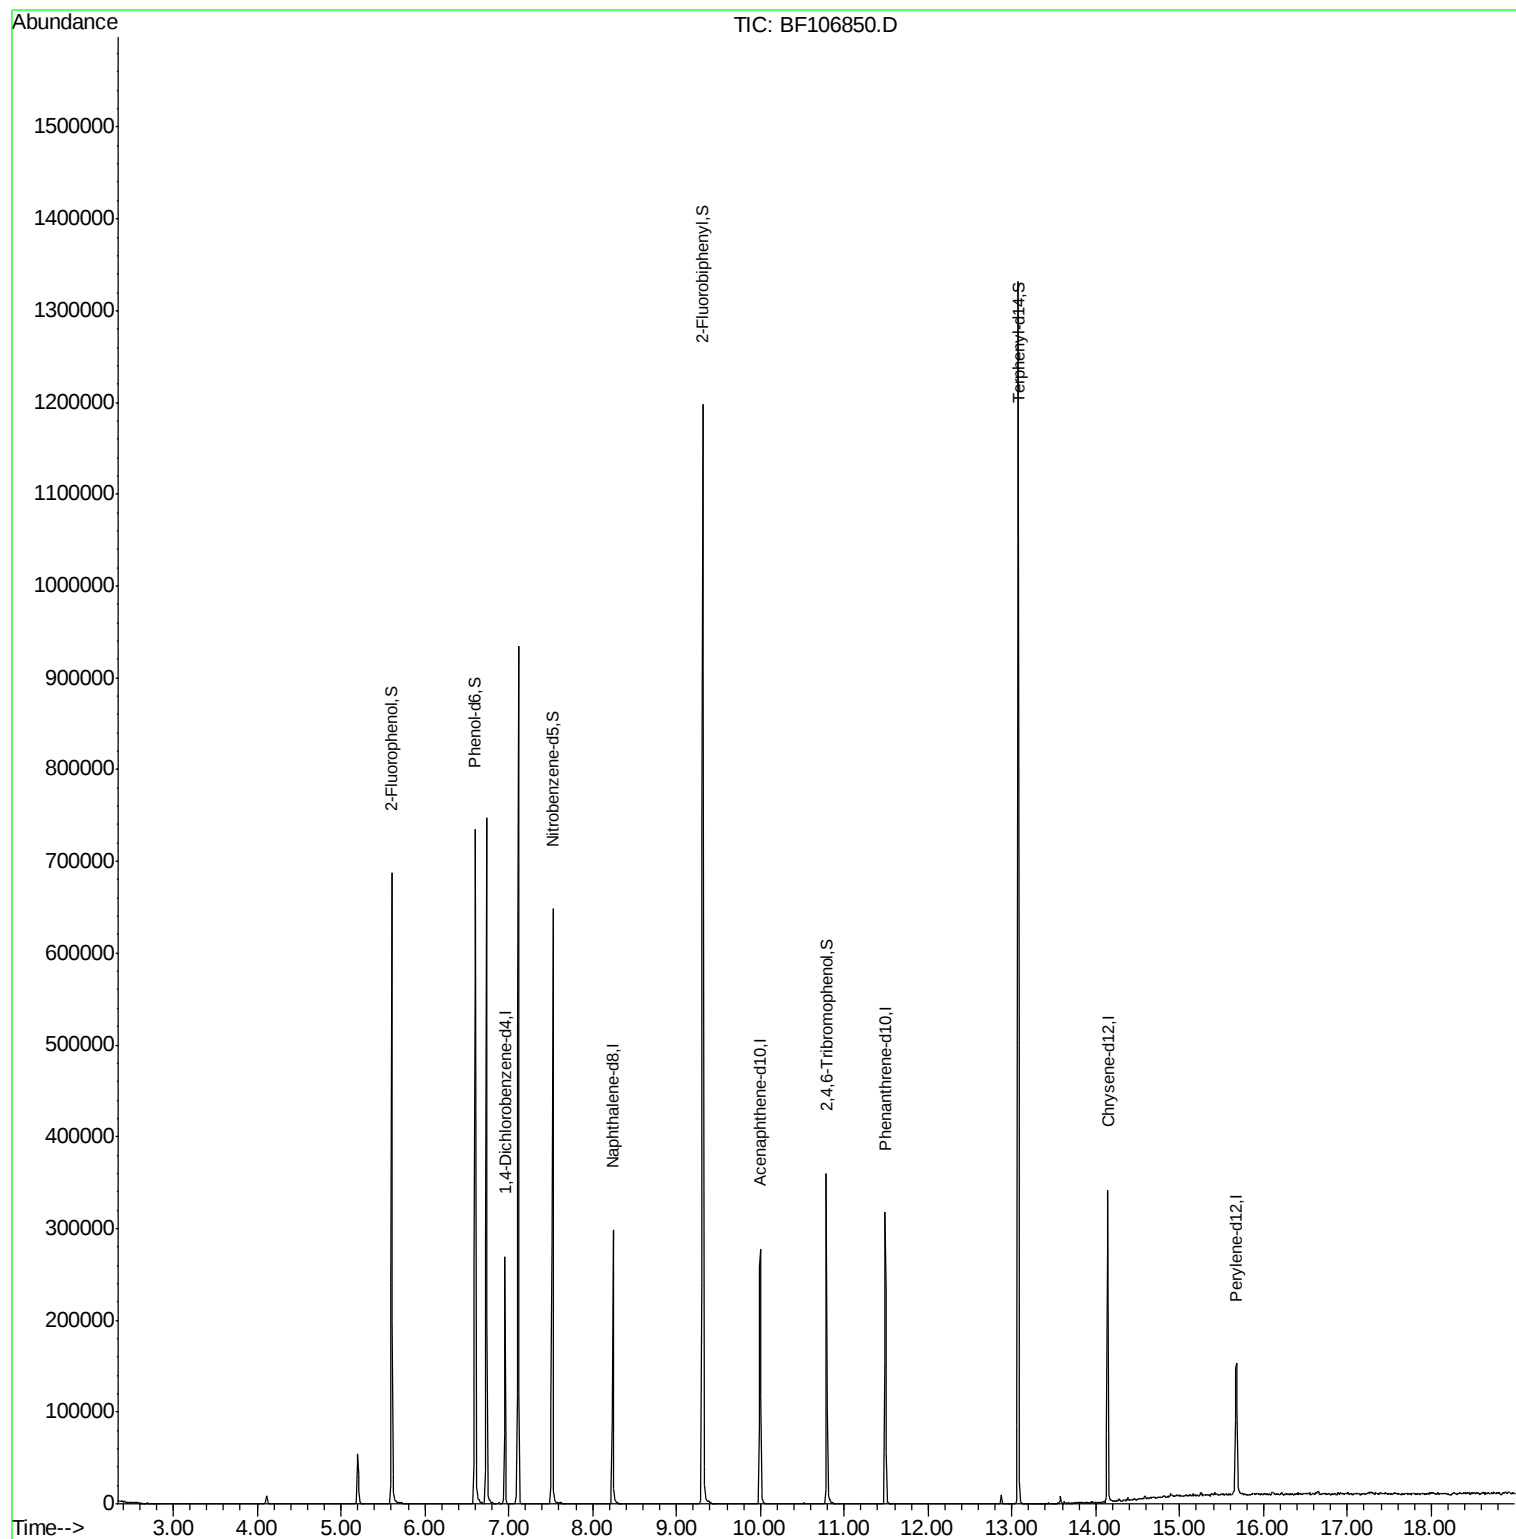




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.96 min Scan# 786
Delta R.T. 0.00 min
Lab File: BF106850.D
Acq: 27 Jun 2018 4:14

Instrument :
BNA_F
ClientSampleId :
PB110514BL

Tot Ion:152 Resp: 42158
Ion Ratio Lower Upper
152 100
150 161.3 124.6 186.8
115 57.4 50.1 75.1

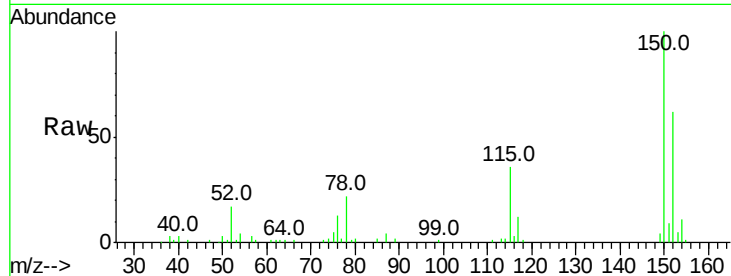


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

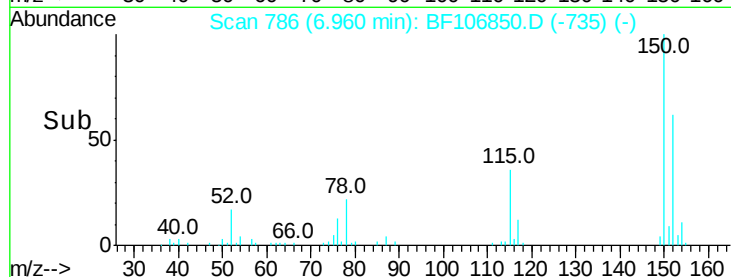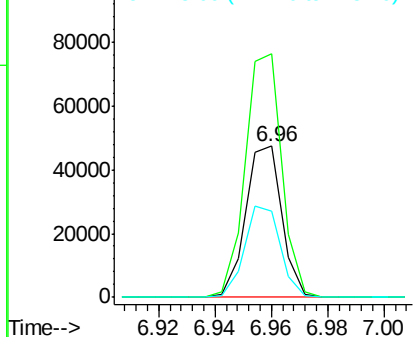



#5

2-Fluorophenol
Concen: 82.652 ng
RT: 5.61 min Scan# 556
Delta R.T. 0.01 min
Lab File: BF106850.D
Acq: 27 Jun 2018 4:14

Tgt Ion:112 Resp: 205775
Ion Ratio Lower Upper
112 100
64 56.1 47.9 71.9
63 27.2 23.7 35.5

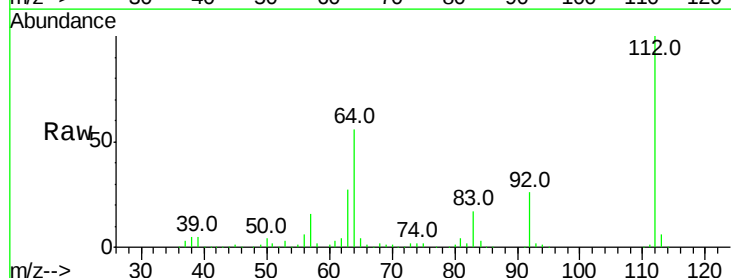

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

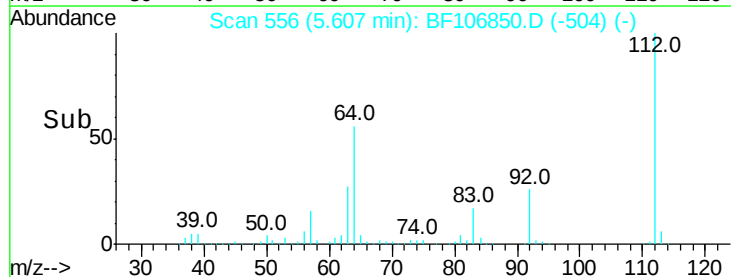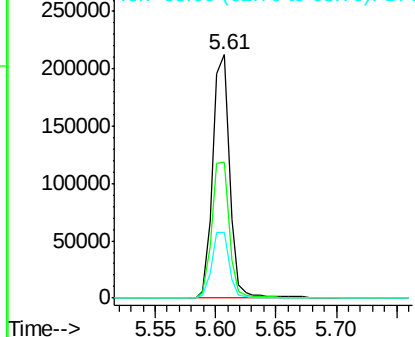



#7

Phenol-d6

Concen: 82.352 ng

RT: 6.60 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF106850.D

Acq: 27 Jun 2018 4:14

Instrument :

BNA_F

ClientSampleId :

PB110514BL


Tot Ion: 99 Resp: 256043

Ion Ratio Lower Upper




99 100

42 16.2 14.5 21.7

71 33.8 25.4 38.0

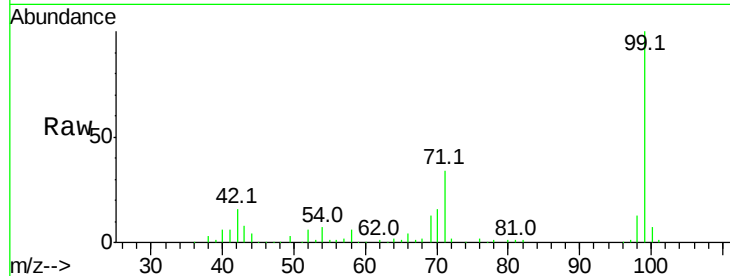

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

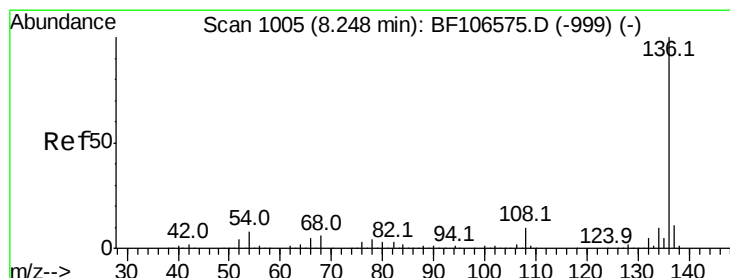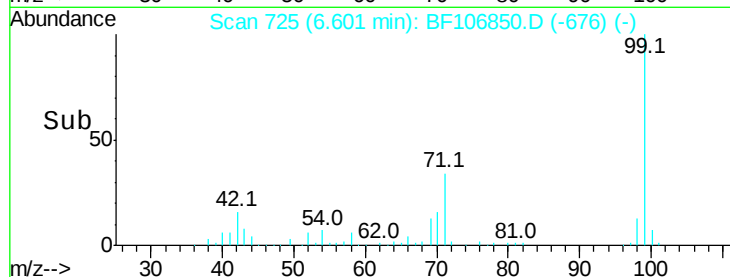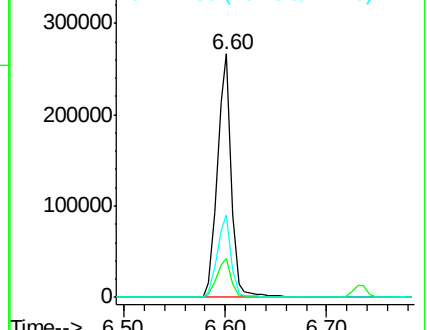

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1004

Delta R.T. -0.01 min

Lab File: BF106850.D

Acq: 27 Jun 2018 4:14

Tgt Ion: 136 Resp: 151199


Ion Ratio Lower Upper

136 100



137 10.6 8.9 13.3

54 7.1 6.6 9.8

68 5.4 5.0 7.4

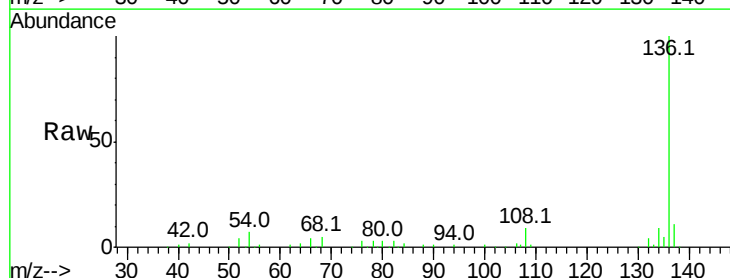

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

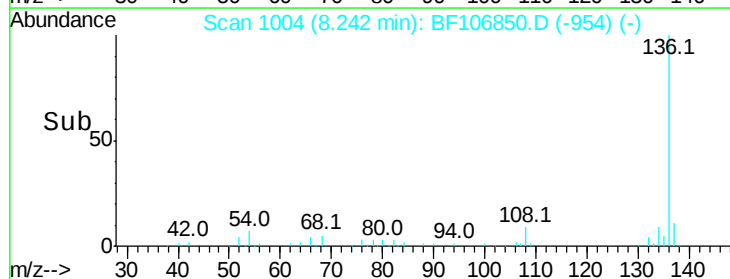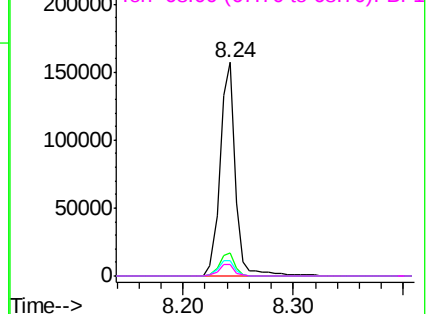






#23
Nitrobenzene-d5
Concen: 84.390 ng
RT: 7.52 min Scan# 882
Delta R.T. -0.01 min
Lab File: BF106850.D
Acq: 27 Jun 2018 4:14

Instrument :
BNA_F
ClientSampleId :
PB110514BL

Tot Ion	82	Resp	229601
Ion Ratio	100	Lower	Upper
128	46.0	36.1	54.1
54	46.8	41.4	62.2

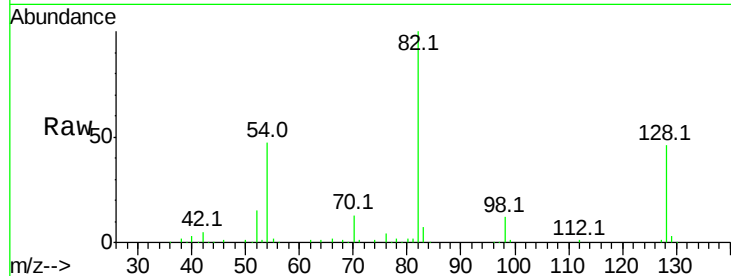


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF1

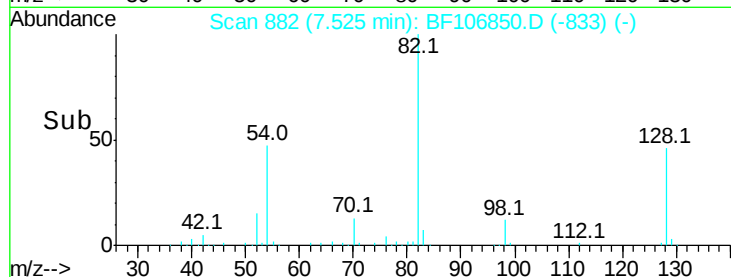
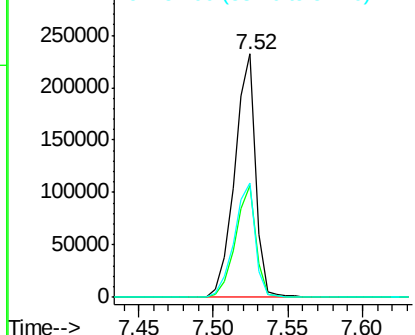



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.00 min Scan# 1303
Delta R.T. -0.01 min
Lab File: BF106850.D
Acq: 27 Jun 2018 4:14

Tgt Ion	164	Resp	67732
Ion Ratio	100	Lower	Upper
162	95.7	86.1	129.1
160	44.1	38.3	57.5

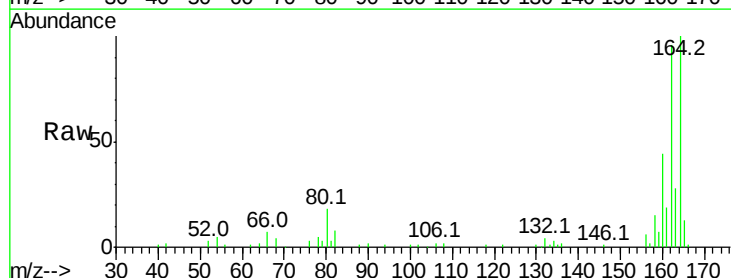

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

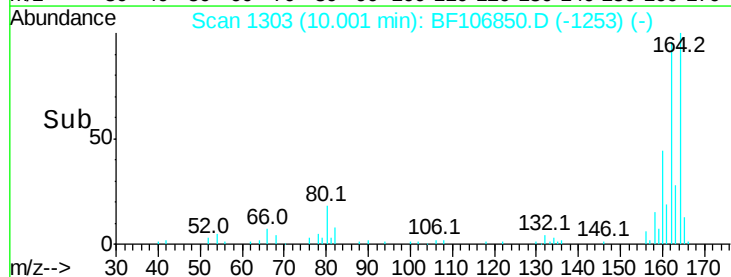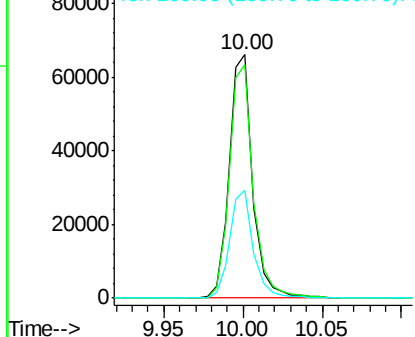


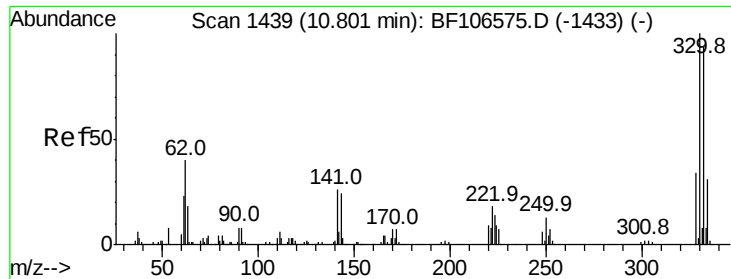



#41
 2,4,6-Tribromophenol
 Concen: 73.349 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF106850.D
 Acq: 27 Jun 2018 4:14

Instrument :
 BNA_F
 ClientSampleId :
 PB110514BL

Tot Ion:330 Resp: 57581
 Ion Ratio Lower Upper
 330 100
 332 95.9 77.0 115.6
 141 23.8 29.9 44.9#

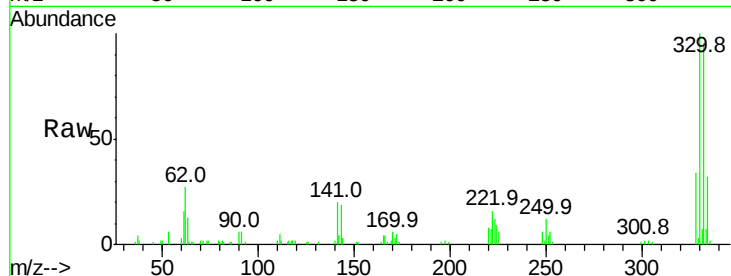


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

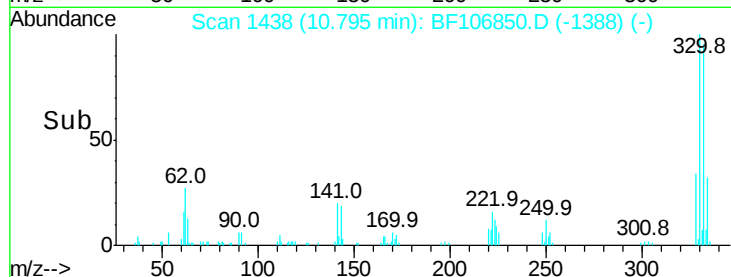
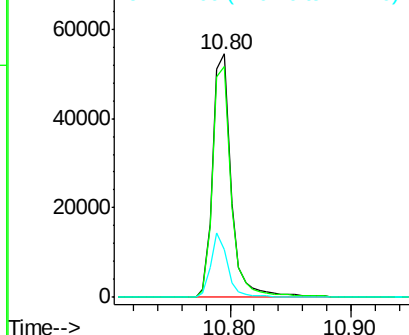


#44
 2-Fluorobiphenyl
 Concen: 116.188 ng
 RT: 9.31 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF106850.D
 Acq: 27 Jun 2018 4:14

Tgt Ion:172 Resp: 443278
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.7 44.5
 170 24.6 19.6 29.4

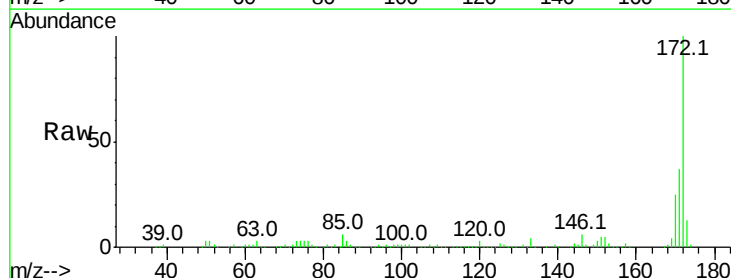

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



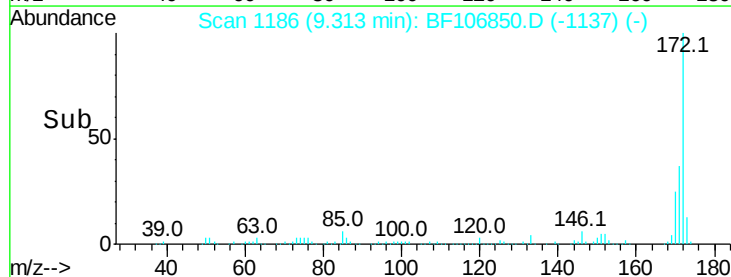
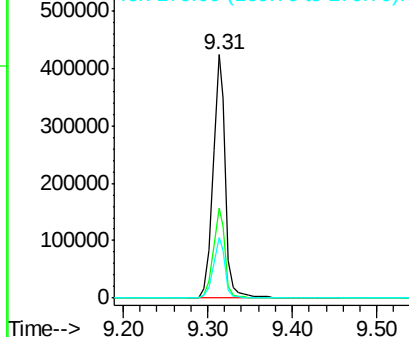




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.49 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF106850.D
Acq: 27 Jun 2018 4:14




Instrument :
BNA_F
ClientSampleId :
PB110514BL


Tot Ion:188 Resp: 128807
Ion Ratio Lower Upper
188 100
94 8.9 8.5 12.7
80 9.7 9.2 13.8

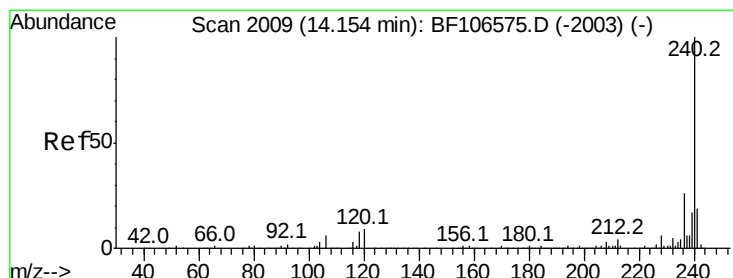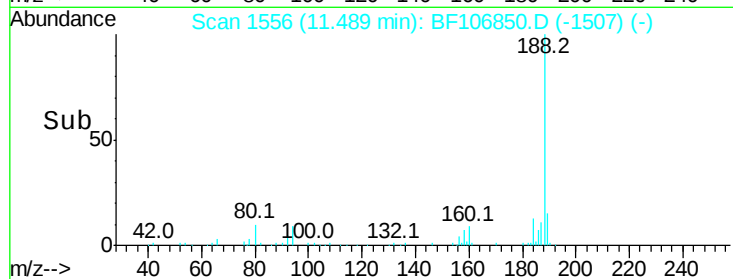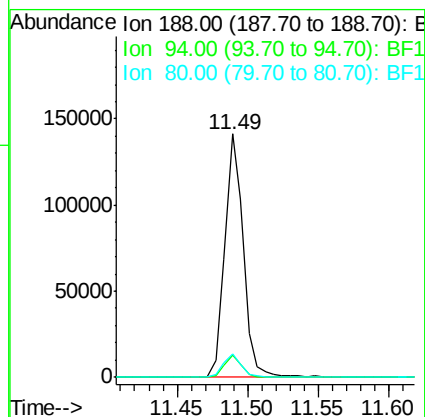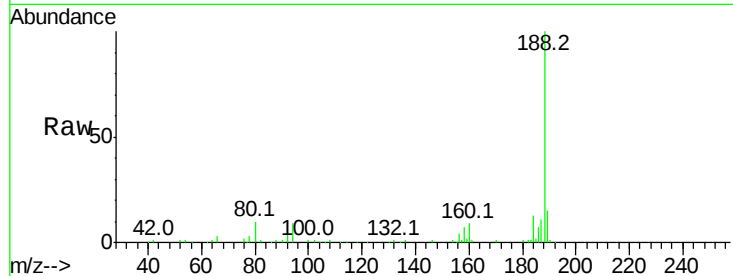

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.14 min Scan# 2007
Delta R.T. -0.02 min
Lab File: BF106850.D
Acq: 27 Jun 2018 4:14

Tgt Ion:240 Resp: 125384
Ion Ratio Lower Upper
240 100
120 8.5 9.5 14.3#
236 26.2 20.7 31.1


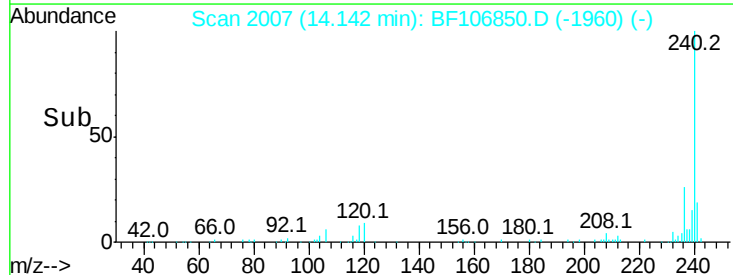
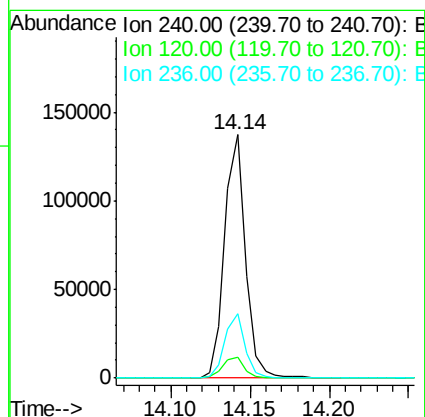
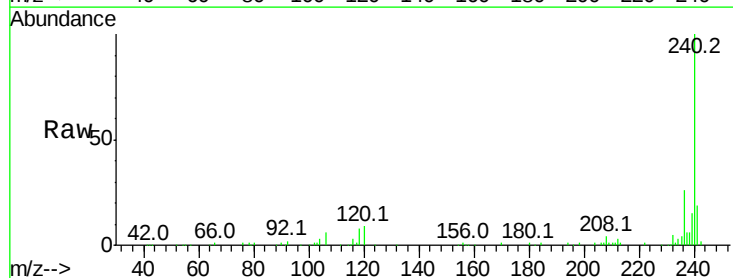


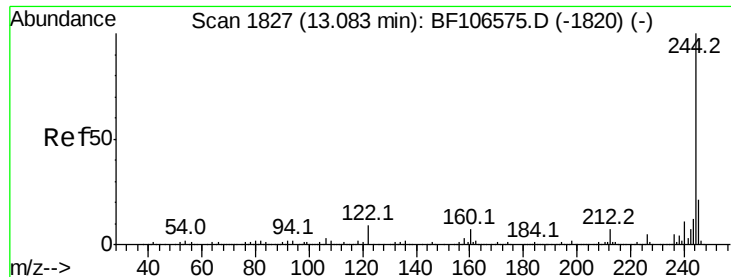

#78
 Terphenyl-d14
 Concen: 95.585 ng
 RT: 13.08 min Scan# 1826
 Delta R.T. -0.01 min
 Lab File: BF106850.D
 Acq: 27 Jun 2018 4:14

Instrument :
 BNA_F
 ClientSampleId :
 PB110514BL

Tot Ion:244 Resp: 494770
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.4 8.0
 122 8.4 11.0 16.4#

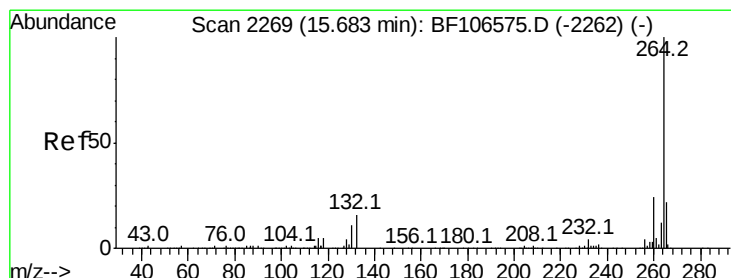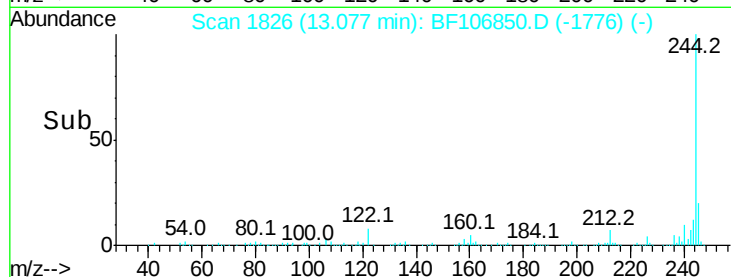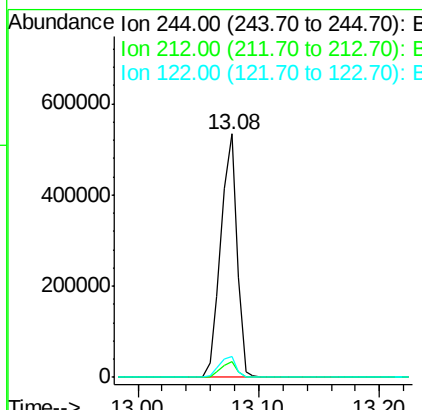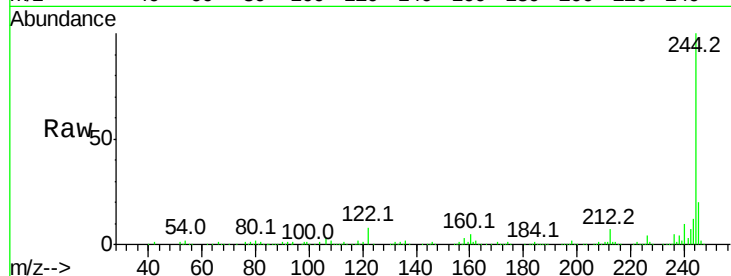

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.68 min Scan# 2268
 Delta R.T. -0.04 min
 Lab File: BF106850.D
 Acq: 27 Jun 2018 4:14

Tgt Ion:264 Resp: 85264
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.2 28.8
 265 20.3 17.5 26.3

