
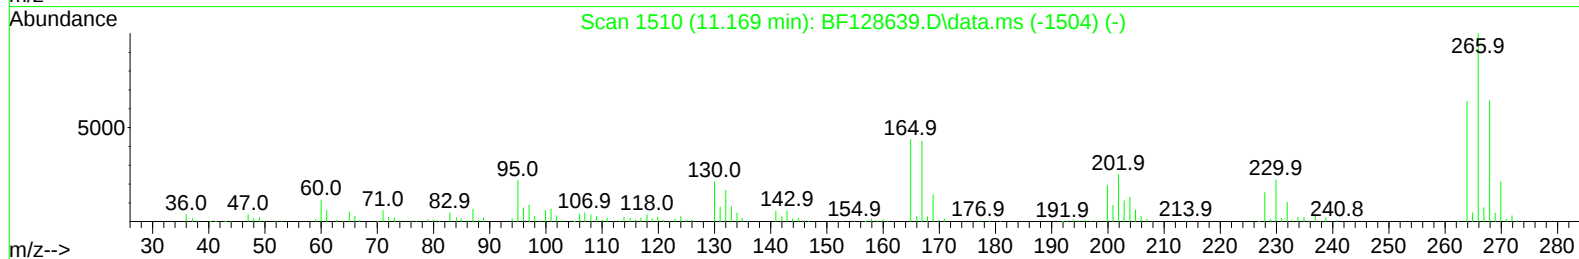
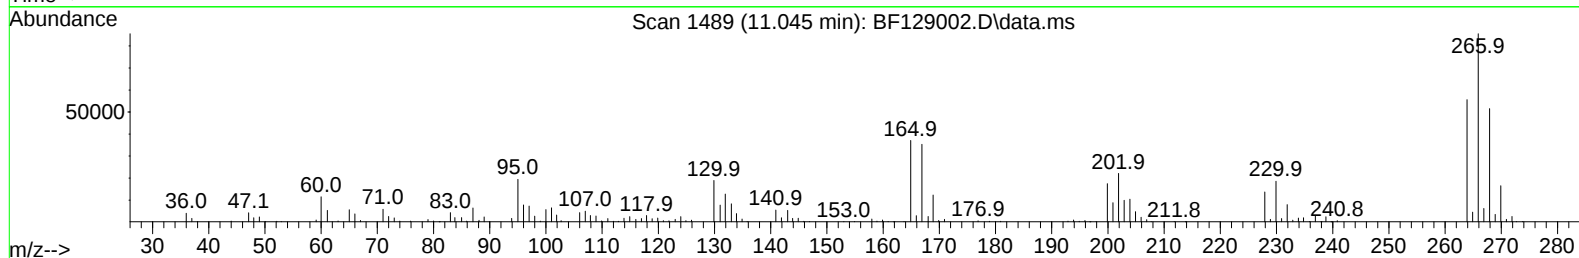


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
 Data File : BF129002.D
 Acq On : 26 Jun 2022 12:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 04:12:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 04:08:24 2022
 Response via : Initial Calibration

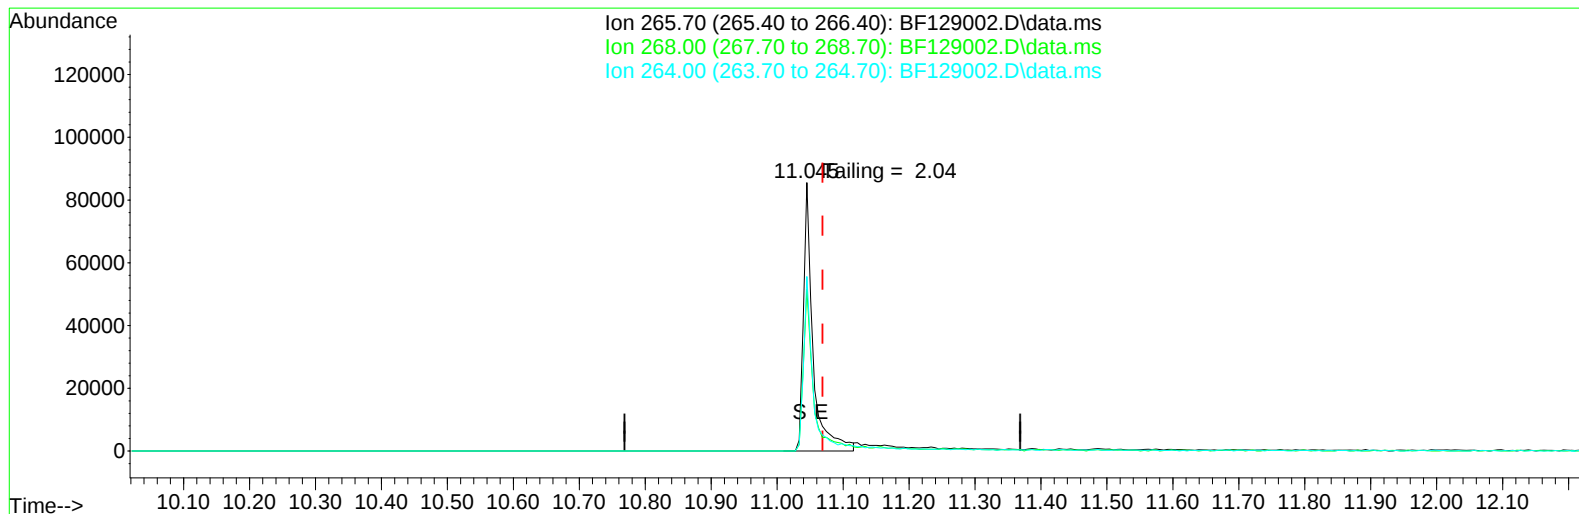

TIC: BF129002.D\data.ms

(70) Pentachlorophenol (C)




11.045min (-0.024) 28280.80 ng

response 96336

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	60.27
264.00	61.80	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129002.D
Acq On : 26 Jun 2022 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 04:12:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 04:08:24 2022
Response via : Initial Calibration

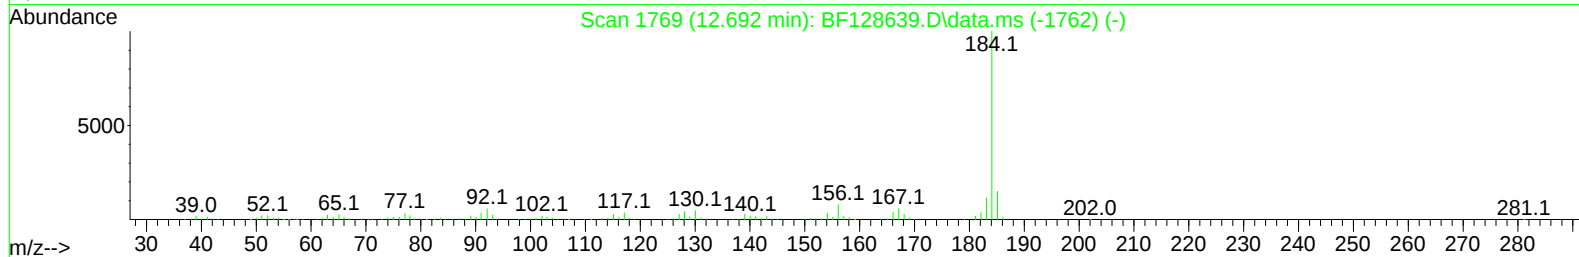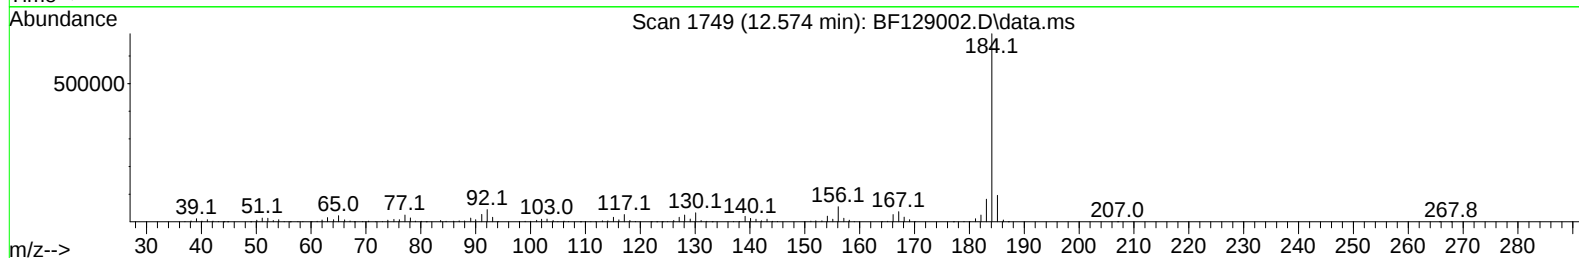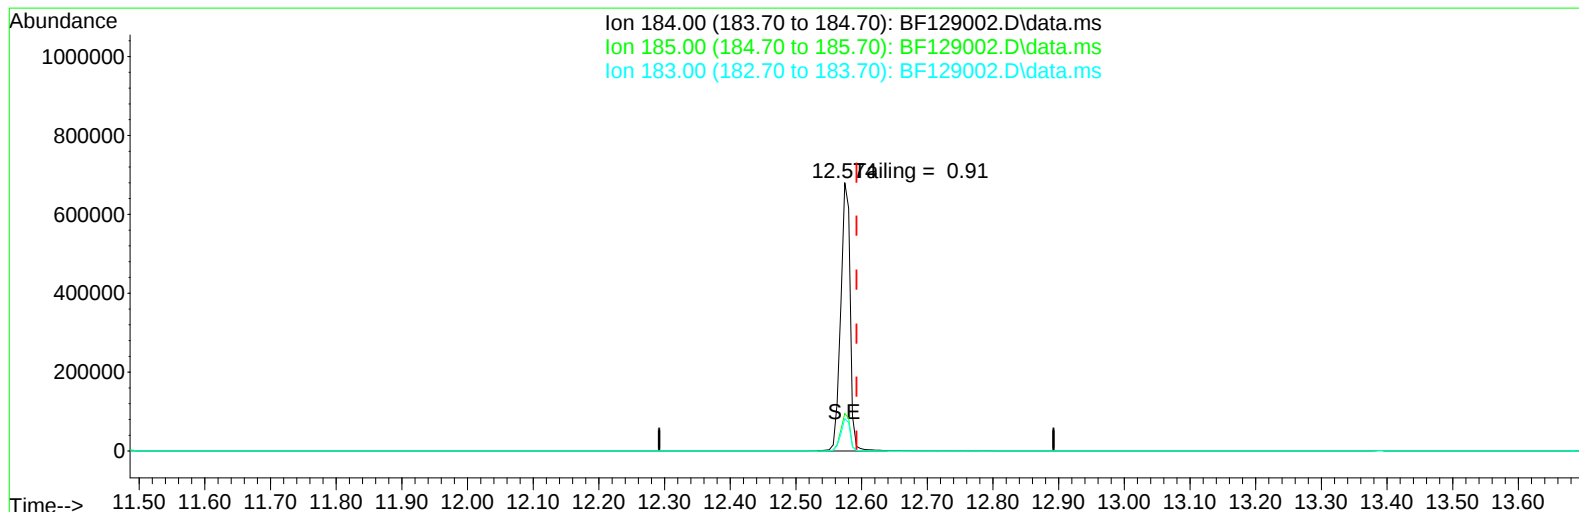

TIC: BF129002.D\data.ms

(77) Benzidine

12.574min (-0.018) 0.00 ng

response 688254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.03
183.00	11.60	12.05
0.00	0.00	0.00