

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
 Data File : BF129014.D
 Acq On : 26 Jun 2022 19:55
 Operator : CG\JU
 Sample : PB145630BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145630BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.934	446	450	459	rBV	37895	54426	1.34%	0.260%
2	5.346	516	520	534	rBV	2002388	2046656	50.41%	9.788%
3	6.363	689	693	709	rBV	1992469	2039528	50.24%	9.754%
4	6.698	747	750	759	rBB	651483	564950	13.92%	2.702%
5	7.275	842	848	851	rBV	1798348	1987396	48.95%	9.505%
6	7.987	964	969	972	rBV	765246	773784	19.06%	3.701%
7	9.063	1146	1152	1155	rBV	3261938	3702521	91.20%	17.707%
8	9.739	1261	1267	1270	rBV	1053126	914300	22.52%	4.373%
9	10.533	1397	1402	1405	rBV	1687826	1445944	35.61%	6.915%
10	11.227	1514	1520	1523	rBV	1214815	992669	24.45%	4.747%
11	12.822	1785	1791	1794	rBV	4229392	4059949	100.00%	19.417%
12	13.874	1966	1970	1973	rBV	943552	895896	22.07%	4.285%
13	13.963	1978	1985	1994	rBV	241497	268686	6.62%	1.285%
14	14.957	2149	2154	2159	rVB	49382	55198	1.36%	0.264%
15	15.304	2208	2213	2223	rBV	686086	842482	20.75%	4.029%
16	15.721	2278	2284	2290	rBV	54757	79633	1.96%	0.381%
17	16.186	2358	2363	2369	rVB	50271	80472	1.98%	0.385%
18	16.739	2450	2457	2466	rBV	26917	57141	1.41%	0.273%
19	17.386	2560	2567	2577	rBV3	18205	47761	1.18%	0.228%




Sum of corrected areas: 20909392

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129014.D
Acq On : 26 Jun 2022 19:55
Operator : CG\JU
Sample : PB145630BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145630BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

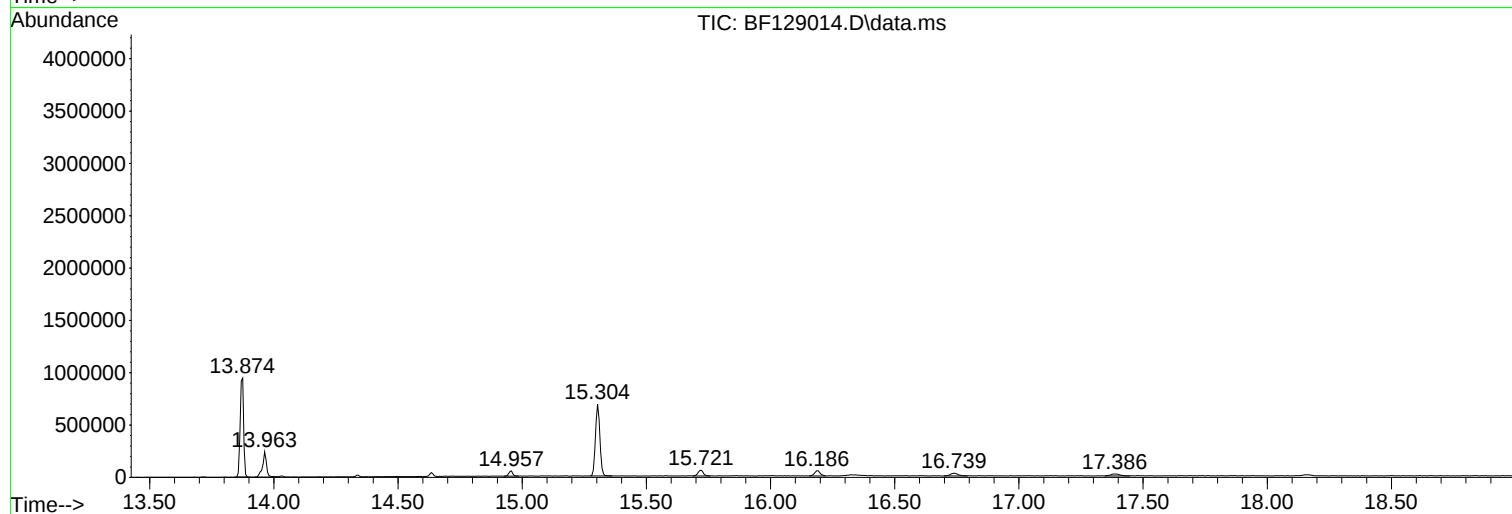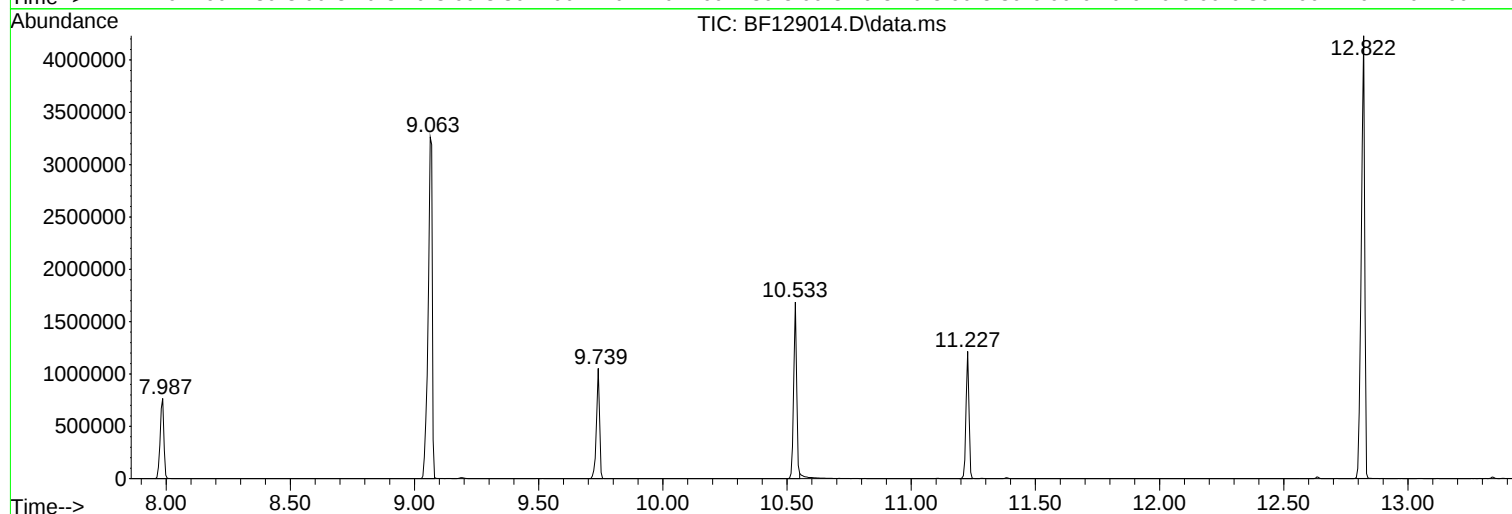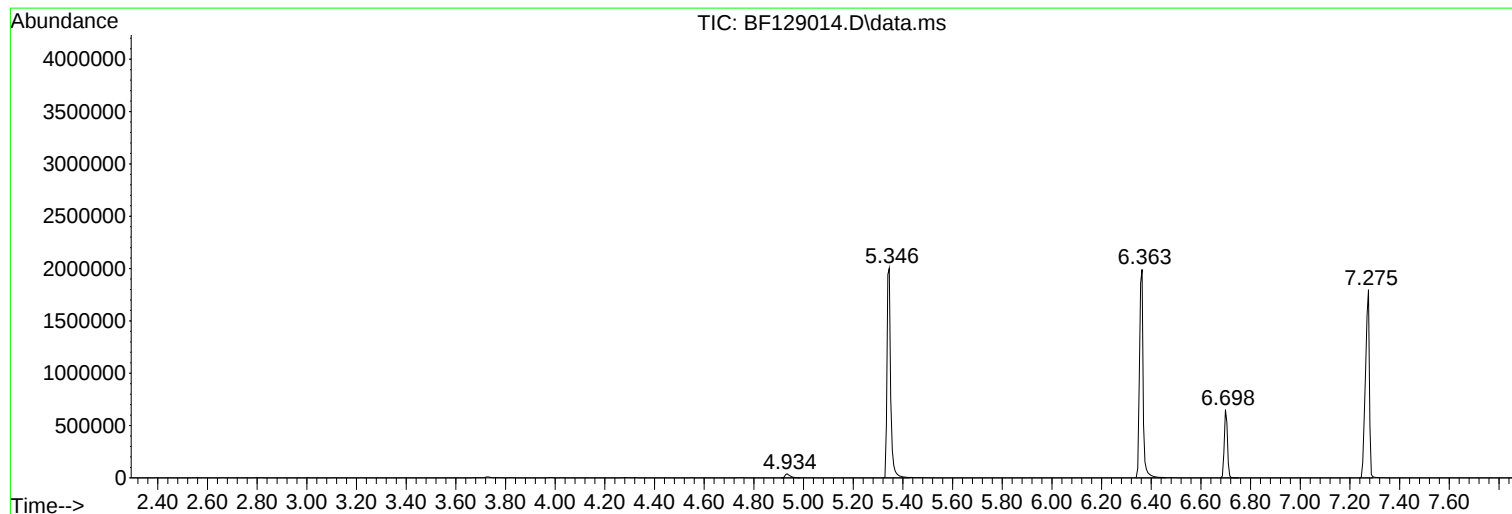

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129014.D
Acq On : 26 Jun 2022 19:55
Operator : CG\JU
Sample : PB145630BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145630BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.963	6.00 ng	268686	Chrysene-d12	13.874

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			Vanadium, cycloheptatrienyl-(pen...]	277	C17H22V	1000155-20-5	43
5			Cobalt,(.eta.<5>-2,4-cyclopentad...]	277	C16H15BCo	036682-12-9	38

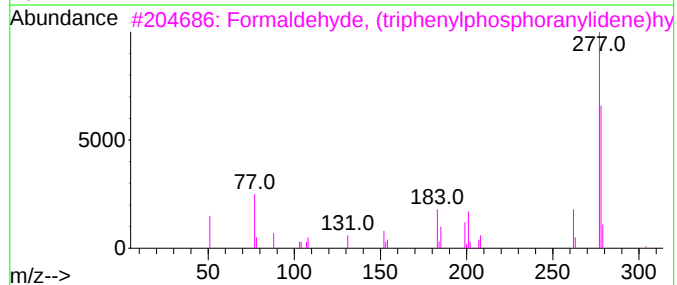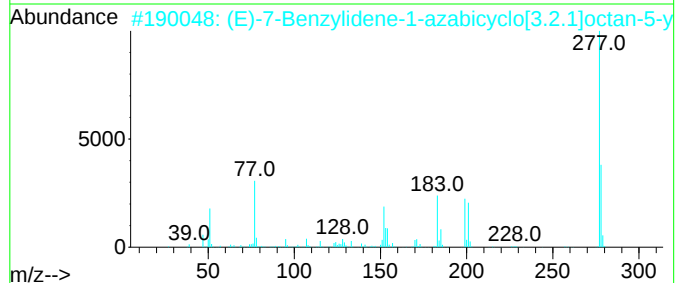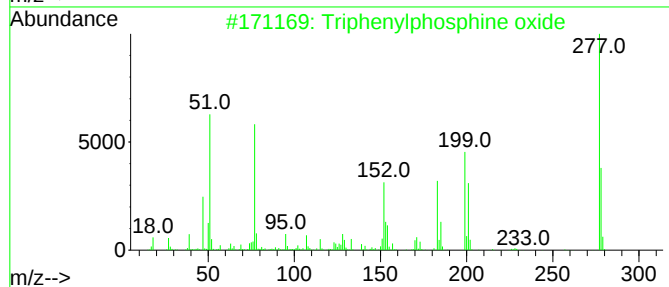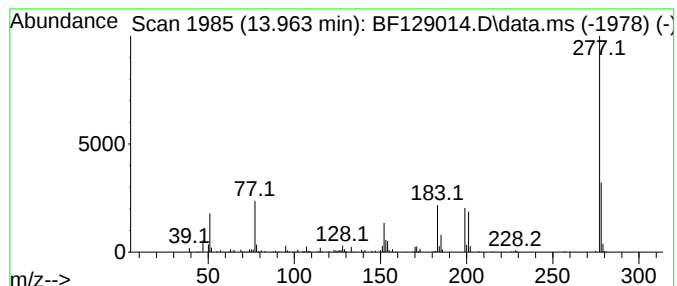

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129014.D
Acq On : 26 Jun 2022 19:55
Operator : CG\JU
Sample : PB145630BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145630BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.963	6.0	ng	268686	5	13.874	895896	20.0