

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
 Data File : BF129018.D
 Acq On : 26 Jun 2022 21:53
 Operator : CG\JU
 Sample : PB145737BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145737BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.345	516	520	538	rBV	3222066	3113934	72.36%	12.999%
2	6.363	689	693	696	rBV	2737439	3033694	70.49%	12.664%
3	6.698	747	750	761	rBV	678679	602798	14.01%	2.516%
4	7.275	842	848	851	rBV	1903155	2133280	49.57%	8.905%
5	7.986	964	969	972	rBV	794593	778783	18.10%	3.251%
6	9.063	1146	1152	1155	rBV	3434314	3986618	92.63%	16.642%
7	9.739	1261	1267	1270	rBV	1044920	909058	21.12%	3.795%
8	10.533	1396	1402	1415	rBV	2158821	2290346	53.22%	9.561%
9	11.227	1514	1520	1523	rBV	1196130	980019	22.77%	4.091%
10	12.821	1785	1791	1794	rBV	4290231	4303582	100.00%	17.965%
11	13.868	1966	1969	1973	rBV	897916	869152	20.20%	3.628%
12	13.963	1979	1985	1992	rBV	228188	261857	6.08%	1.093%
13	15.304	2208	2213	2224	rVB	559850	692258	16.09%	2.890%




Sum of corrected areas: 23955379

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129018.D
Acq On : 26 Jun 2022 21:53
Operator : CG\JU
Sample : PB145737BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

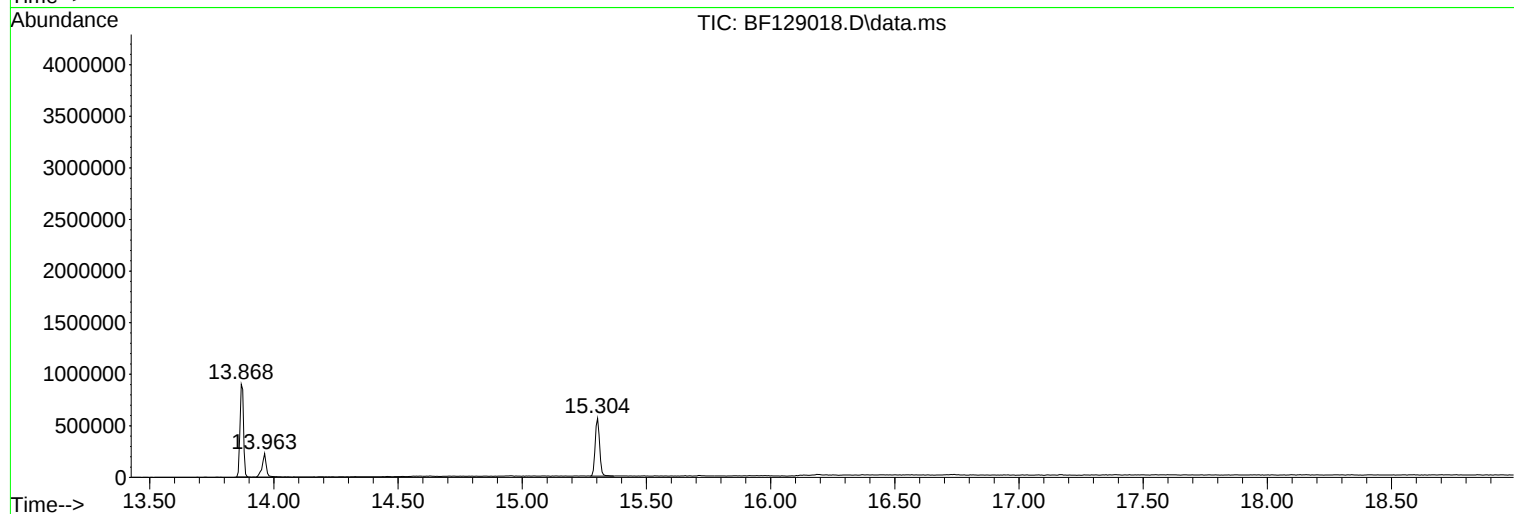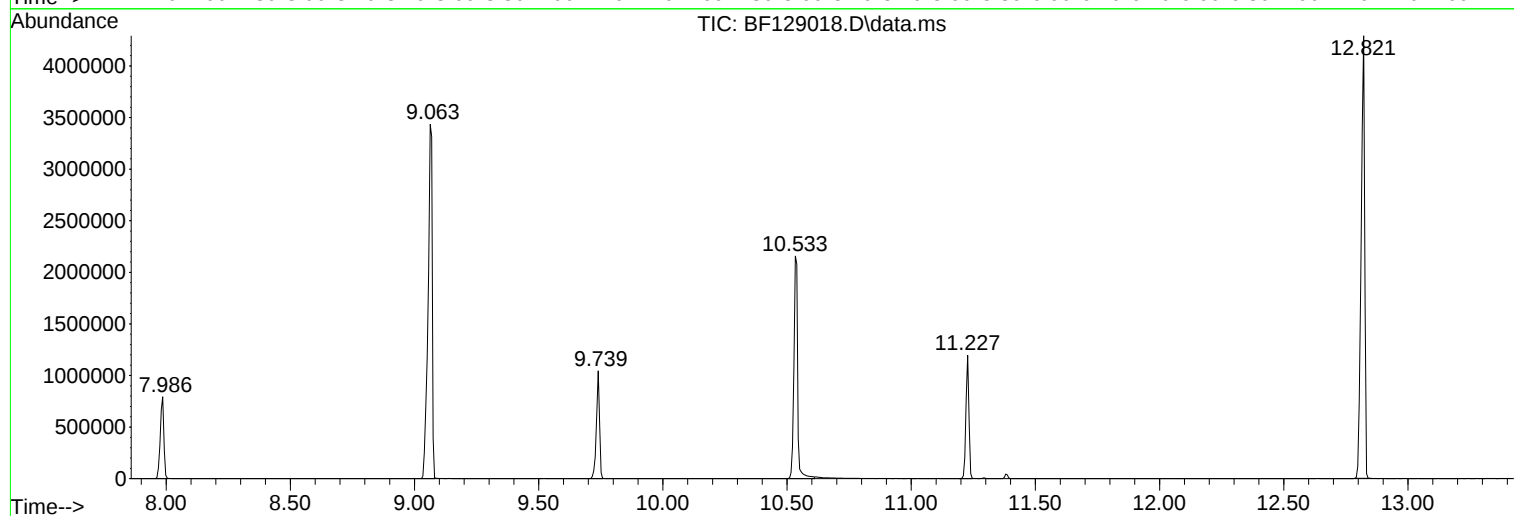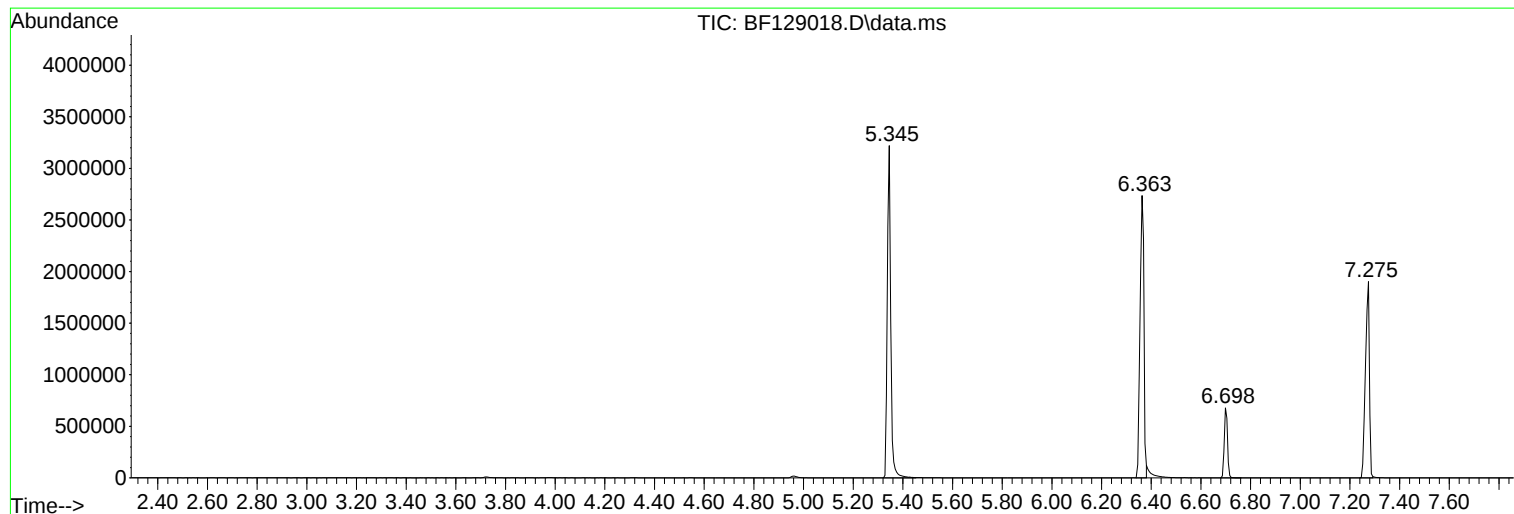

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129018.D
Acq On : 26 Jun 2022 21:53
Operator : CG\JU
Sample : PB145737BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145737BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.963	6.03 ng	261857	Chrysene-d12	13.868

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	52
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	42
4			Cobalt, (.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	17
5			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5C12NOS2	017046-34-3	16

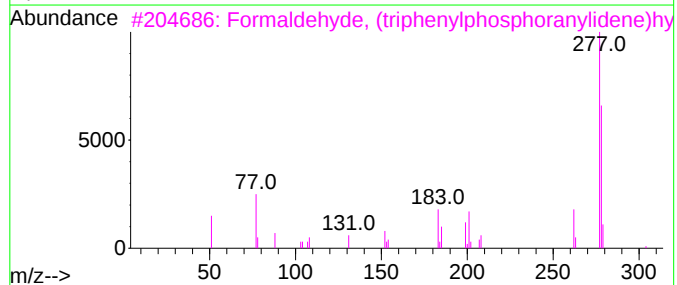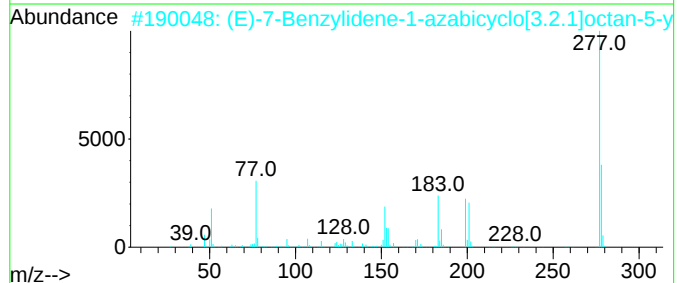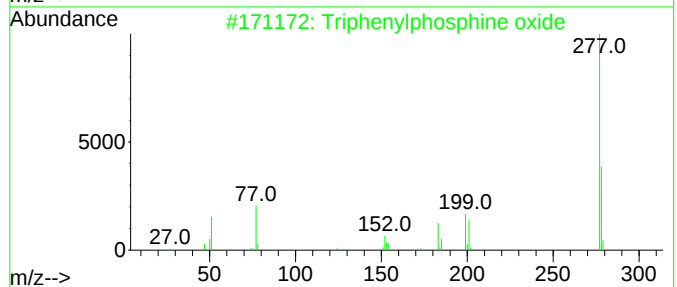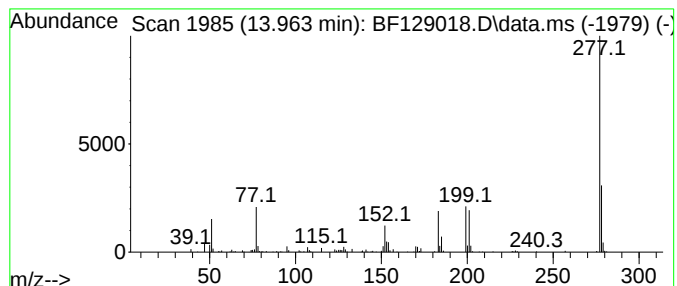

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129018.D
Acq On : 26 Jun 2022 21:53
Operator : CG\JU
Sample : PB145737BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.963	6.0	ng	261857	5	13.868	869152	20.0