
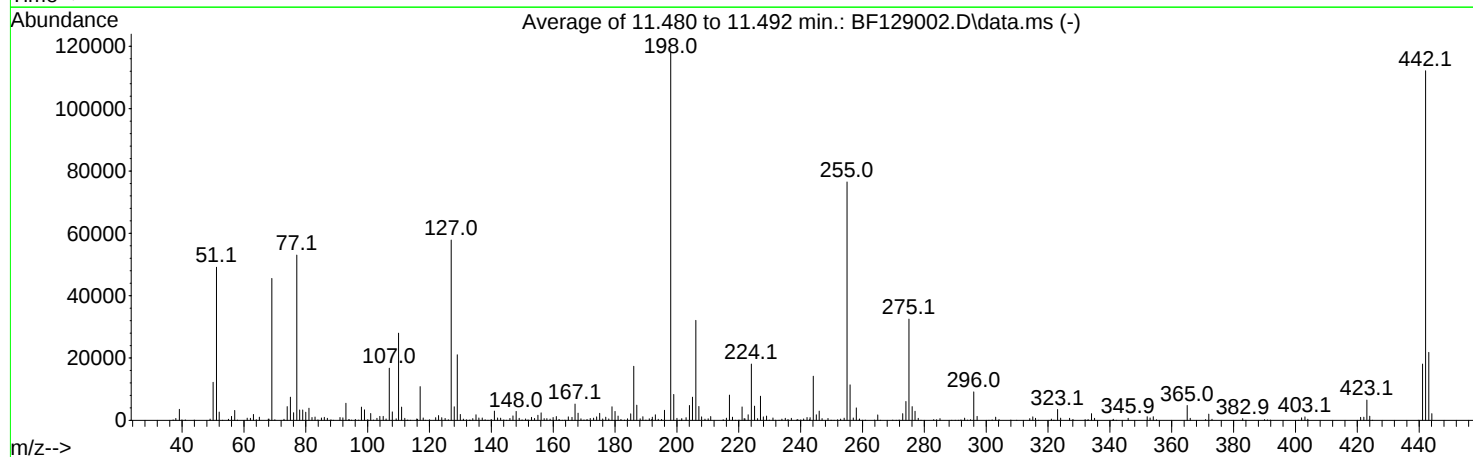


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
 Data File : BF129002.D
 Acq On : 26 Jun 2022 12:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 16:19:25 2022

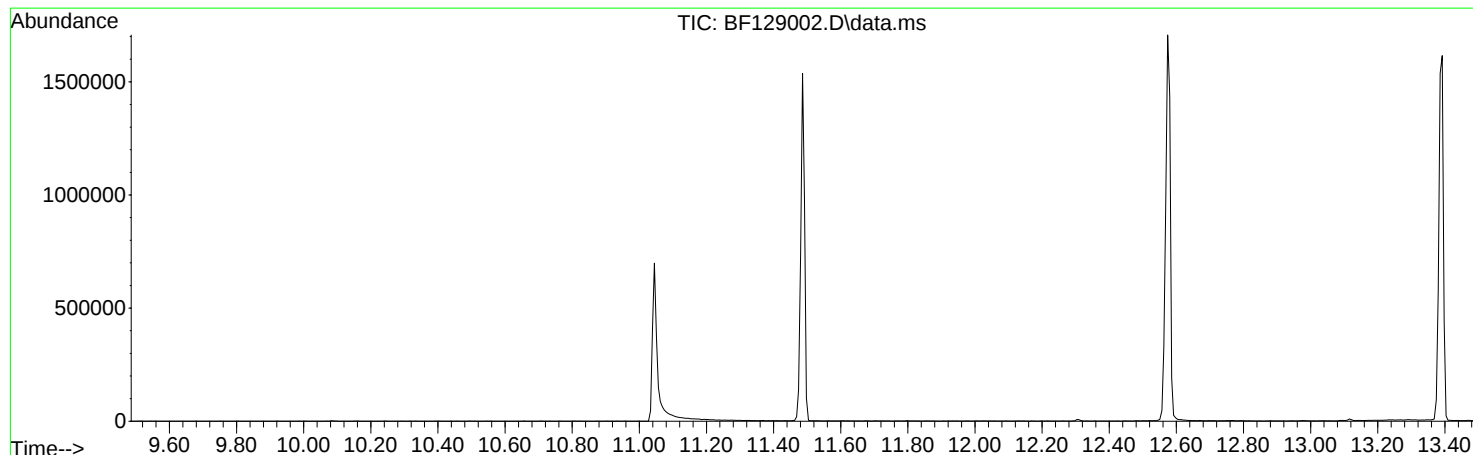




AutoFind: Scans 1563, 1564, 1565; Background Corrected with Scan 1557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	49136	PASS
68	69	0.00	2	1.0	434	PASS
69	198	0.00	100	38.6	45539	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	49.0	57848	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	118024	PASS
199	198	5	9	7.0	8303	PASS
275	198	10	60	27.5	32483	PASS
365	198	1	100	4.1	4793	PASS
441	198	0.01	100	15.3	18070	PASS
442	442	50	100	100.0	112163	PASS
443	442	15	24	19.5	21837	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129002.D
Acq On : 26 Jun 2022 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 27 04:12:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 04:08:24 2022
Response via : Initial Calibration

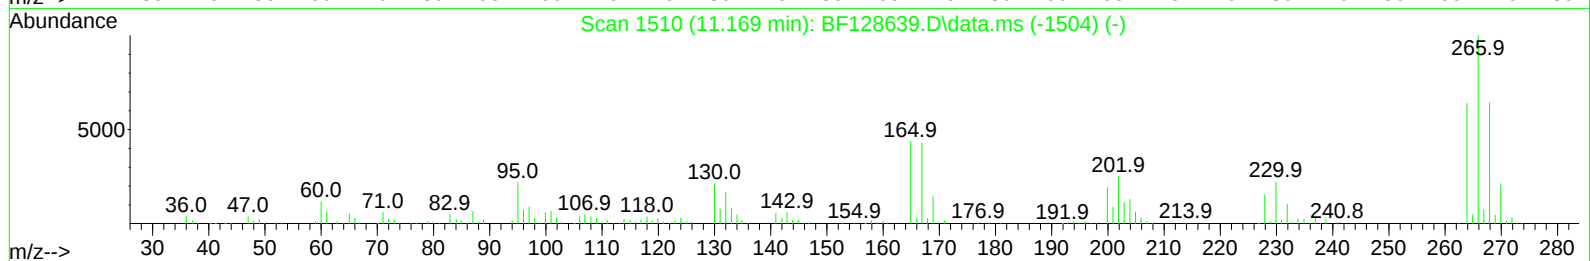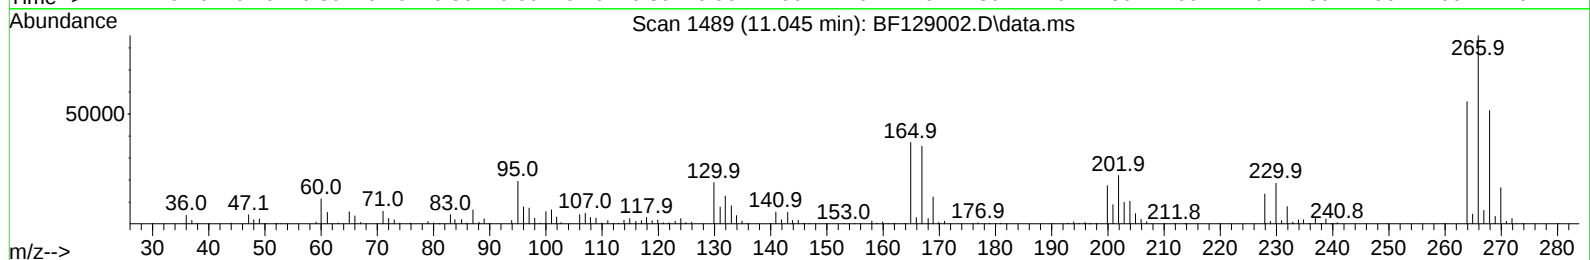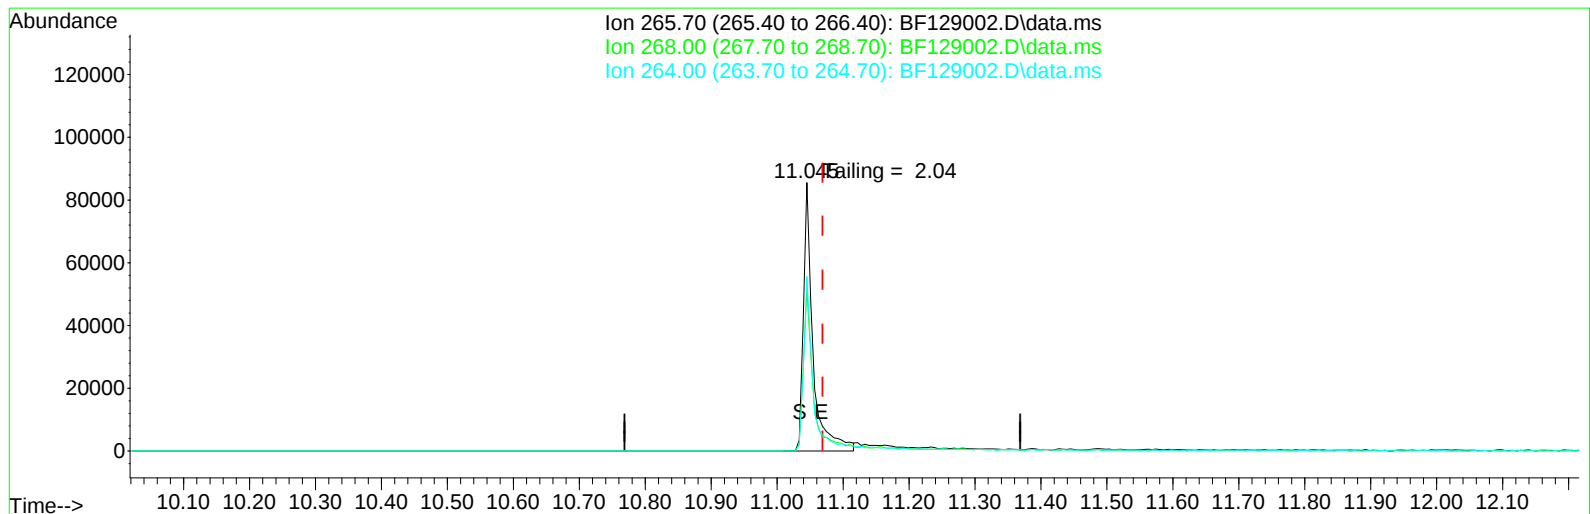

TIC: BF129002.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.024) 28280.80 ng




response 96336

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	60.27
264.00	61.80	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062622\
Data File : BF129002.D
Acq On : 26 Jun 2022 12:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 27 04:12:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 04:08:24 2022
Response via : Initial Calibration

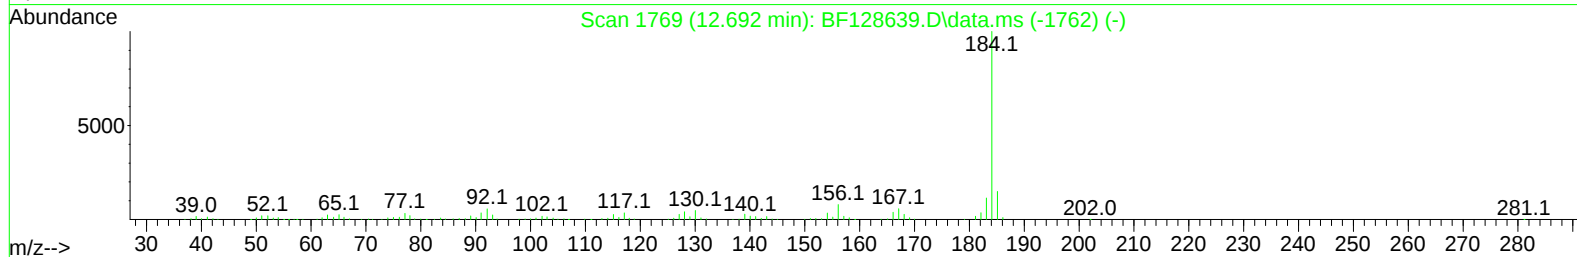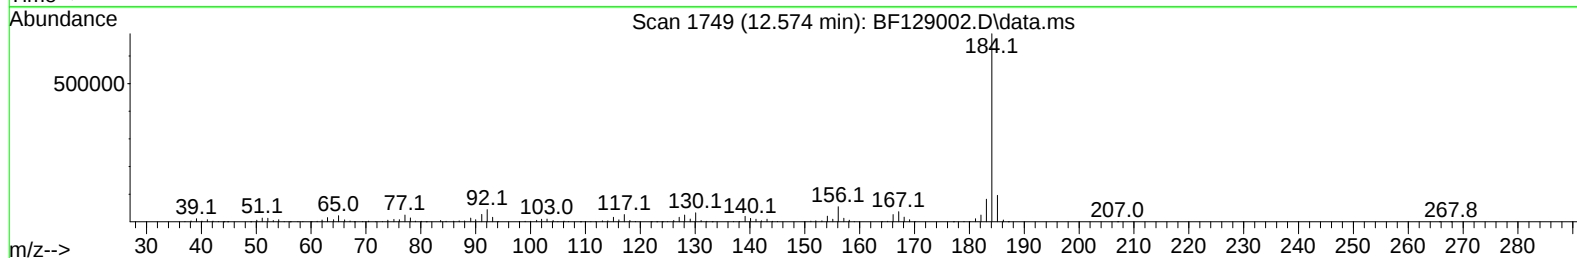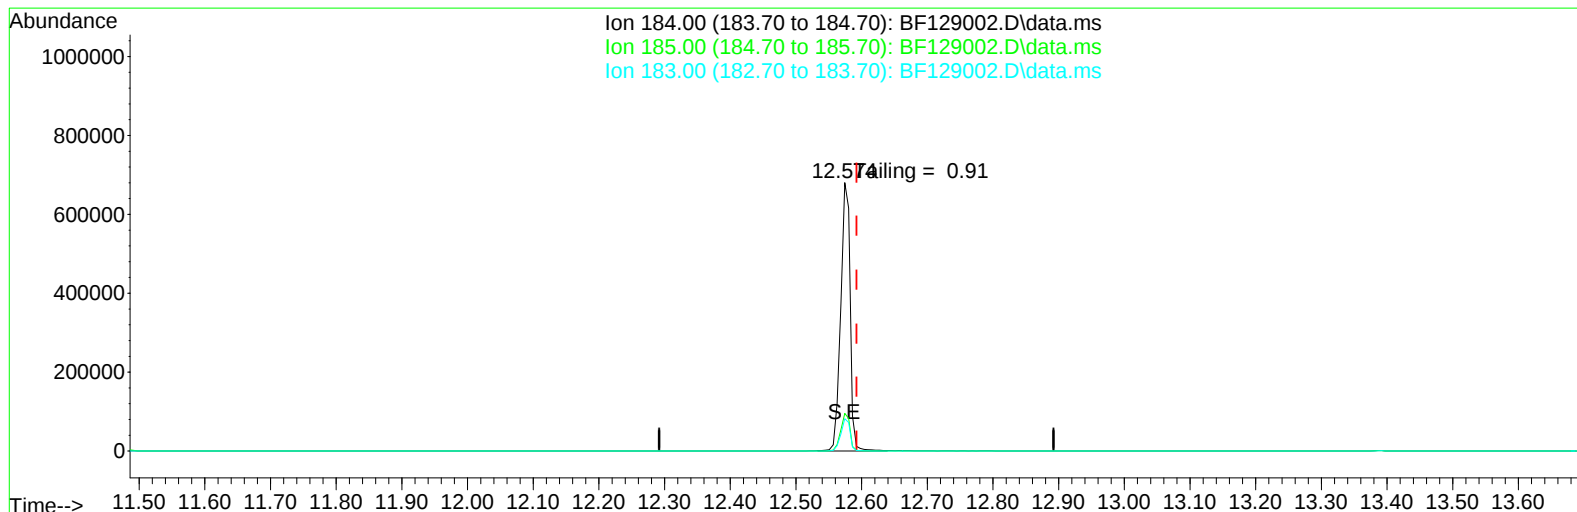

TIC: BF129002.D\data.ms

(77) Benzidine

12.574min (-0.018) 0.00 ng

response 688254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.03
183.00	11.60	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/26/2022	BNA_F	<u>BF129002.D</u>
Compound Name	Response	Retention Time
DDT	297607	13.39
DDD	746	13.09
DDE	568	12.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1314	298921	0.44

Instrument :
BNA_F
ClientSampleId :
DFTPP