
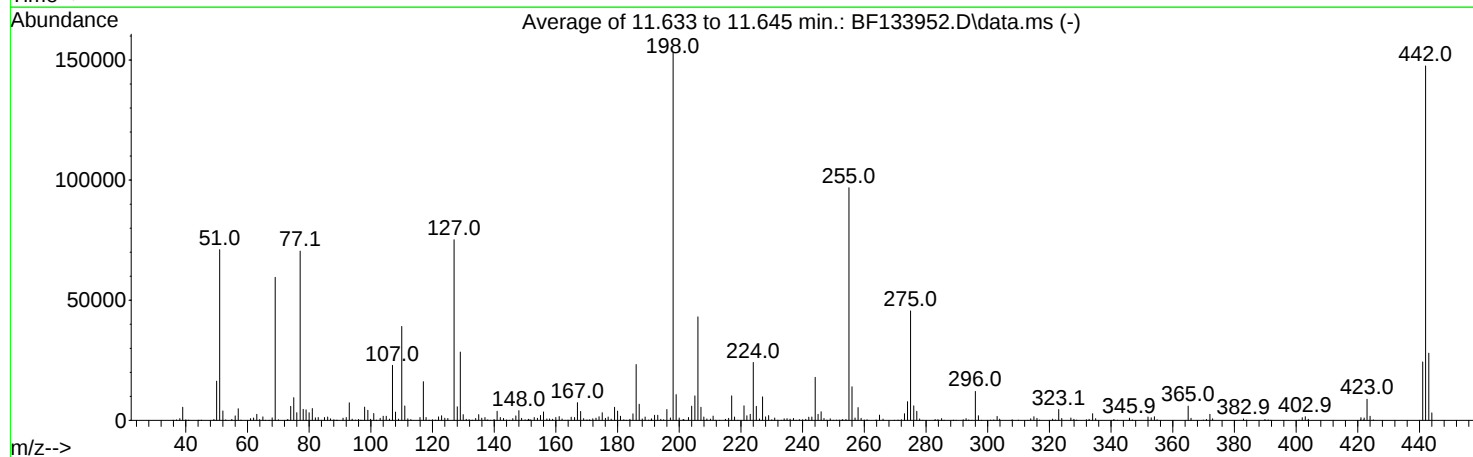


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062623\
 Data File : BF133952.D
 Acq On : 26 Jun 2023 14:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 26 23:12:04 2023

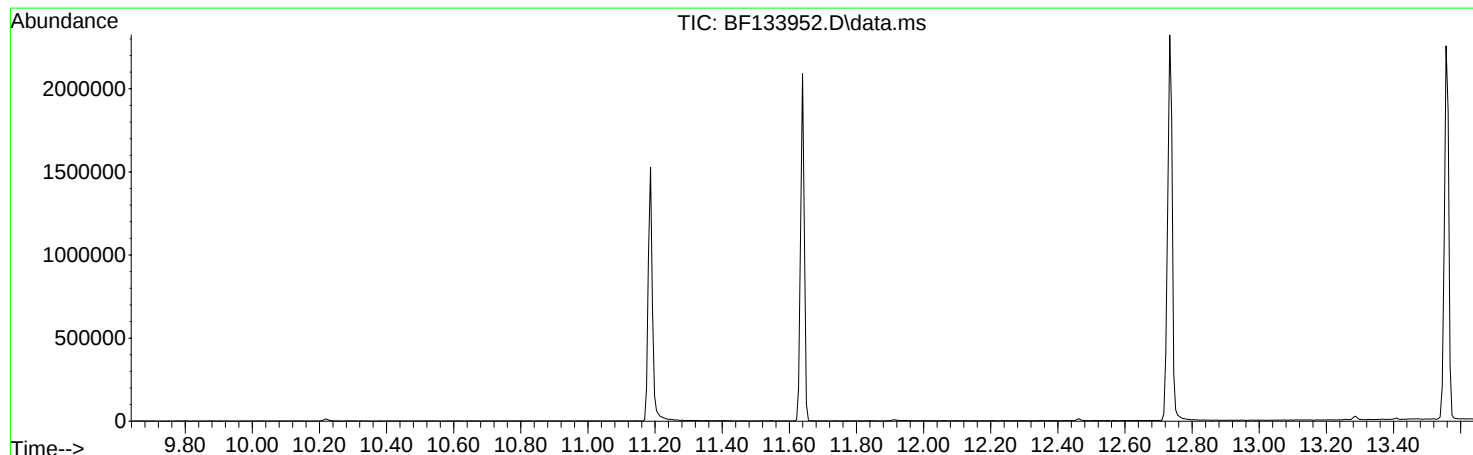

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	71069	PASS
68	69	0.00	2	1.8	1094	PASS
69	198	0.00	100	38.9	59539	PASS
70	69	0.00	2	0.5	270	PASS
127	198	10	80	49.1	75219	PASS
197	198	0.00	2	0.7	1006	PASS
198	198	100	100	100.0	153117	PASS
199	198	5	9	7.0	10739	PASS
275	198	10	60	29.7	45536	PASS
365	198	1	100	3.9	5946	PASS
441	198	0.01	100	15.9	24328	PASS
442	442	50	100	100.0	147541	PASS
443	442	15	24	19.0	27994	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/26/2023	BNA_F	<u>BF133952.D</u>
Compound Name	Response	Retention Time
DDT	393321	13.557
DDD	5174	13.286
DDE	0	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5174	398495	1.30

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062623\
 Data File : BF133952.D
 Acq On : 26 Jun 2023 14:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 27 07:40:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 23:12:04 2023
 Response via : Initial Calibration

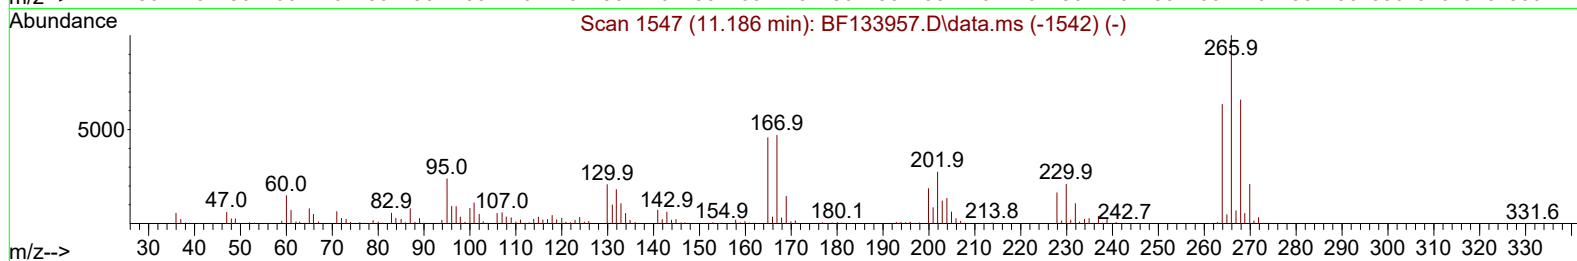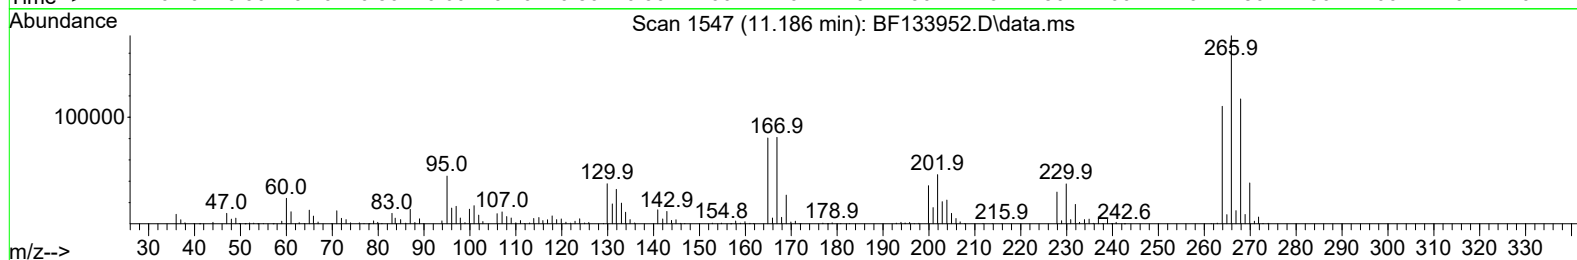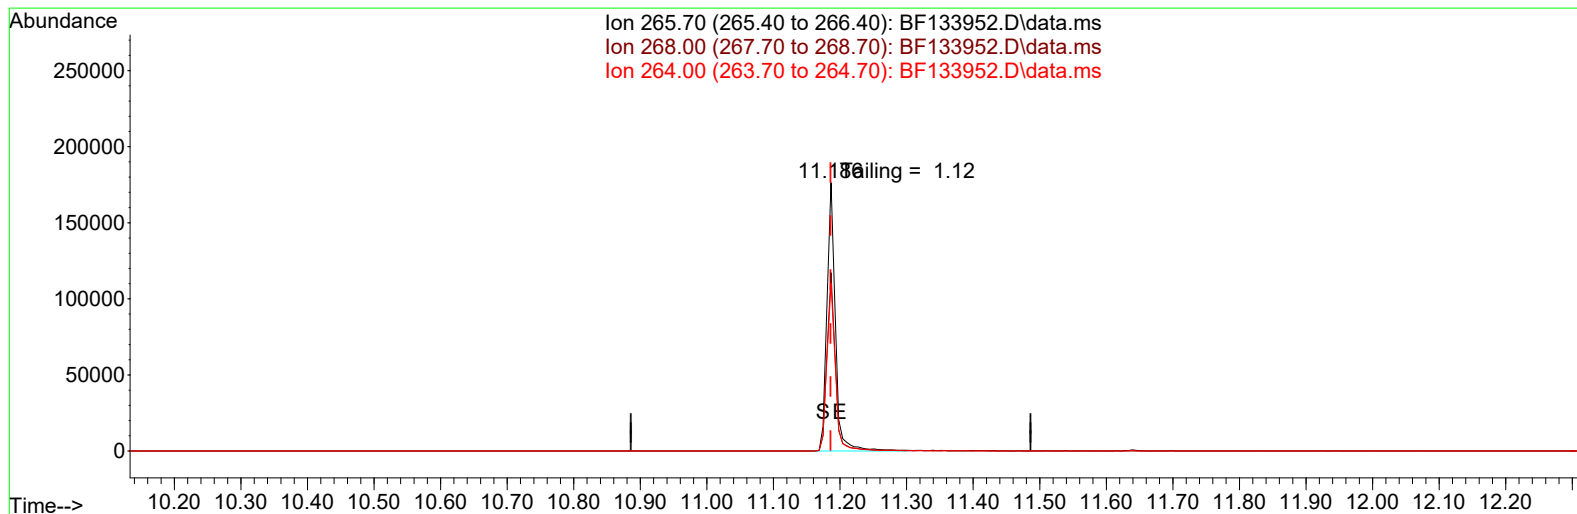

TIC: BF133952.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 35045.89 ng




response 156312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	66.41
264.00	63.30	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062623\
 Data File : BF133952.D
 Acq On : 26 Jun 2023 14:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 27 07:40:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 23:12:04 2023
 Response via : Initial Calibration

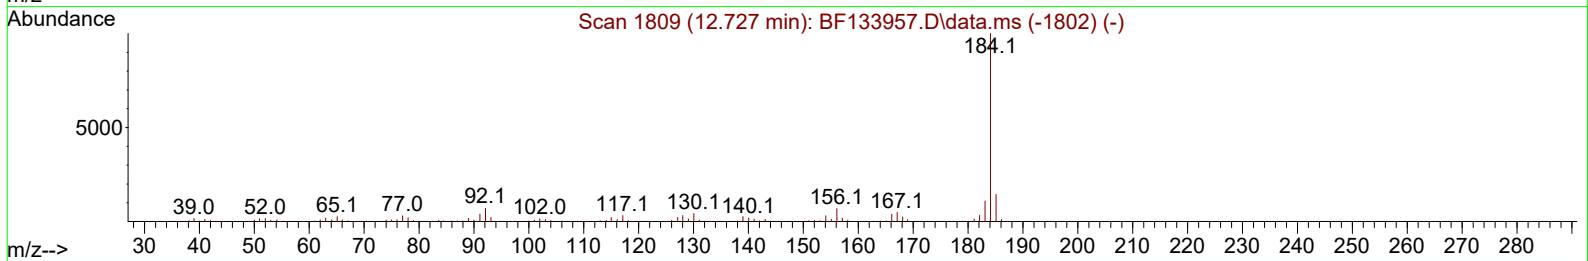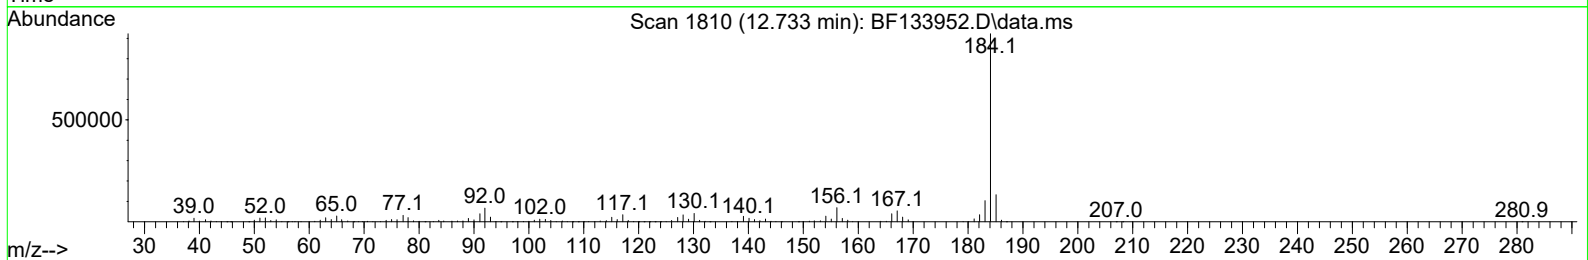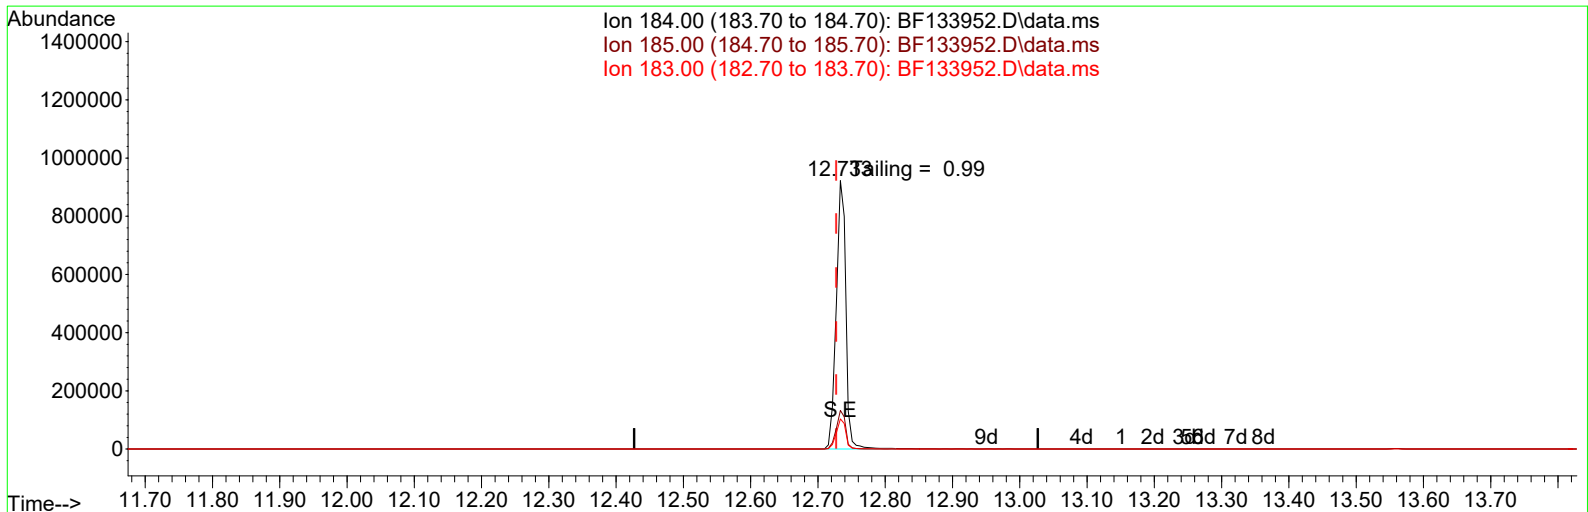

TIC: BF133952.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 601006.30 ng m

response 915235

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.40
183.00	11.00	11.21
0.00	0.00	0.00