


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062623\
Data File : BF133968.D
Acq On : 27 Jun 2023 00:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 26 23:12:04 2023

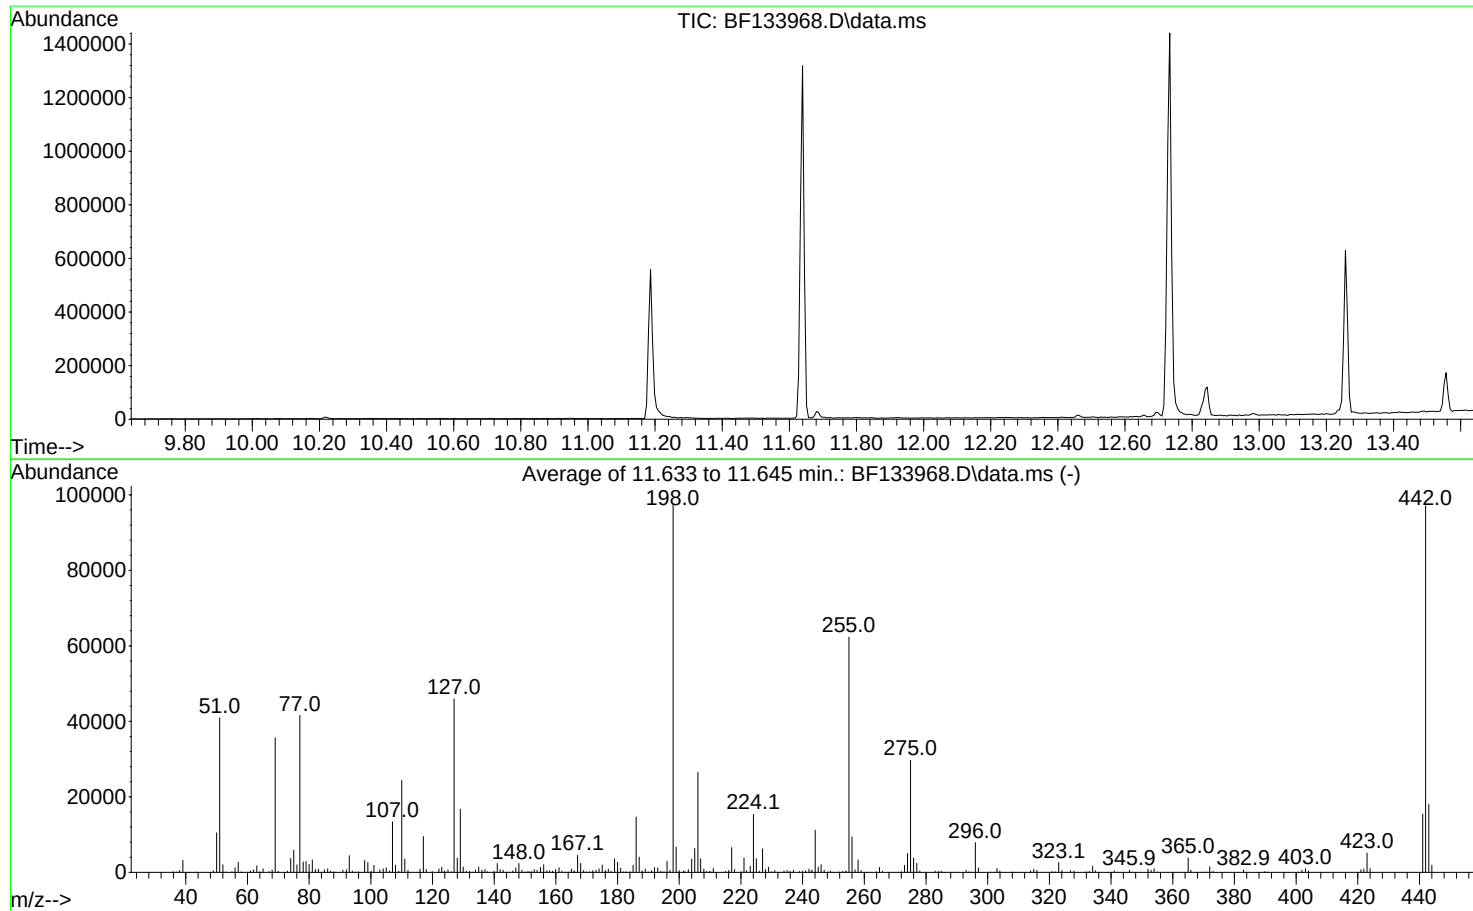

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	40925	PASS
68	69	0.00	2	1.8	647	PASS
69	198	0.00	100	36.6	35663	PASS
70	69	0.00	2	0.8	292	PASS
127	198	10	80	47.1	45939	PASS
197	198	0.00	2	0.6	547	PASS
198	198	100	100	100.0	97461	PASS
199	198	5	9	6.9	6686	PASS
275	198	10	60	30.5	29677	PASS
365	198	1	100	3.9	3843	PASS
441	198	0.01	100	15.9	15488	PASS
442	442	50	100	100.0	97107	PASS
443	442	15	24	18.5	17962	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/26/2023	BNA_F	<u>BF133968.D</u>
Compound Name	Response	Retention Time
DDT	22255	13.557
DDD	95937	13.257
DDE	17308	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
113245	135500	83.58

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062623\
 Data File : BF133968.D
 Acq On : 27 Jun 2023 00:54
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 27 07:27:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 23:12:04 2023
 Response via : Initial Calibration

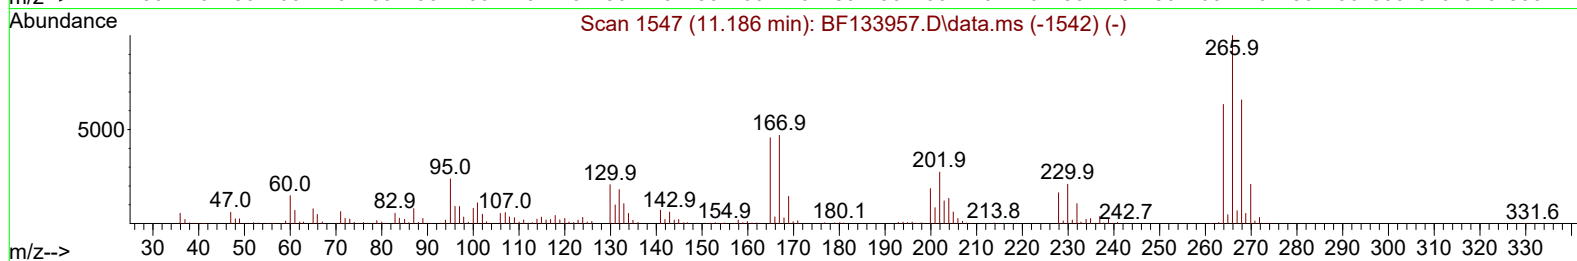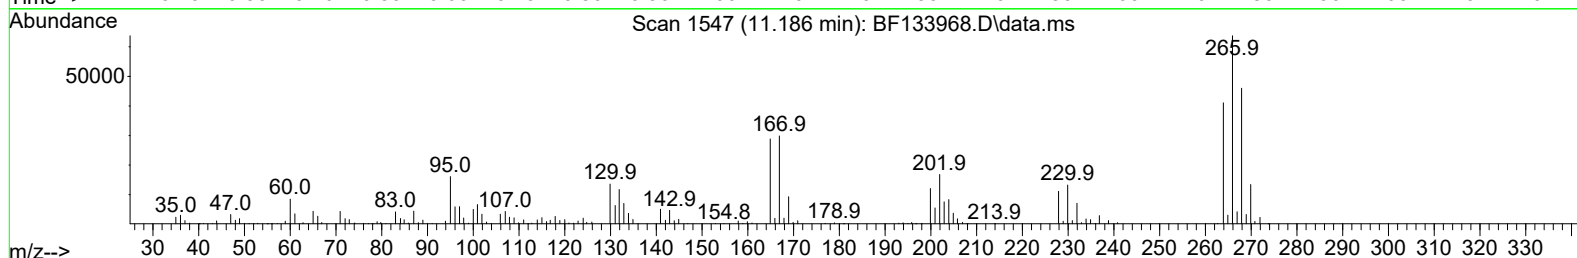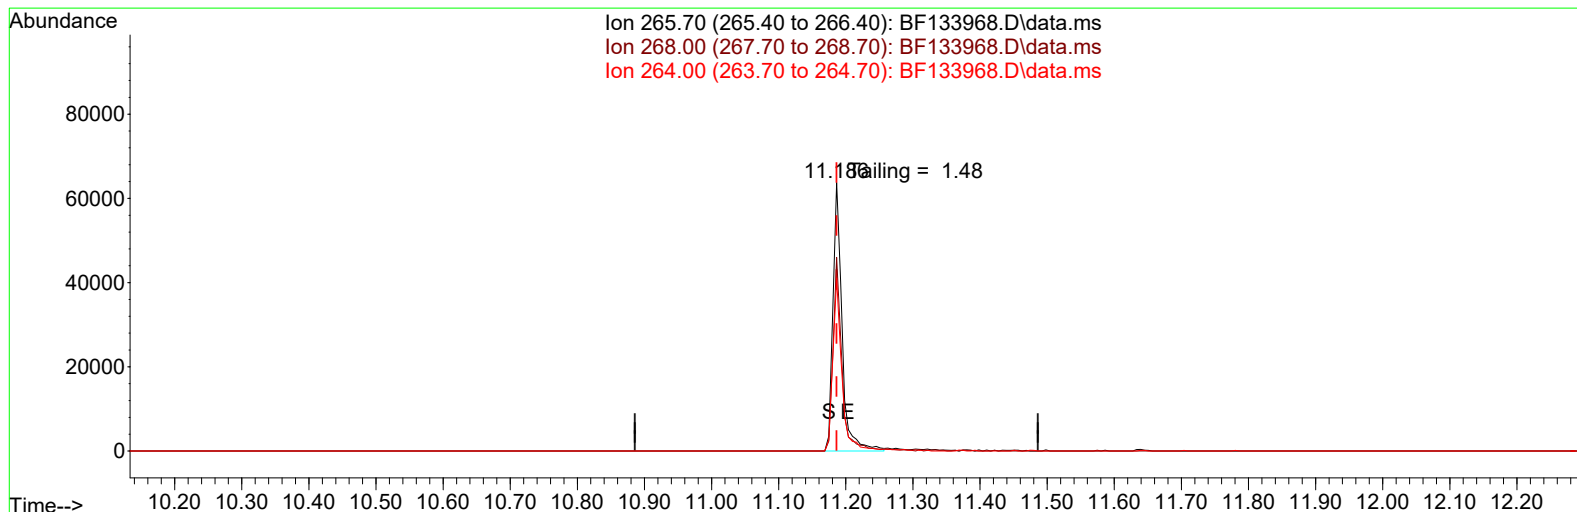

TIC: BF133968.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 19871.68 ng




response 61278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	72.13
264.00	63.30	64.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062623\
Data File : BF133968.D
Acq On : 27 Jun 2023 00:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 27 07:27:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

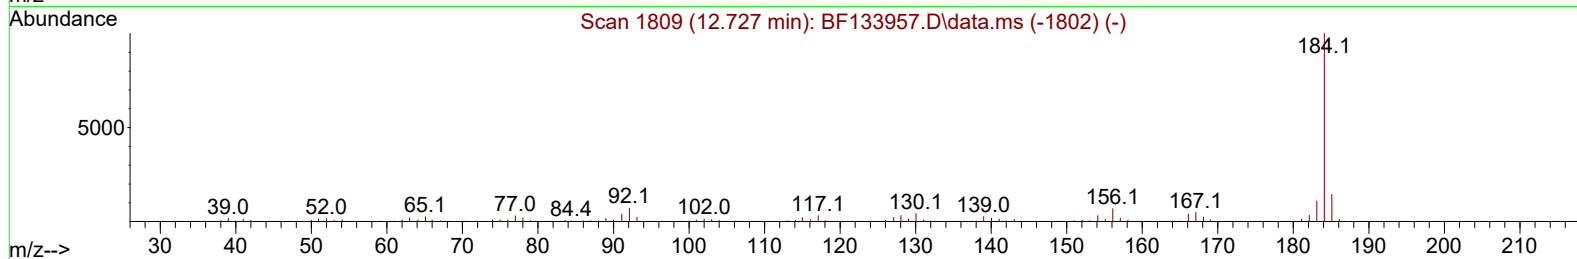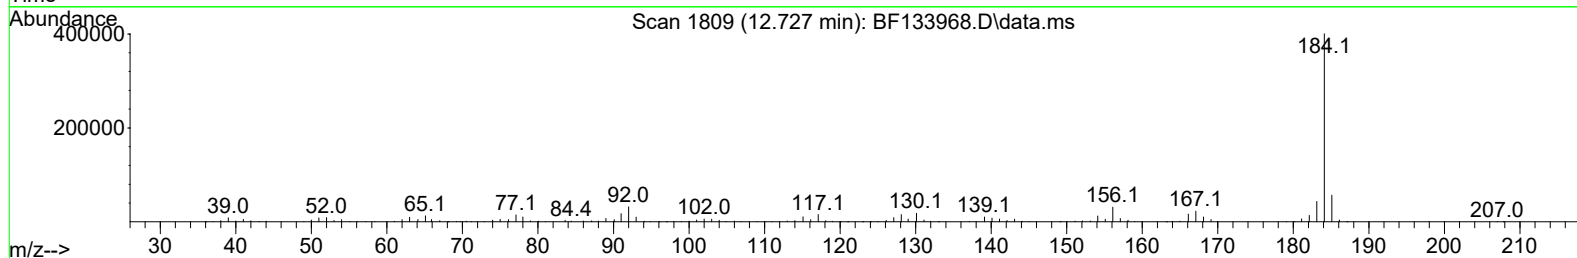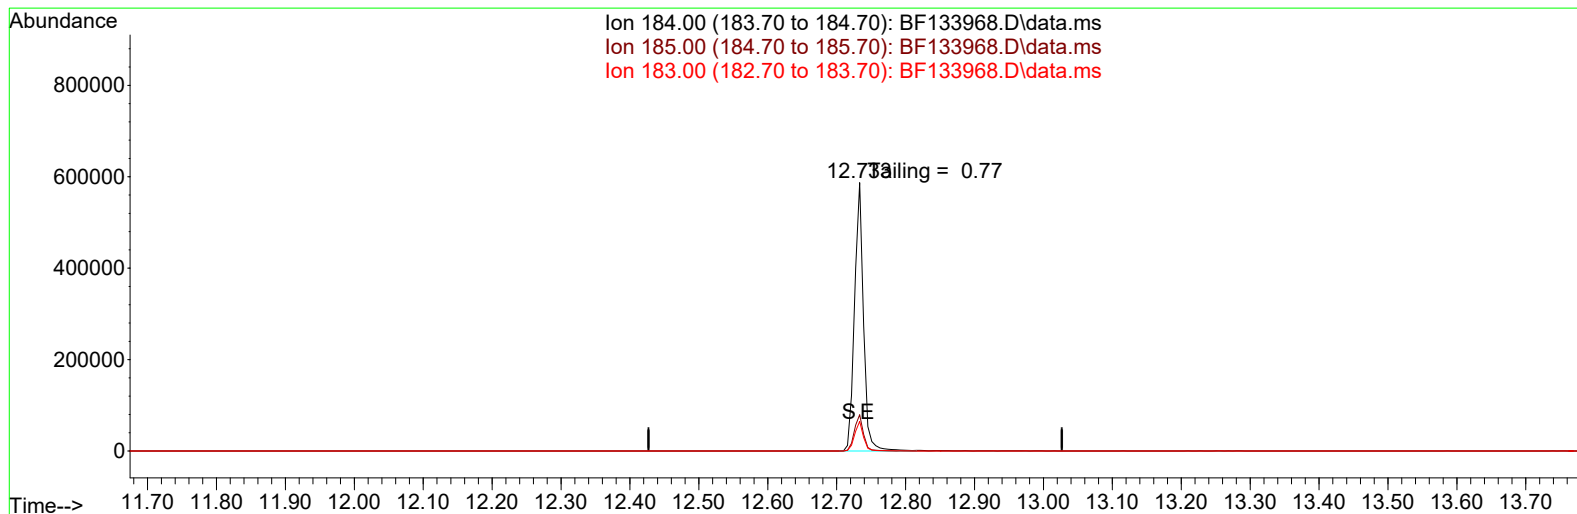

TIC: BF133968.D\data.ms

(77) Benzidine

12.727min (-12.727) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.50	0.00#
183.00	11.00	0.00#
0.00	0.00	0.00