

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106874.D
 Acq On : 27 Jun 2018 16:16
 Operator : JU/SJ
 Sample : J3680-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-01-E6-F6-E6A-F6A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.195	482	486	494	rBV	88016	106432	9.32%	1.088%
2	5.595	550	554	558	rBV	947287	881317	77.15%	9.009%
3	6.595	719	724	727	rBV	889038	922696	80.77%	9.432%
4	6.731	742	747	750	rBV	1025676	931556	81.54%	9.523%
5	6.954	781	785	788	rBV	366442	301142	26.36%	3.078%
6	7.107	807	811	815	rBV	805043	751054	65.74%	7.677%
7	7.519	876	881	884	rBV	641290	598774	52.41%	6.121%
8	8.236	999	1003	1021	rVB	475957	403546	35.32%	4.125%
9	9.313	1181	1186	1189	rBV	1180036	1142397	100.00%	11.678%
10	9.701	1248	1252	1259	rBB	171691	135012	11.82%	1.380%
11	9.907	1284	1287	1291	rBV2	12316	12702	1.11%	0.130%
12	9.995	1298	1302	1306	rBV2	563999	480126	42.03%	4.908%
13	10.407	1369	1372	1374	rVB	26263	22149	1.94%	0.226%
14	10.789	1433	1437	1441	rBV	815865	763060	66.79%	7.800%
15	10.877	1449	1452	1458	rBV	30936	29166	2.55%	0.298%
16	11.324	1525	1528	1531	rBV	14523	12543	1.10%	0.128%
17	11.489	1552	1556	1559	rBV	572700	488588	42.77%	4.994%
18	13.071	1821	1825	1828	rBV	1162766	1037213	90.79%	10.603%
19	13.954	1972	1975	1980	rBV	24088	30296	2.65%	0.310%
20	14.142	2003	2007	2011	rBV	372188	332513	29.11%	3.399%
21	15.689	2263	2270	2277	rBV	292841	400291	35.04%	4.092%


Sum of corrected areas: 9782573

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106874.D
Acq On : 27 Jun 2018 16:16
Operator : JU/SJ
Sample : J3680-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-E6-F6-E6A-F6A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

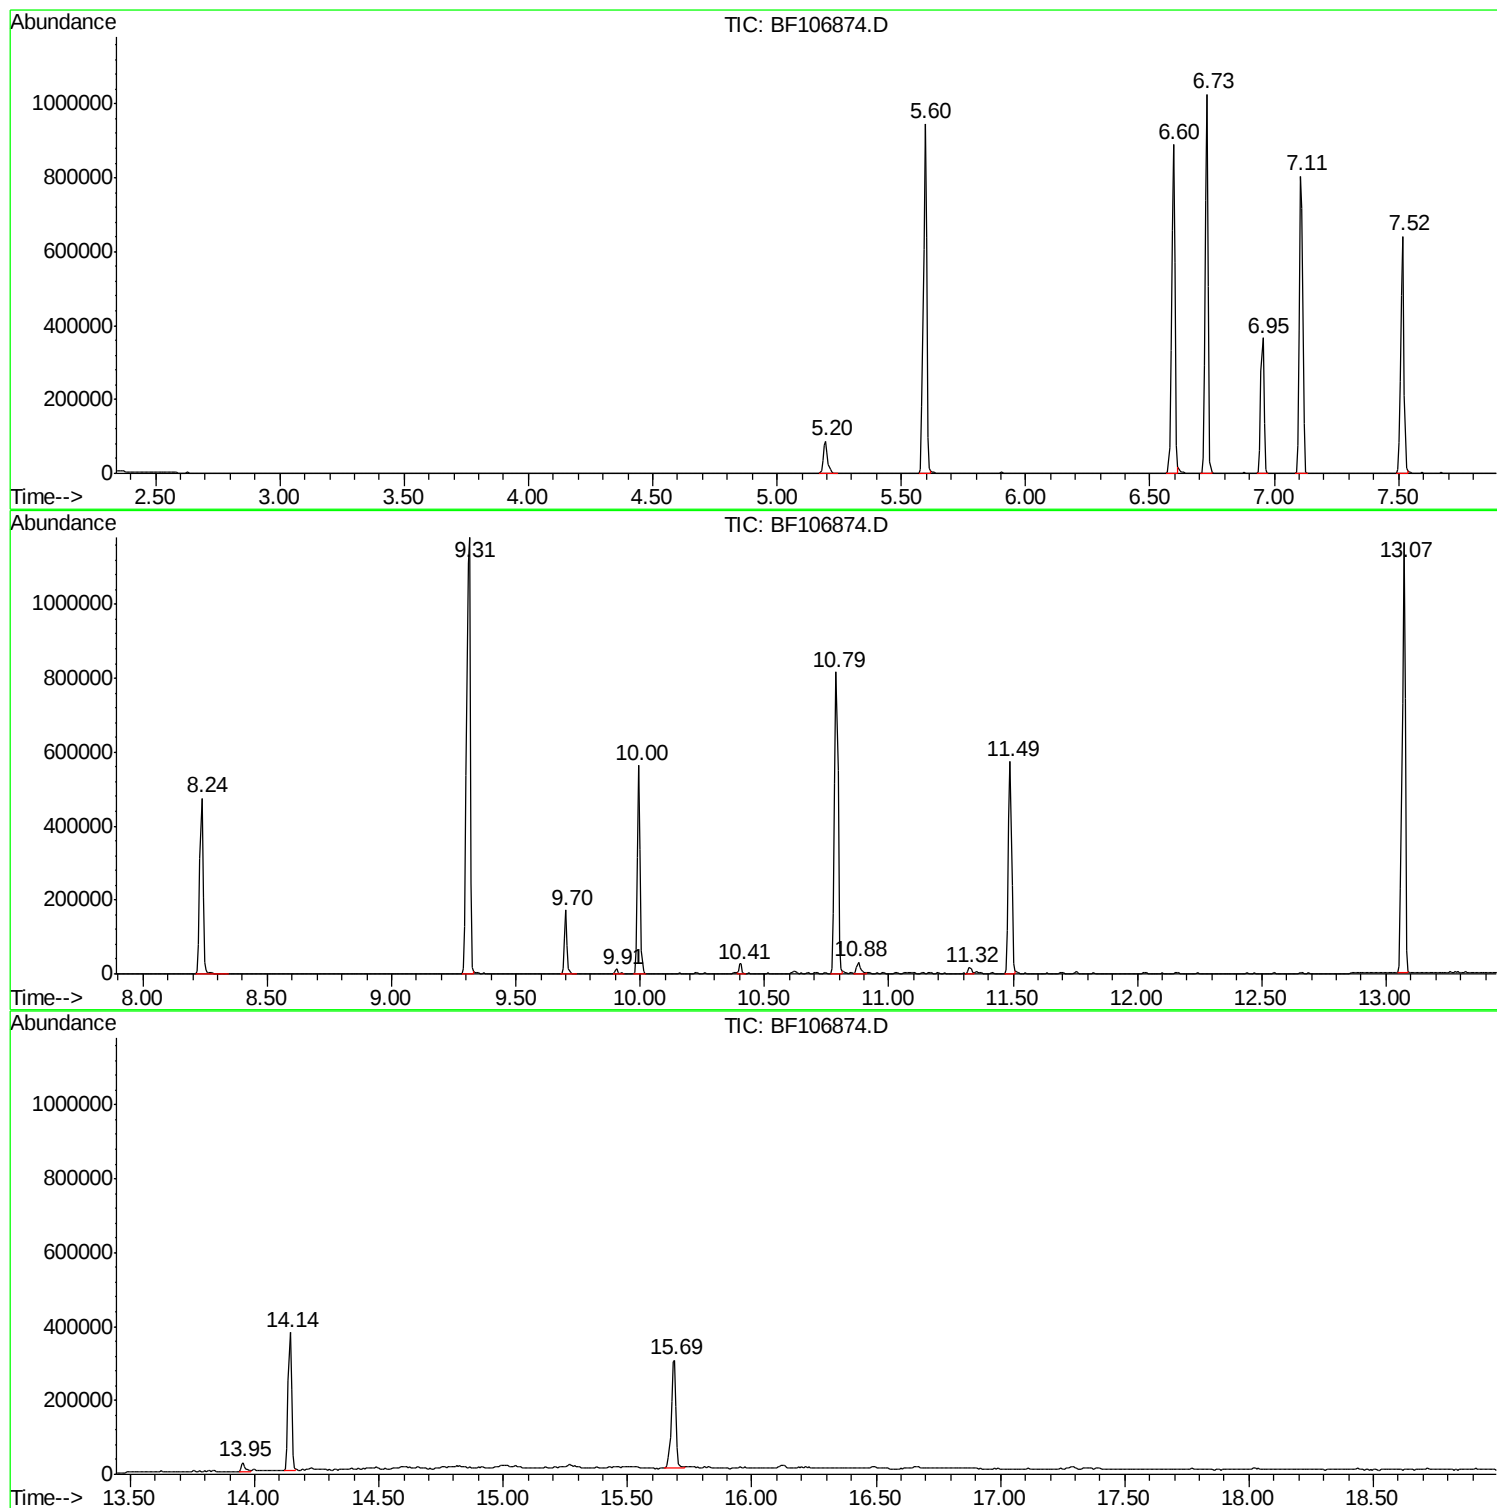

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106874.D
Acq On : 27 Jun 2018 16:16
Operator : JU/SJ
Sample : J3680-01
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-E6-F6-E6A-F6A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD		R.T.
5.20	7.07 ng	106432	1,4-Dichlorobenzene-d4		6.95
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3	5-Hexen-2-one	98	C6H10O	000109-49-9	9
4	Acetone	58	C3H6O	000067-64-1	9
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

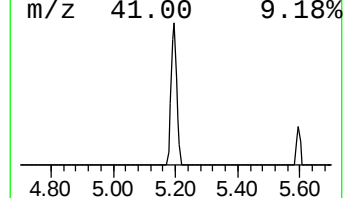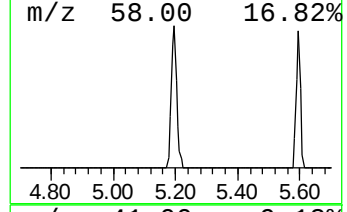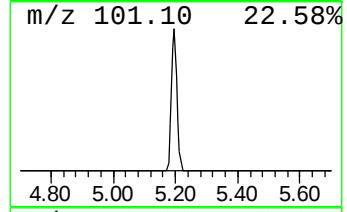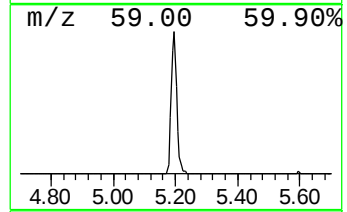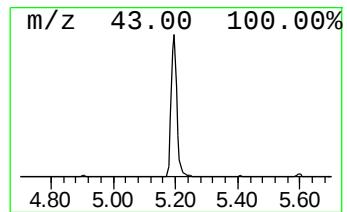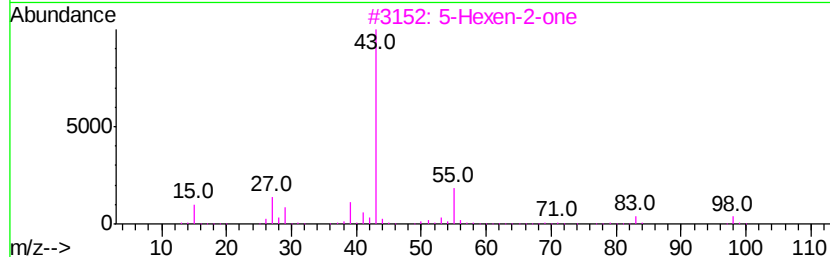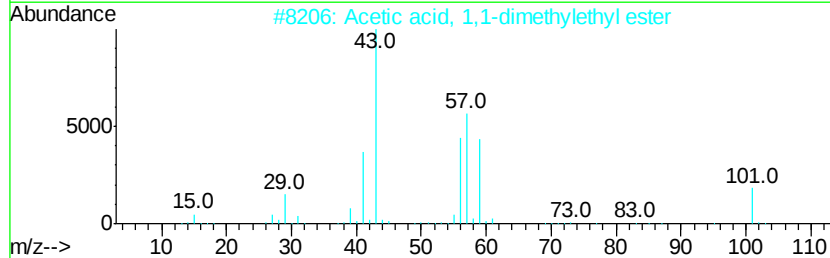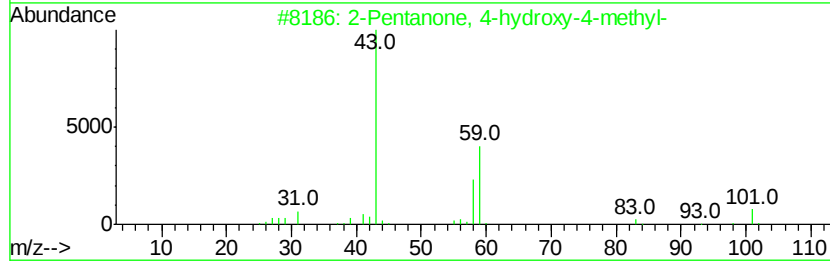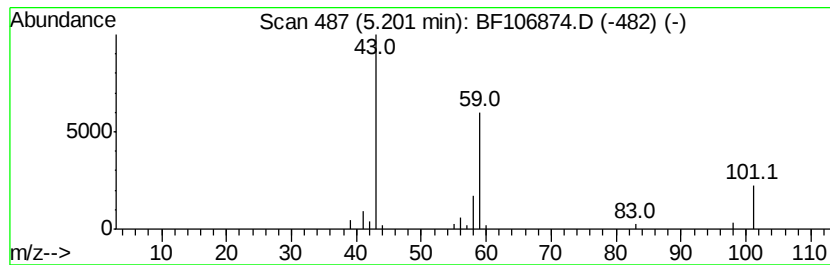

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106874.D
Acq On : 27 Jun 2018 16:16
Operator : JU/SJ
Sample : J3680-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-E6-F6-E6A-F6A









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.73 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.73	61.87 ng	931556	1,4-Dichlorobenzene-d4	6.95

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pvrazine	132	C4H2ClFN2	1000146-10-7	27		
2	5-Aminoindole	132	C8H8N2	005192-03-0	12		
3	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12		
4	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10		
5	4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9		

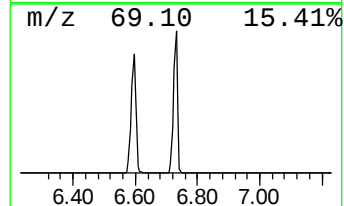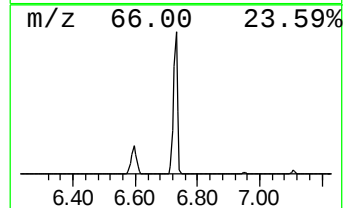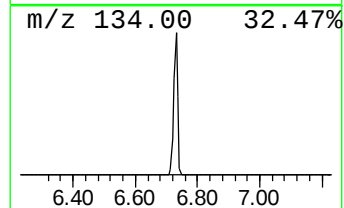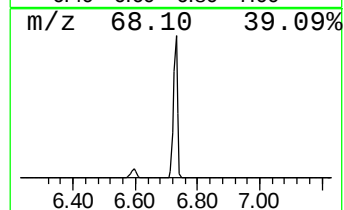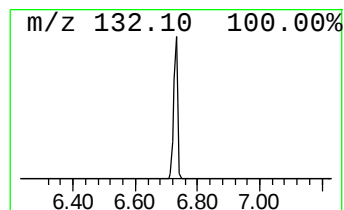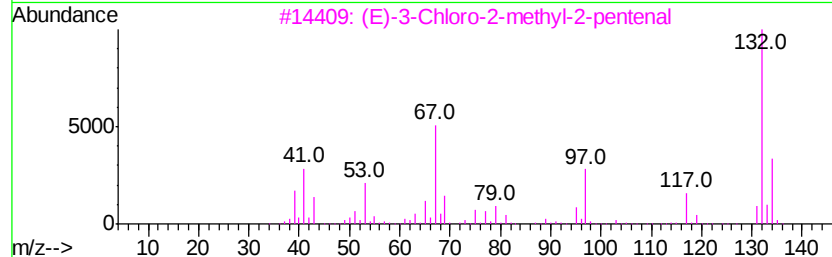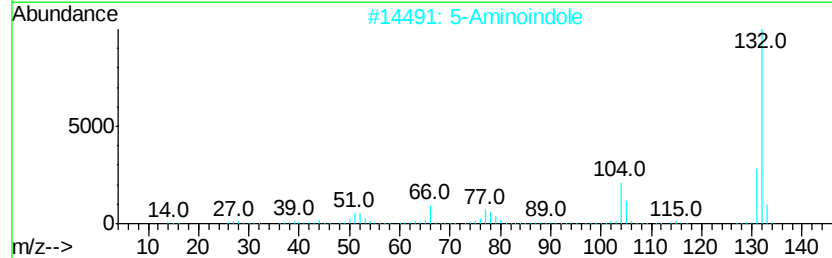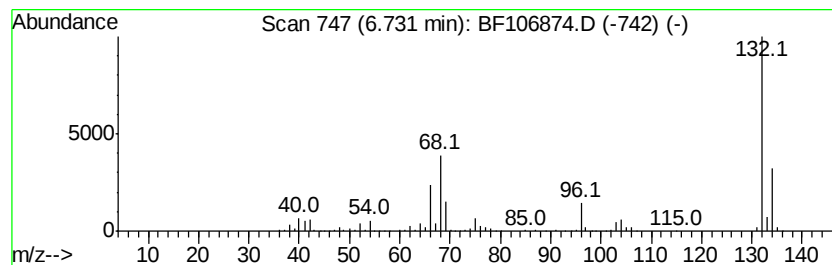

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
Data File : BF106874.D
Acq On : 27 Jun 2018 16:16
Operator : JU/SJ
Sample : J3680-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-01-E6-F6-E6A-F6A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.20	7.1	ng	106432	1	6.95	301142	20.0
unknown6.73	6.73	61.9	ng	931556	1	6.95	301142	20.0