

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106902.D
 Acq On : 28 Jun 2018 5:33
 Operator : JU/SJ
 Sample : J3719-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062518-DBRI-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.184	481	484	494	rBB	21245	25298	2.14%	0.345%
2	5.595	550	554	567	rBB	438925	393685	33.26%	5.371%
3	6.595	720	724	729	rBV	297714	269959	22.81%	3.683%
4	6.731	743	747	750	rBV	794010	664471	56.14%	9.066%
5	6.954	781	785	788	rBV	324343	250384	21.16%	3.416%
6	7.113	807	812	815	rBV	1027868	905851	76.54%	12.360%
7	7.525	876	882	885	rBV	672281	701606	59.28%	9.573%
8	8.236	999	1003	1016	rBV	325081	283218	23.93%	3.864%
9	9.313	1181	1186	1189	rBV	1288727	1183555	100.00%	16.149%
10	9.701	1249	1252	1257	rBB	16077	14900	1.26%	0.203%
11	9.995	1299	1302	1310	rVB	296257	261707	22.11%	3.571%
12	10.654	1411	1414	1417	rBV	88751	64796	5.47%	0.884%
13	10.789	1433	1437	1446	rBV	446248	401043	33.88%	5.472%
14	11.489	1552	1556	1563	rBV	270057	231910	19.59%	3.164%
15	13.071	1821	1825	1828	rBV	1194487	1115245	94.23%	15.217%
16	13.948	1971	1974	1980	rBV	30527	29616	2.50%	0.404%
17	14.136	2002	2006	2013	rBV	344520	313194	26.46%	4.273%
18	15.671	2259	2267	2275	rBV	158650	218714	18.48%	2.984%


Sum of corrected areas: 7329152

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106902.D
Acq On : 28 Jun 2018 5:33
Operator : JU/SJ
Sample : J3719-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

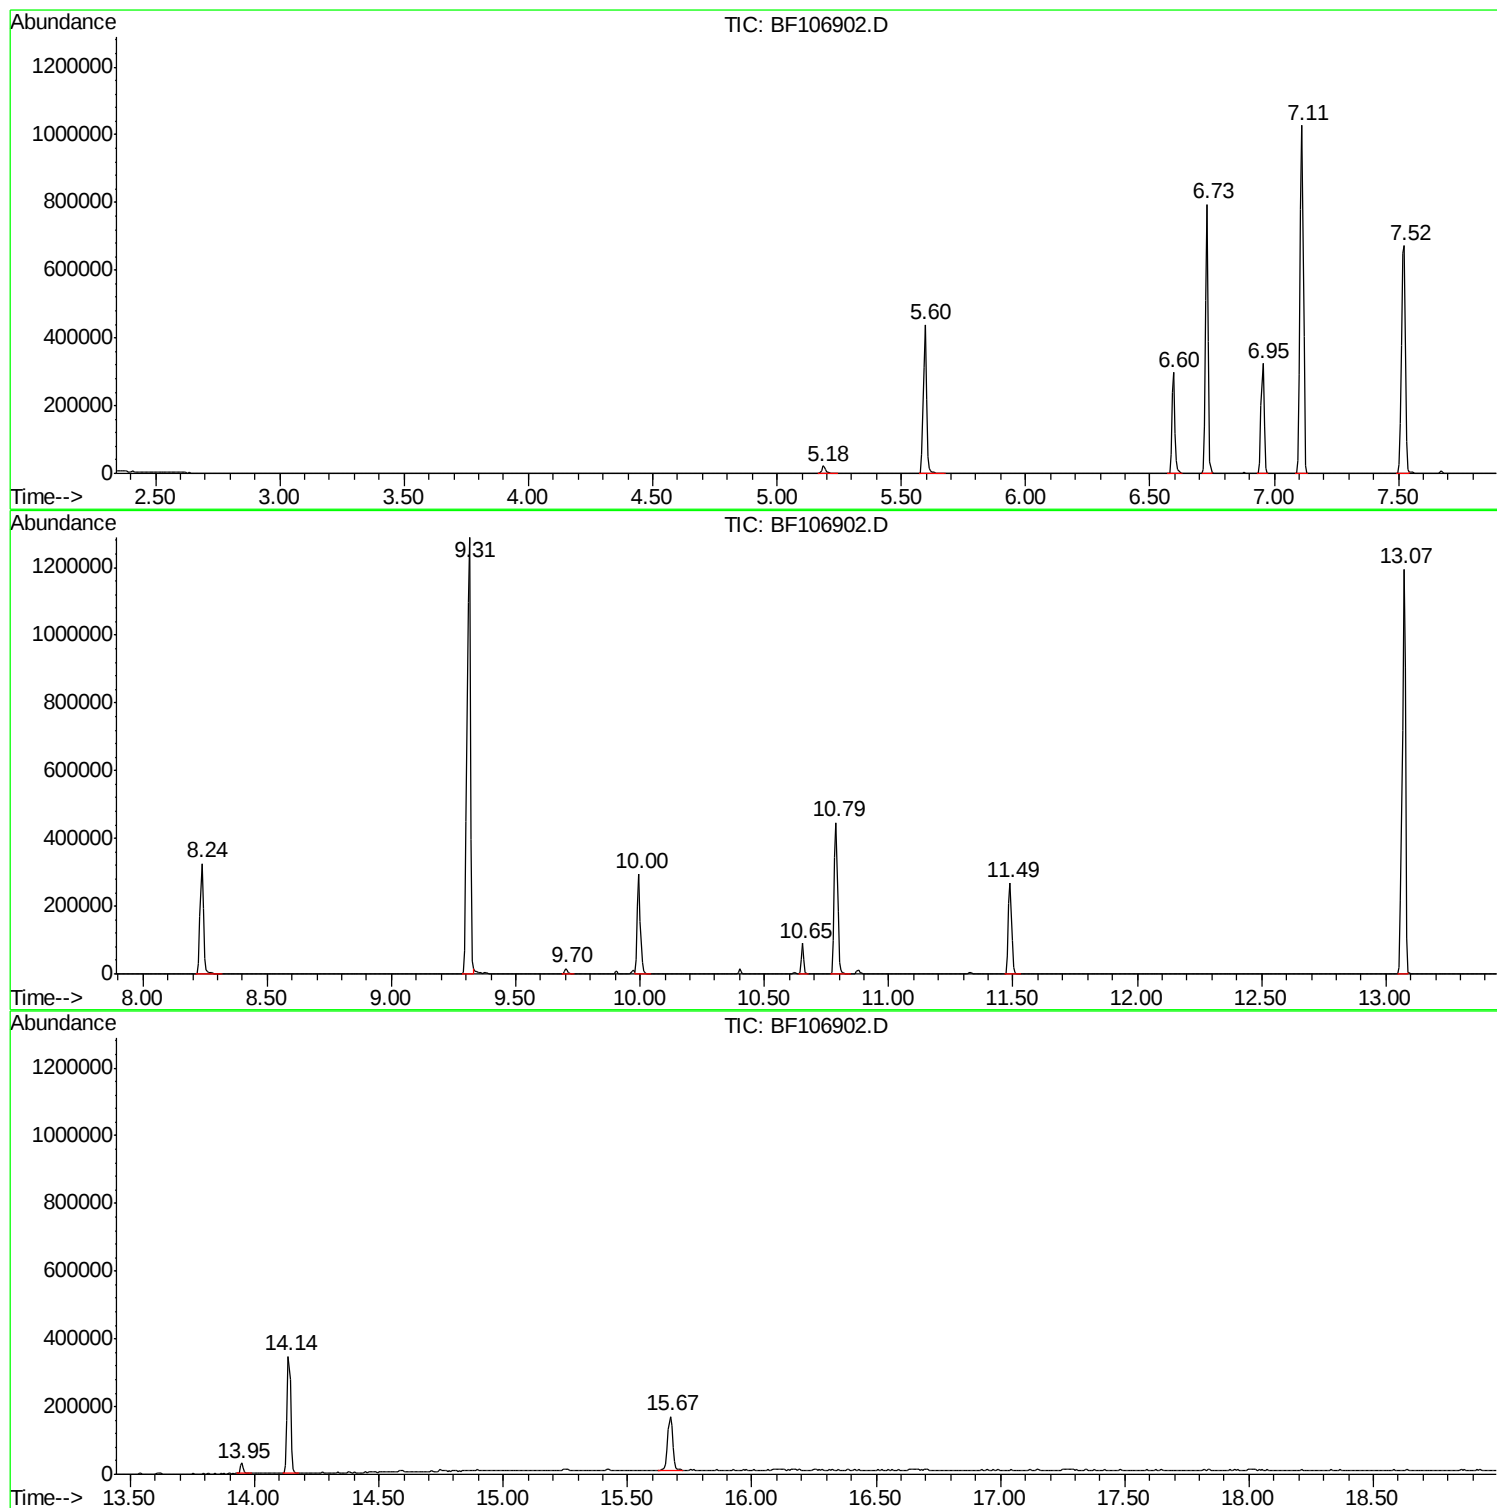

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
Data_File : BF106902.D
Acq_On : 28-Jun-2018 5:333
Operator : JU/SJJ
Sample : J3719-011
Misc :
ALS_Vial : 39 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
