

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106903.D
 Acq On : 28 Jun 2018 5:59
 Operator : JU/SJ
 Sample : J3719-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062518-DBRI-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.184	482	484	491	rBV	18275	20844	1.77%	0.288%
2	5.596	550	554	567	rBB	424917	374483	31.86%	5.172%
3	6.595	720	724	734	rBB	270559	259543	22.08%	3.585%
4	6.731	743	747	750	rBV	766464	653934	55.63%	9.031%
5	6.954	781	785	788	rBV	316653	249721	21.24%	3.449%
6	7.113	807	812	815	rBV	990409	899092	76.48%	12.417%
7	7.519	876	881	884	rBV	637621	698596	59.43%	9.648%
8	8.237	999	1003	1021	rBB	338968	287213	24.43%	3.967%
9	9.313	1181	1186	1189	rBV	1291264	1175537	100.00%	16.235%
10	9.701	1249	1252	1258	rBB	23279	20136	1.71%	0.278%
11	9.995	1299	1302	1309	rVB	307668	266520	22.67%	3.681%
12	10.654	1411	1414	1417	rBV	88249	61644	5.24%	0.851%
13	10.789	1433	1437	1446	rBV	471559	408388	34.74%	5.640%
14	11.489	1552	1556	1567	rBB	269055	239100	20.34%	3.302%
15	13.072	1821	1825	1828	rBV	1207509	1103107	93.84%	15.235%
16	14.136	2002	2006	2015	rBV	335502	307830	26.19%	4.251%
17	15.671	2260	2267	2274	rBV	161887	214988	18.29%	2.969%


Sum of corrected areas: 7240676

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106903.D
Acq On : 28 Jun 2018 5:59
Operator : JU/SJ
Sample : J3719-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

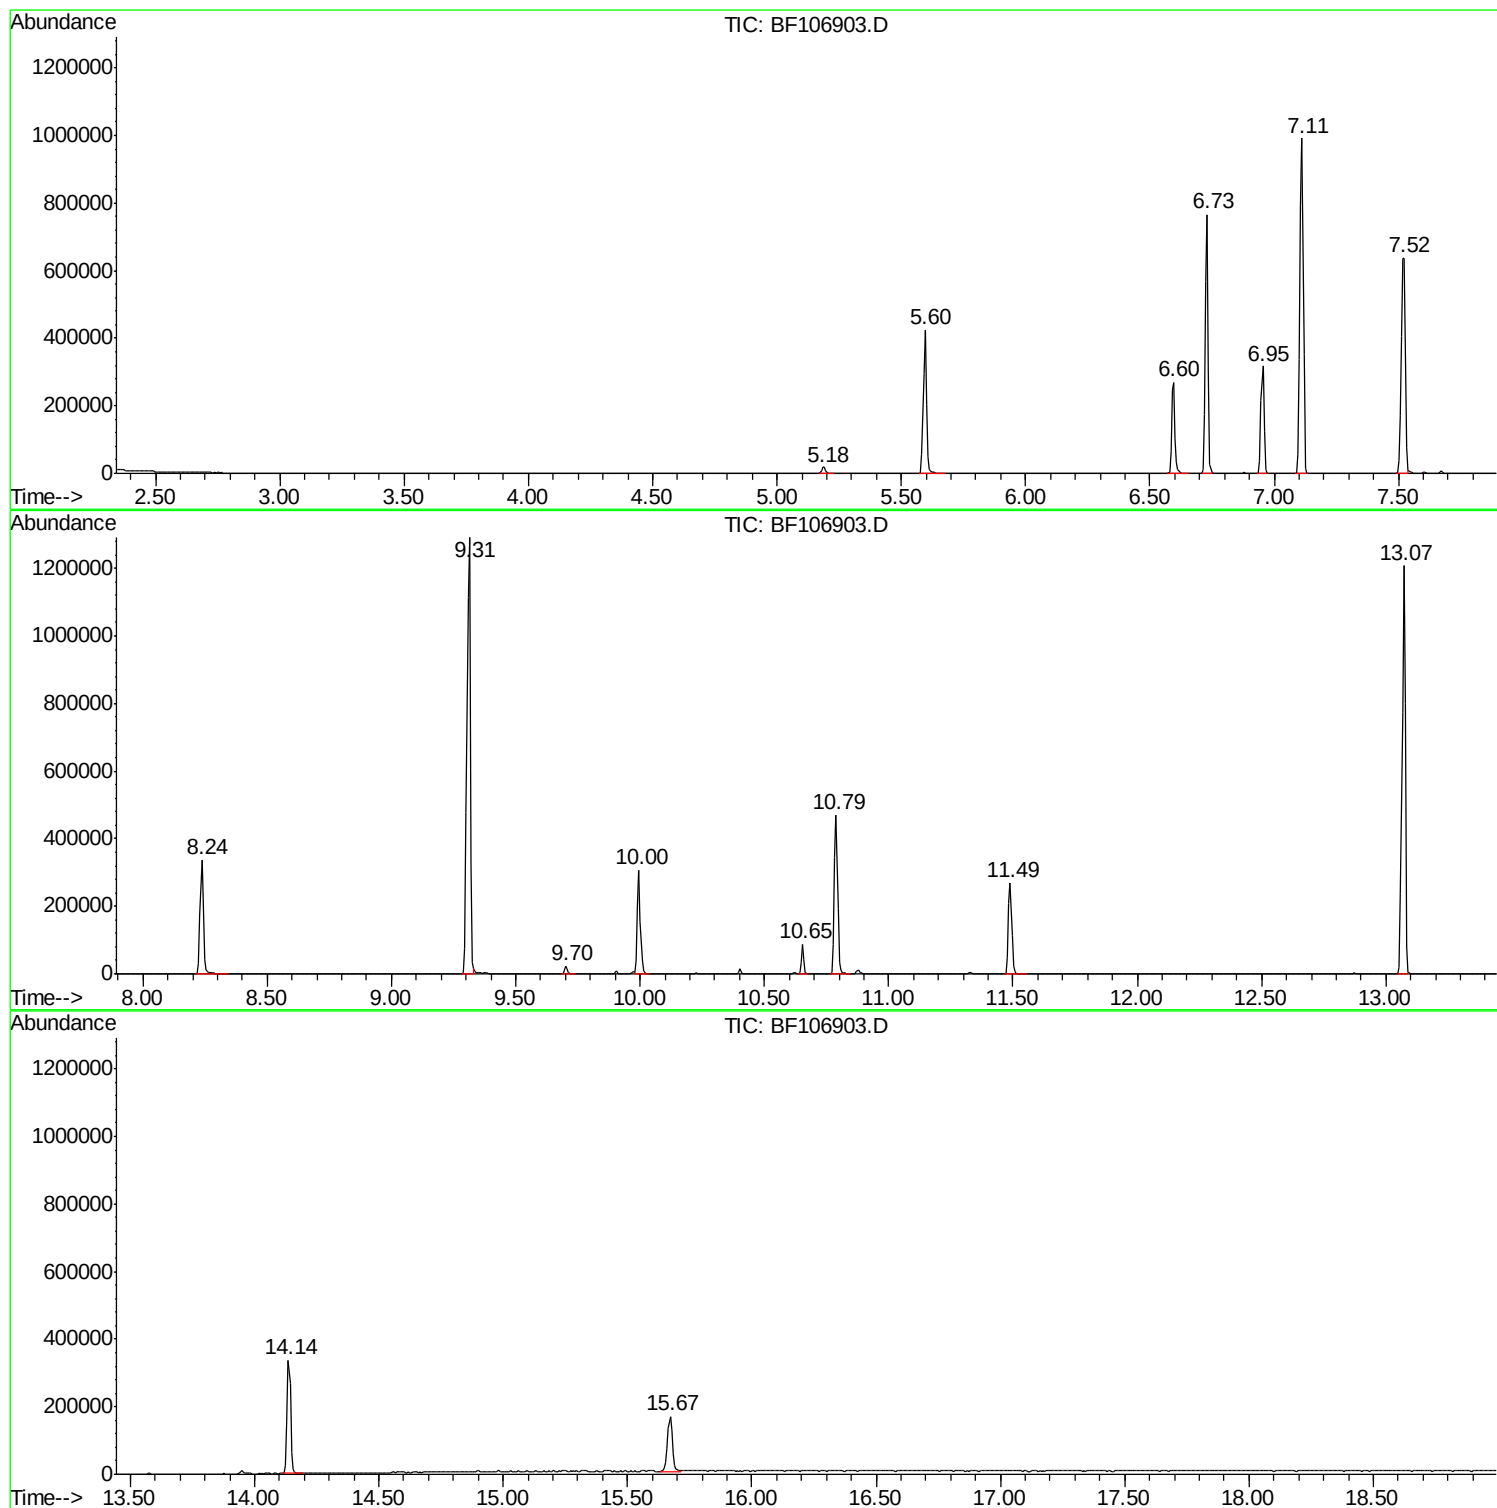

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
Data_File : BF106903.D
Acq_On : 28-Jun-2018 5:59
Operator : JU/SJJ
Sample : J3719-022
Misc :
ALS_Vial : 40 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-D-M

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
