

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106904.D
 Acq On : 28 Jun 2018 6:26
 Operator : JU/SJ
 Sample : J3719-03
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062518-DBRI-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.184	481	484	493	rBB	17806	18550	1.53%	0.252%
2	5.590	550	553	566	rBB	356107	352194	29.00%	4.781%
3	6.590	720	723	735	rBB	228827	233191	19.20%	3.166%
4	6.731	743	747	750	rBV	733430	628073	51.71%	8.526%
5	6.954	781	785	788	rBV	322518	257169	21.17%	3.491%
6	7.113	807	812	815	rBV	1010439	905274	74.53%	12.289%
7	7.519	876	881	884	rBV	659314	702952	57.87%	9.543%
8	8.237	999	1003	1017	rBV	353898	303745	25.01%	4.123%
9	9.313	1181	1186	1189	rBV	1338944	1214636	100.00%	16.489%
10	9.701	1249	1252	1259	rBB	35423	30815	2.54%	0.418%
11	9.995	1299	1302	1311	rVB	344208	294013	24.21%	3.991%
12	10.401	1369	1371	1374	rVB	17144	13065	1.08%	0.177%
13	10.654	1411	1414	1417	rBV	92056	66218	5.45%	0.899%
14	10.789	1433	1437	1446	rBV	467880	424930	34.98%	5.768%
15	10.878	1449	1452	1461	rVB	14520	15681	1.29%	0.213%
16	11.489	1552	1556	1564	rBV	286156	259258	21.34%	3.519%
17	13.072	1821	1825	1828	rBV	1206699	1115898	91.87%	15.148%
18	14.136	2002	2006	2013	rBV	352260	312098	25.69%	4.237%
19	15.665	2260	2266	2277	rVB	158414	218658	18.00%	2.968%


Sum of corrected areas: 7366418

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106904.D
Acq On : 28 Jun 2018 6:26
Operator : JU/SJ
Sample : J3719-03
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

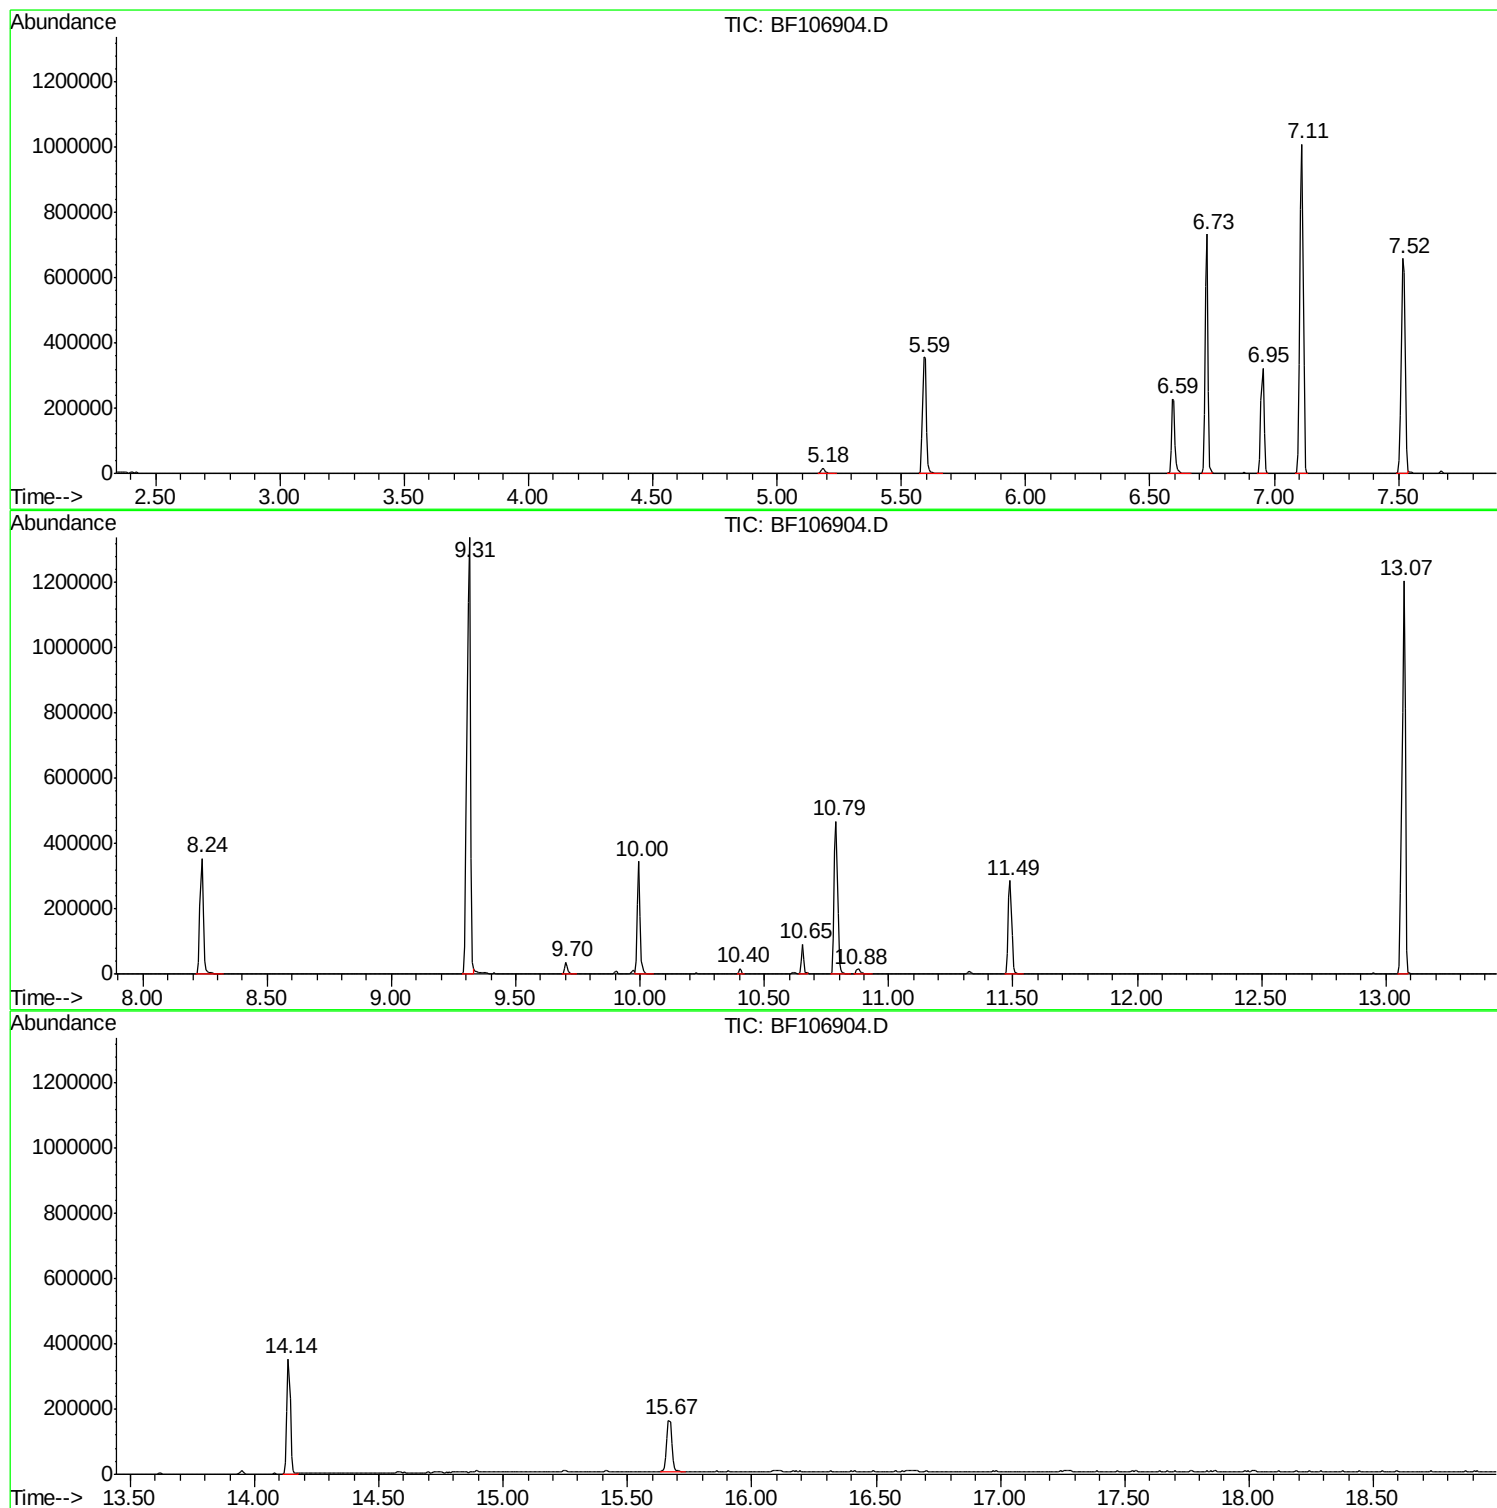

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
Data_File : BF106904.D
Acq_On : 28_Jun_2018_ 6:266
Operator : JU/SJJ
Sample : J3719-033
Misc :
ALS_Vial : 41_ Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-D-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
