

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106906.D
 Acq On : 28 Jun 2018 7:18
 Operator : JU/SJ
 Sample : J3719-05
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062518-DBRI-F-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.184	481	484	493	rBB	20520	21066	1.79%	0.292%
2	5.590	550	553	568	rBB	362615	356965	30.25%	4.949%
3	6.589	720	723	732	rBV	280053	257331	21.81%	3.568%
4	6.731	743	747	750	rBV	738190	622323	52.73%	8.628%
5	6.954	781	785	788	rBV	312546	246159	20.86%	3.413%
6	7.113	807	812	815	rBV	948373	864871	73.29%	11.990%
7	7.519	876	881	884	rBV	650180	676194	57.30%	9.375%
8	8.236	999	1003	1017	rBV	343432	290448	24.61%	4.027%
9	9.313	1181	1186	1189	rBV	1278679	1180109	100.00%	16.361%
10	9.701	1249	1252	1258	rBB	21050	18573	1.57%	0.257%
11	9.995	1299	1302	1309	rVB	314425	278663	23.61%	3.863%
12	10.654	1411	1414	1417	rBV	82391	60725	5.15%	0.842%
13	10.789	1433	1437	1448	rBB	443275	413521	35.04%	5.733%
14	11.489	1552	1556	1564	rBV	276870	242326	20.53%	3.360%
15	13.071	1821	1825	1828	rBV	1179017	1106678	93.78%	15.343%
16	13.948	1970	1974	1981	rBV	30055	32081	2.72%	0.445%
17	14.136	2003	2006	2012	rVB	307588	302343	25.62%	4.192%
18	14.983	2146	2150	2154	rVB	41065	38126	3.23%	0.529%
19	15.677	2262	2268	2274	rBV2	150726	204565	17.33%	2.836%


Sum of corrected areas: 7213067

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106906.D
Acq On : 28 Jun 2018 7:18
Operator : JU/SJ
Sample : J3719-05
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

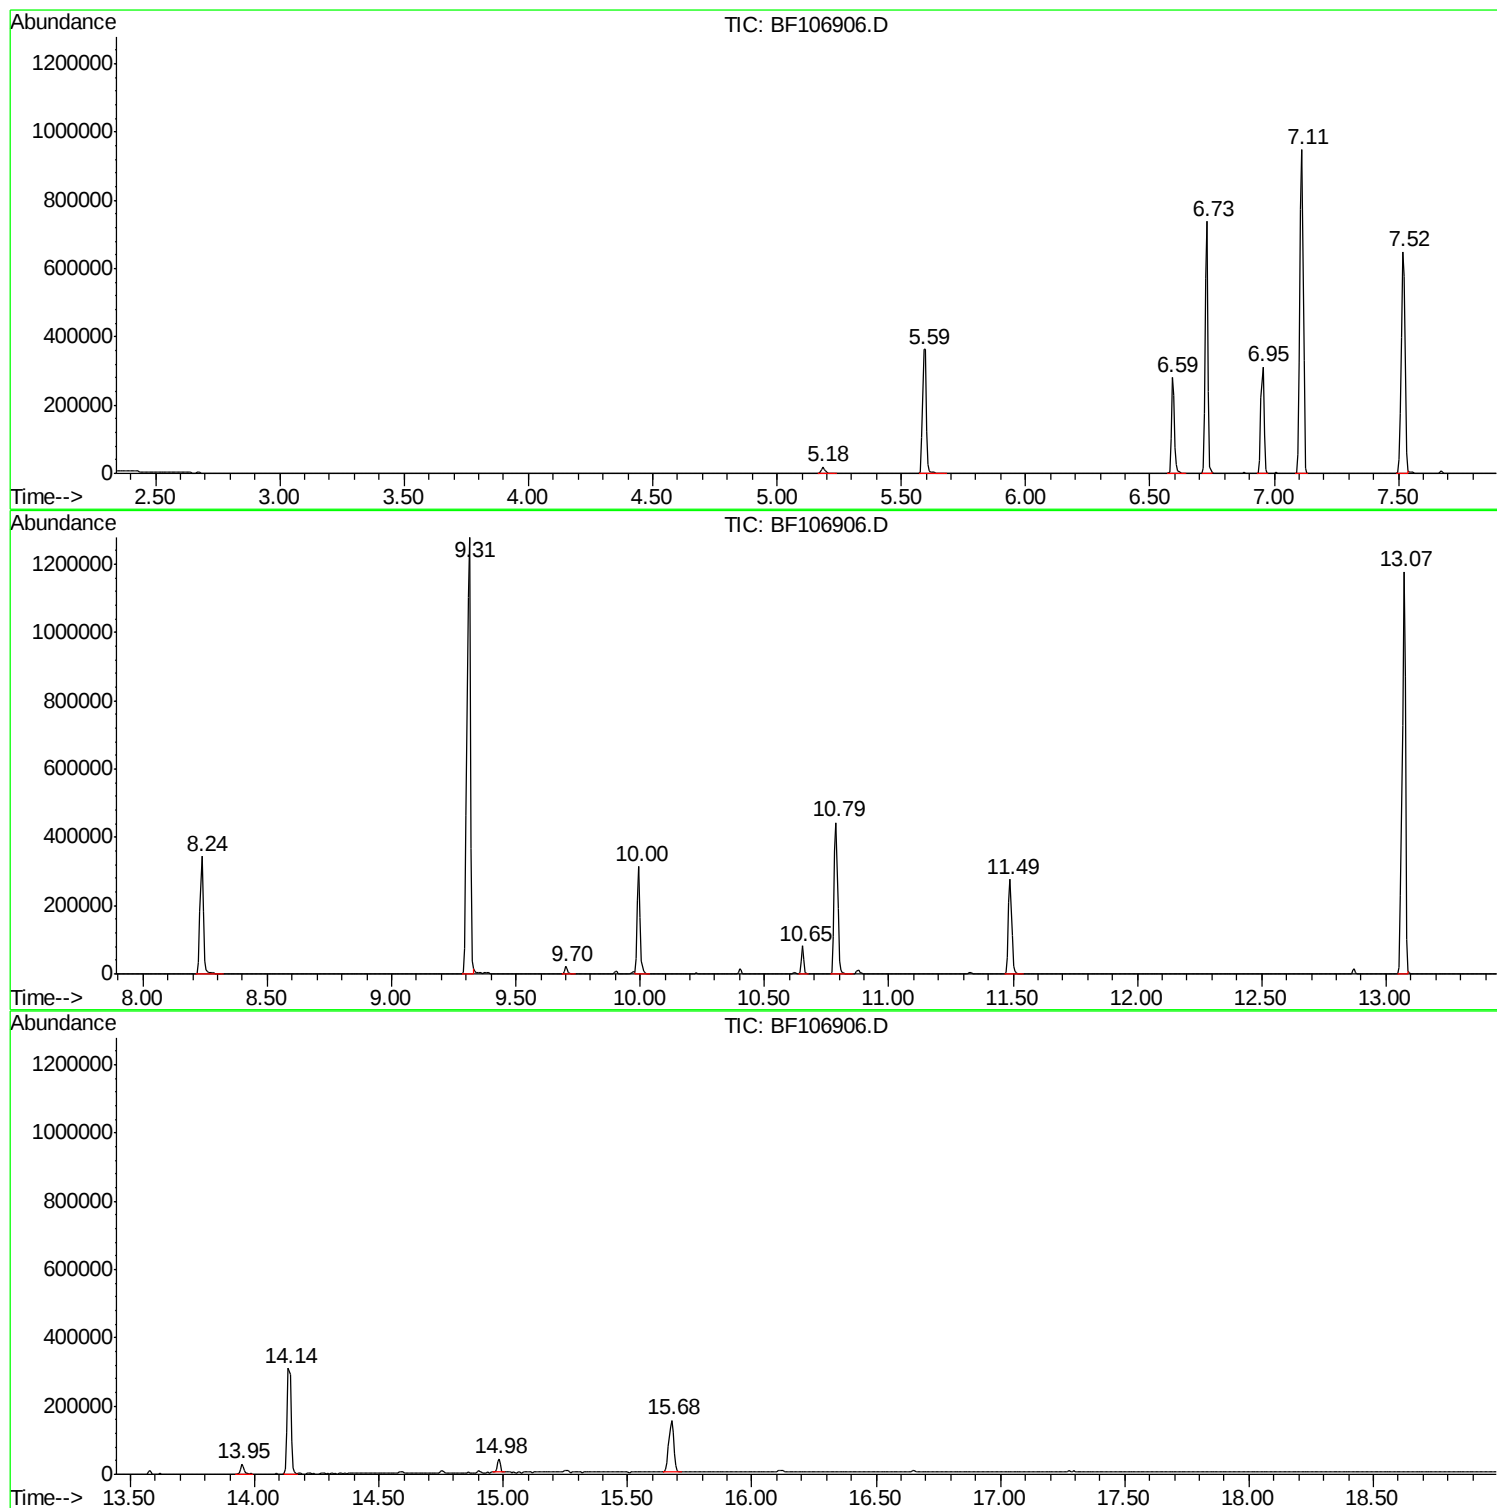

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
Data_File : BF106906.D
Acq_On : 28-Jun-2018 7:188
Operator : JU/SJJ
Sample : J3719-055
Misc :
ALS_Vial : 43 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-U-M

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
