

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106907.D
 Acq On : 28 Jun 2018 7:45
 Operator : JU/SJ
 Sample : J3719-06
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062518-DBRI-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.184	481	484	492	rBB	23709	24235	2.08%	0.339%
2	5.595	550	554	566	rBB	336967	334129	28.63%	4.679%
3	6.589	720	723	734	rBB	239865	216805	18.58%	3.036%
4	6.731	743	747	750	rBV	676885	609466	52.22%	8.535%
5	6.954	781	785	788	rBV	323621	259012	22.19%	3.627%
6	7.113	807	812	815	rBV	955331	863720	74.01%	12.095%
7	7.519	876	881	884	rBV	654730	676943	58.00%	9.480%
8	8.236	999	1003	1017	rBV	354772	302717	25.94%	4.239%
9	9.313	1181	1186	1189	rBV	1221568	1167089	100.00%	16.344%
10	9.701	1249	1252	1257	rBB	19930	17990	1.54%	0.252%
11	9.995	1299	1302	1310	rVB	331847	290817	24.92%	4.073%
12	10.654	1411	1414	1417	rBV	96700	67907	5.82%	0.951%
13	10.789	1433	1437	1447	rBB	430550	408843	35.03%	5.725%
14	11.489	1552	1556	1565	rBV	272849	260426	22.31%	3.647%
15	13.071	1821	1825	1828	rBV	1158845	1077716	92.34%	15.092%
16	13.948	1971	1974	1981	rBV	23531	25832	2.21%	0.362%
17	14.136	2002	2006	2012	rBV	341906	313573	26.87%	4.391%
18	15.671	2258	2267	2277	rBV	163123	223725	19.17%	3.133%


Sum of corrected areas: 7140945

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106907.D
Acq On : 28 Jun 2018 7:45
Operator : JU/SJ
Sample : J3719-06
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

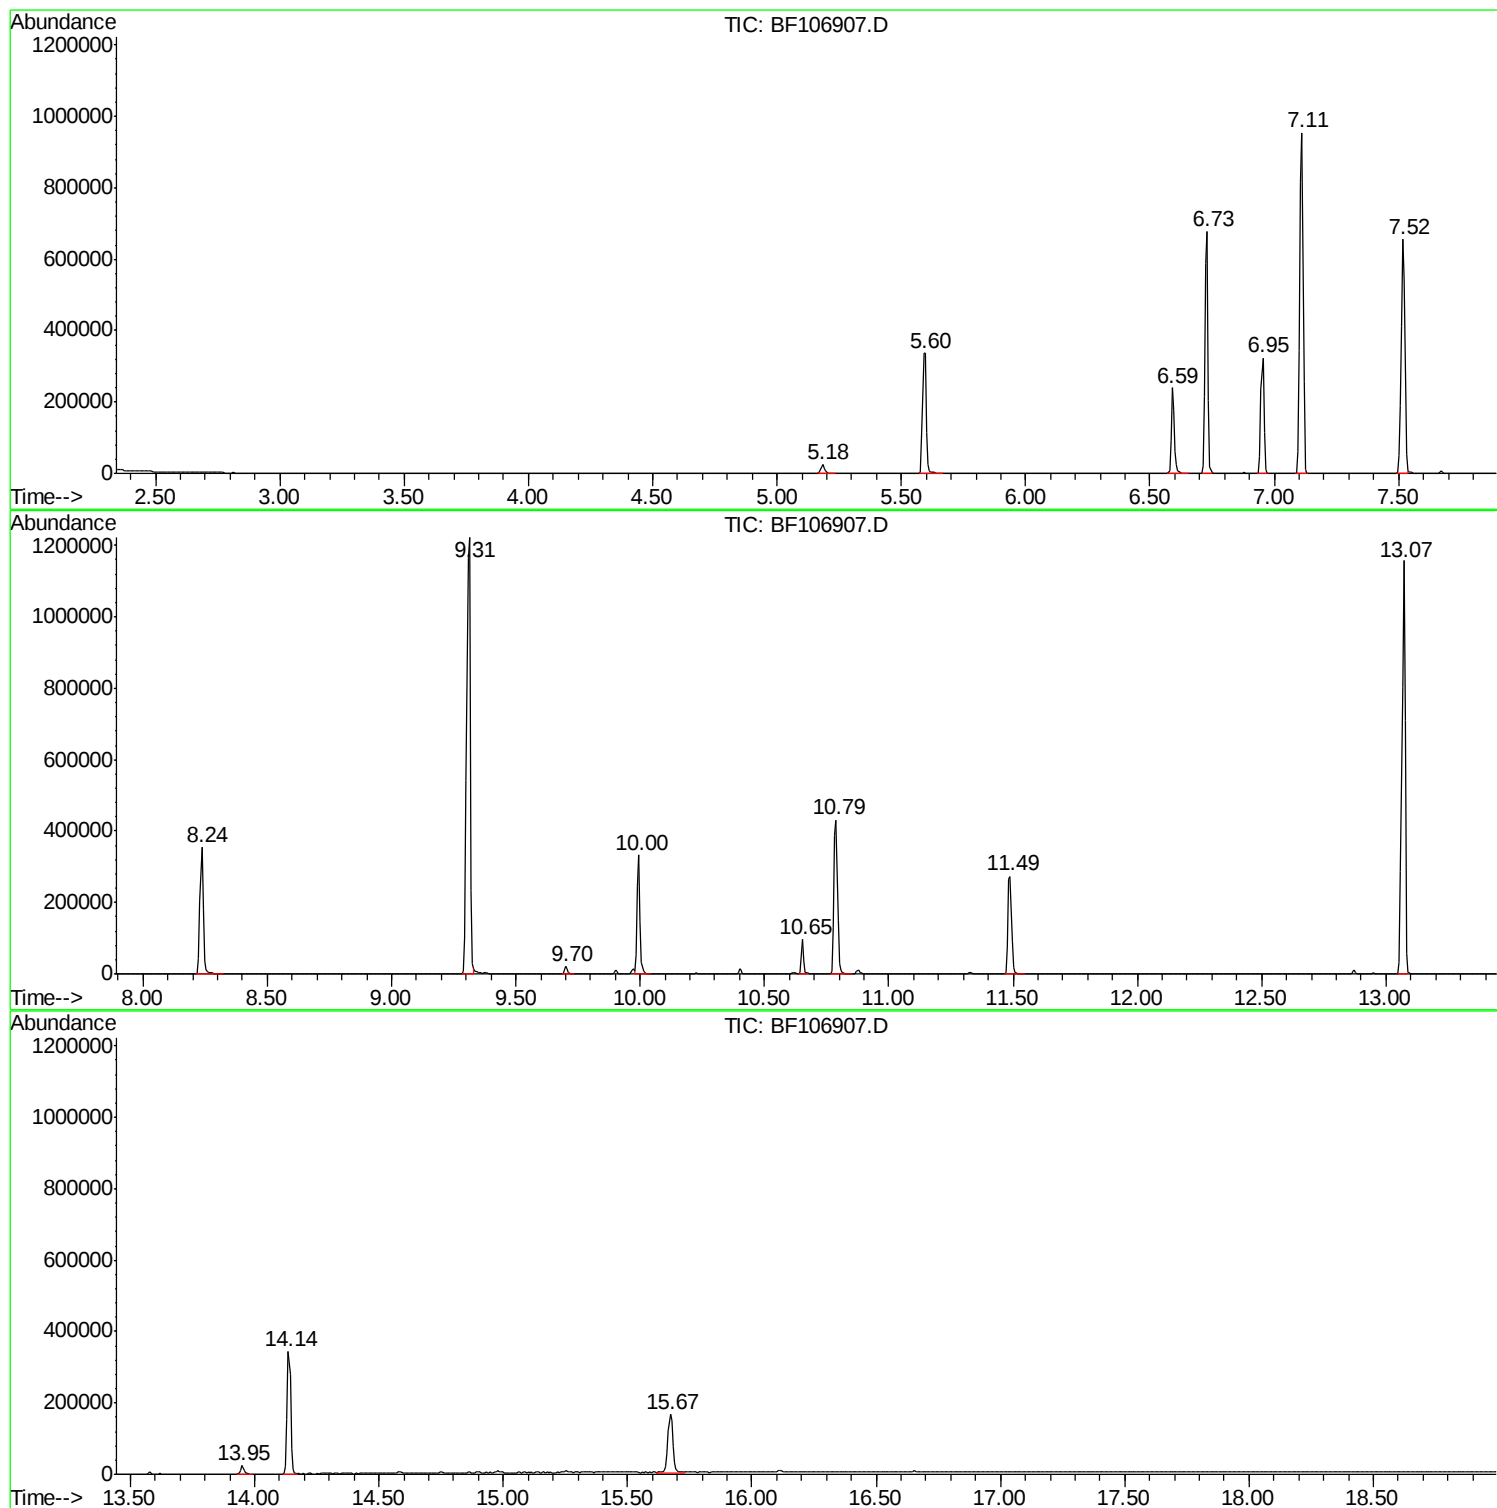

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
Data_File : BF106907.D
Acq_On : 28-Jun-2018 7:455
Operator : JU/SJJ
Sample : J3719-066
Misc :
ALS_Vial : 44 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
062518-DBRI-F-U-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
