

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106908.D
 Acq On : 28 Jun 2018 8:11
 Operator : JU/SJ
 Sample : J3719-07
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 062518-TIPC-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.184	481	484	491	rBB	19049	19763	1.65%	0.274%
2	5.590	550	553	561	rBV	358611	332719	27.76%	4.607%
3	6.590	720	723	730	rBV	248953	221106	18.45%	3.061%
4	6.731	743	747	750	rBV	681826	609144	50.82%	8.434%
5	6.954	781	785	788	rBV	305013	248402	20.72%	3.439%
6	7.113	807	812	815	rBV	949038	876442	73.12%	12.135%
7	7.519	876	881	884	rBV	674333	681173	56.83%	9.431%
8	8.236	999	1003	1014	rBV	334158	289987	24.19%	4.015%
9	9.313	1181	1186	1189	rBV	1214651	1198609	100.00%	16.596%
10	9.701	1249	1252	1258	rBB	34359	29529	2.46%	0.409%
11	9.995	1299	1302	1311	rVB	317927	280532	23.40%	3.884%
12	10.401	1369	1371	1374	rVB	16947	12097	1.01%	0.167%
13	10.654	1411	1414	1417	rBV	211212	153938	12.84%	2.131%
14	10.789	1433	1437	1448	rBB	427259	405548	33.83%	5.615%
15	10.877	1449	1452	1456	rBV	11645	12015	1.00%	0.166%
16	11.489	1552	1556	1564	rBV	266112	245185	20.46%	3.395%
17	13.071	1821	1825	1828	rBV	1210773	1093029	91.19%	15.134%
18	14.136	2002	2006	2012	rBV	322554	303188	25.29%	4.198%
19	15.671	2260	2267	2275	rVB	159450	210024	17.52%	2.908%


Sum of corrected areas: 7222430

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062718\
Data File : BF106908.D
Acq On : 28 Jun 2018 8:11
Operator : JU/SJ
Sample : J3719-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
062518-TIPC-F-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

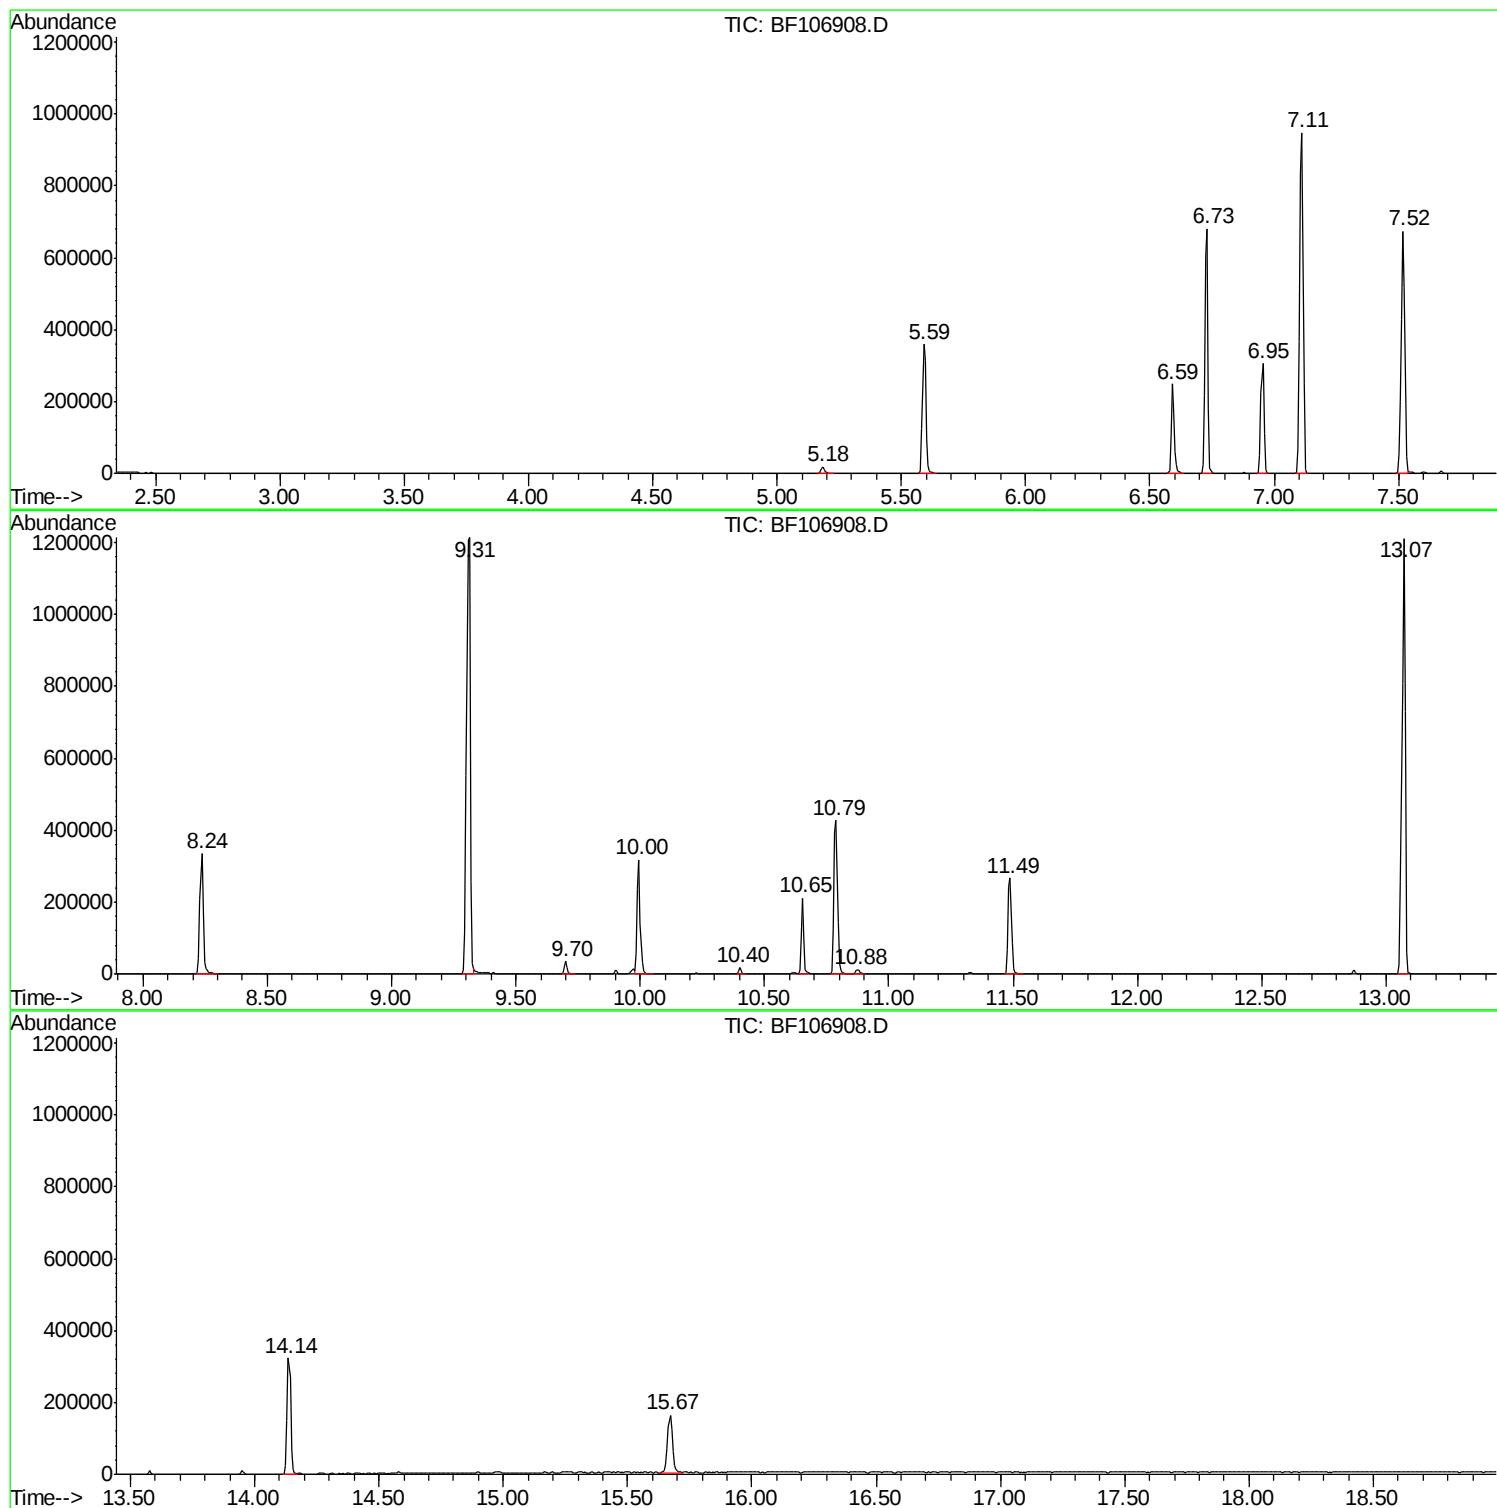

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\\
Data_File : BF106908.D
Acq_On : 28-Jun-2018 8:111
Operator : JU/SJJ
Sample : J3719-077
Misc :
ALS_Vial : 45 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
062518-TIPC-F-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
