


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106862.D
 Acq On : 27 Jun 2018 10:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 25 18:50:17 2018

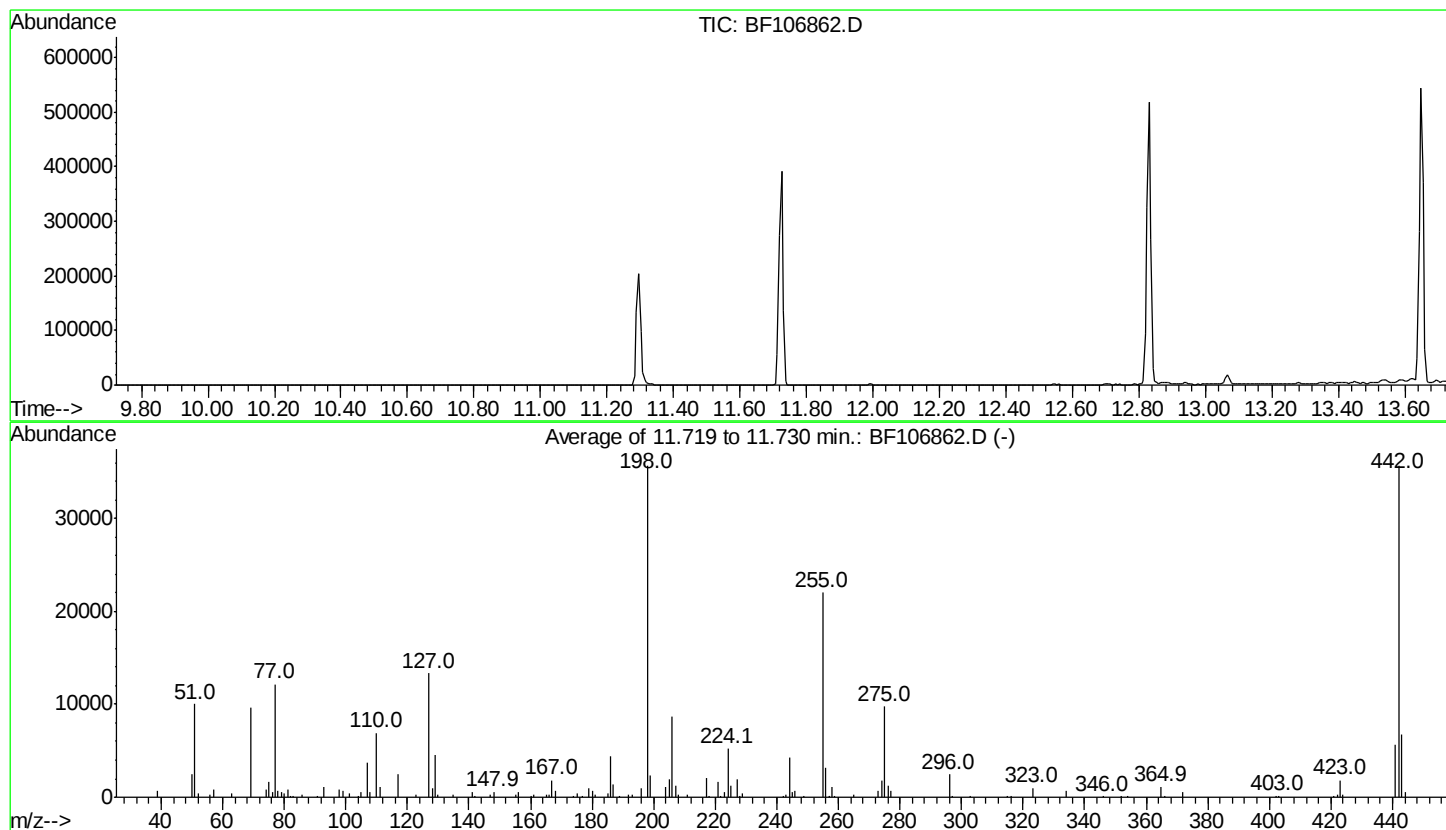

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	10017	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.1	9662	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.4	13341	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35682	PASS
199	198	5	9	6.5	2321	PASS
275	198	10	60	27.3	9752	PASS
365	198	1	100	3.3	1168	PASS
441	443	0.01	100	83.2	5626	PASS
442	198	50	100	99.9	35632	PASS
443	442	15	24	19.0	6761	PASS