


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062718\
 Data File : BF106889.D
 Acq On : 27 Jun 2018 23:45
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 25 18:50:17 2018

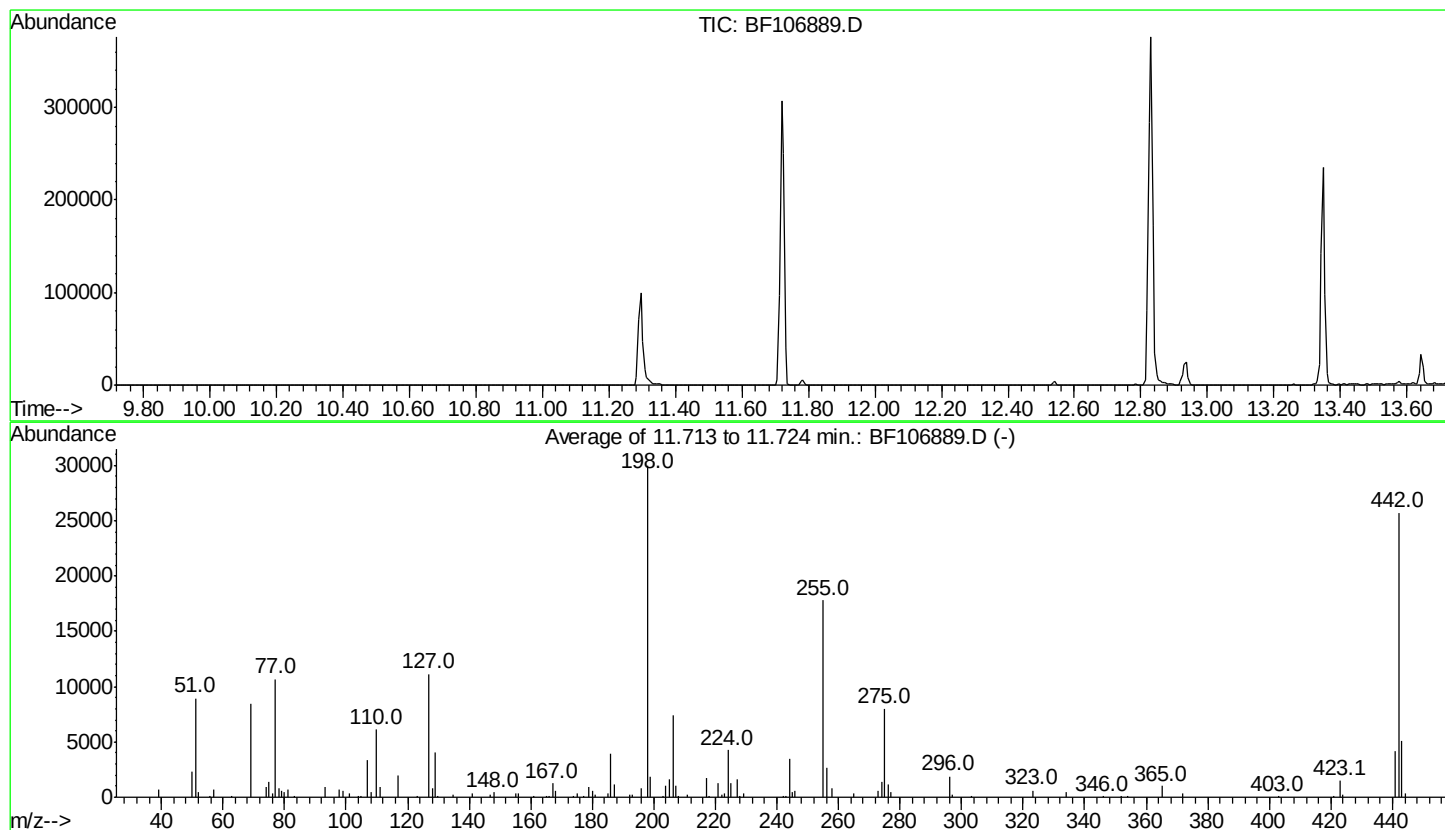

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	8923	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.1	8418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.1	11108	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29973	PASS
199	198	5	9	6.3	1892	PASS
275	198	10	60	26.8	8024	PASS
365	198	1	100	3.3	996	PASS
441	443	0.01	100	83.0	4199	PASS
442	198	50	100	85.7	25695	PASS
443	442	15	24	19.7	5062	PASS