
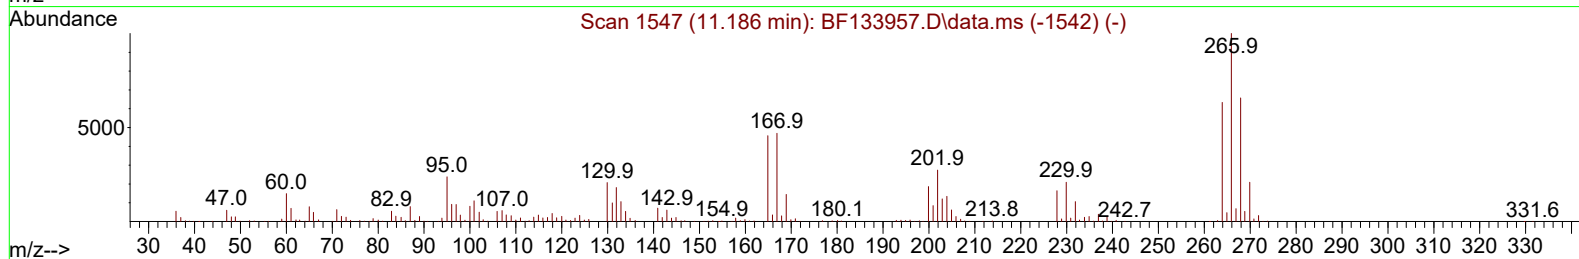
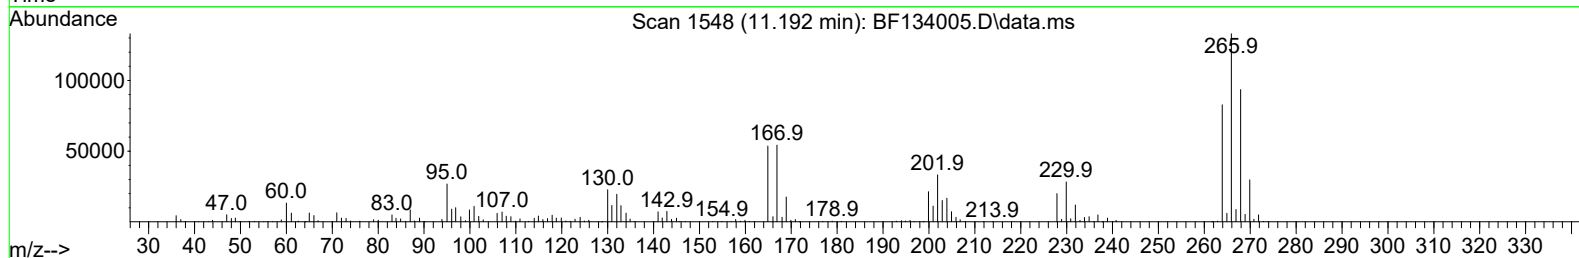


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF134005.D
Acq On : 28 Jun 2023 00:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:32:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

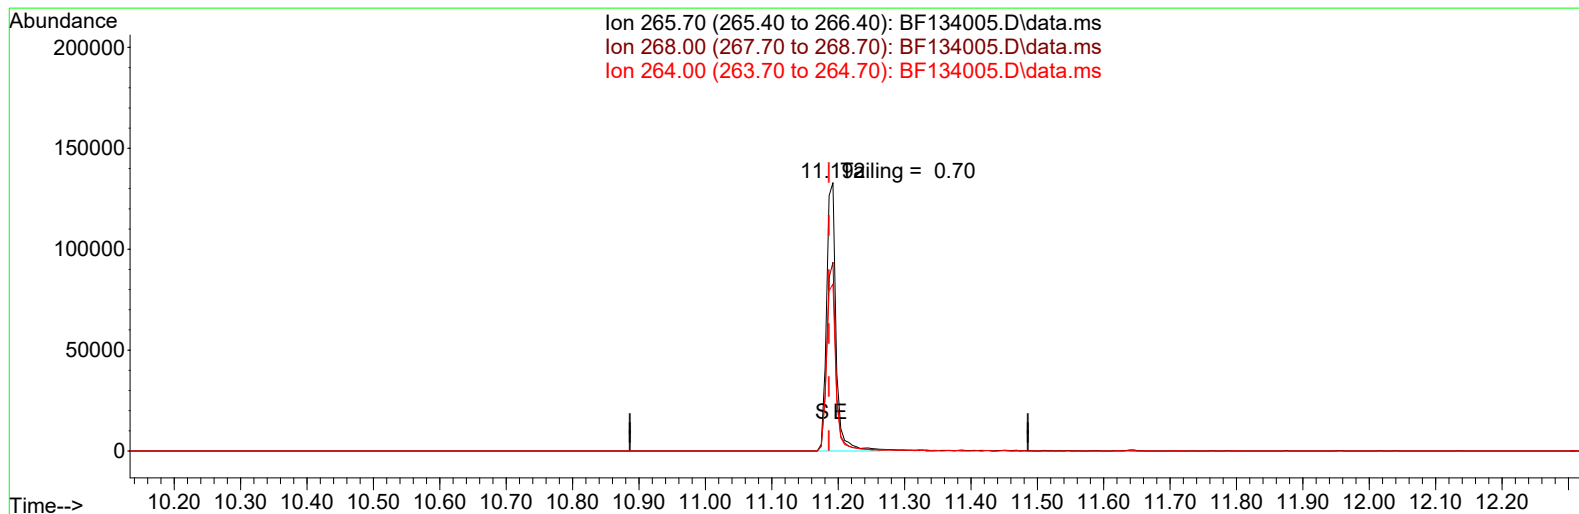

TIC: BF134005.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.006) 22292.73 ng

response 134479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	70.30
264.00	63.30	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF134005.D
Acq On : 28 Jun 2023 00:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:32:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

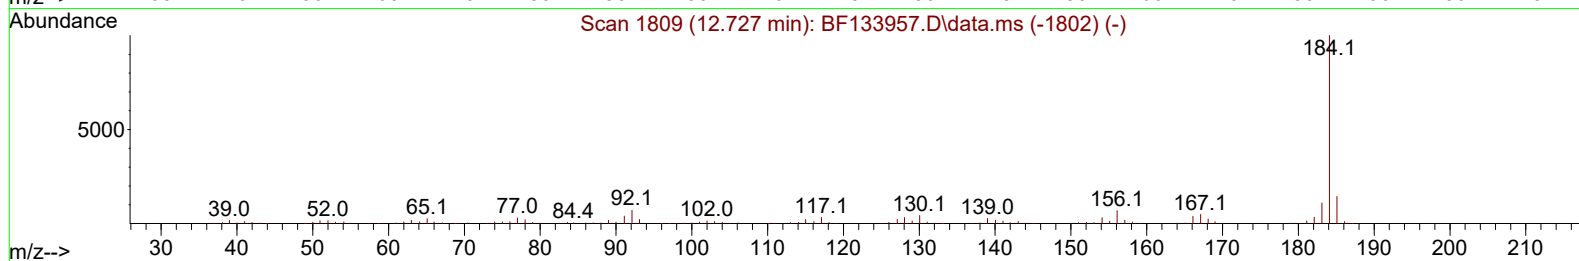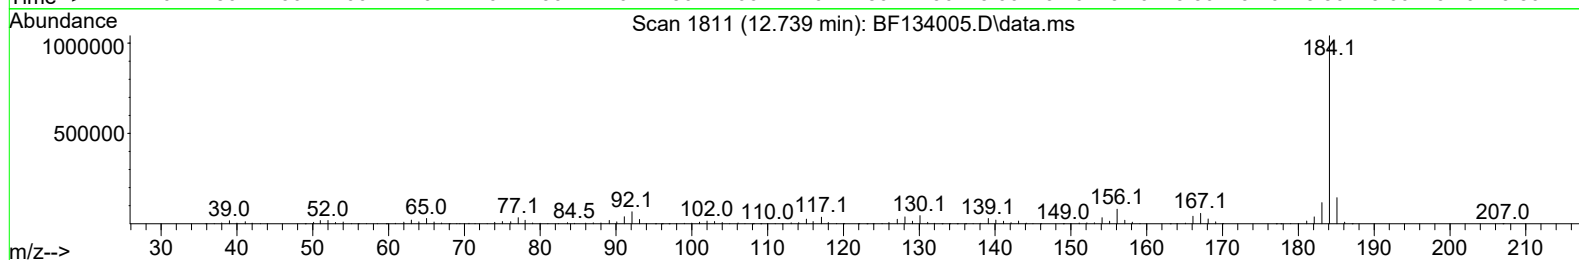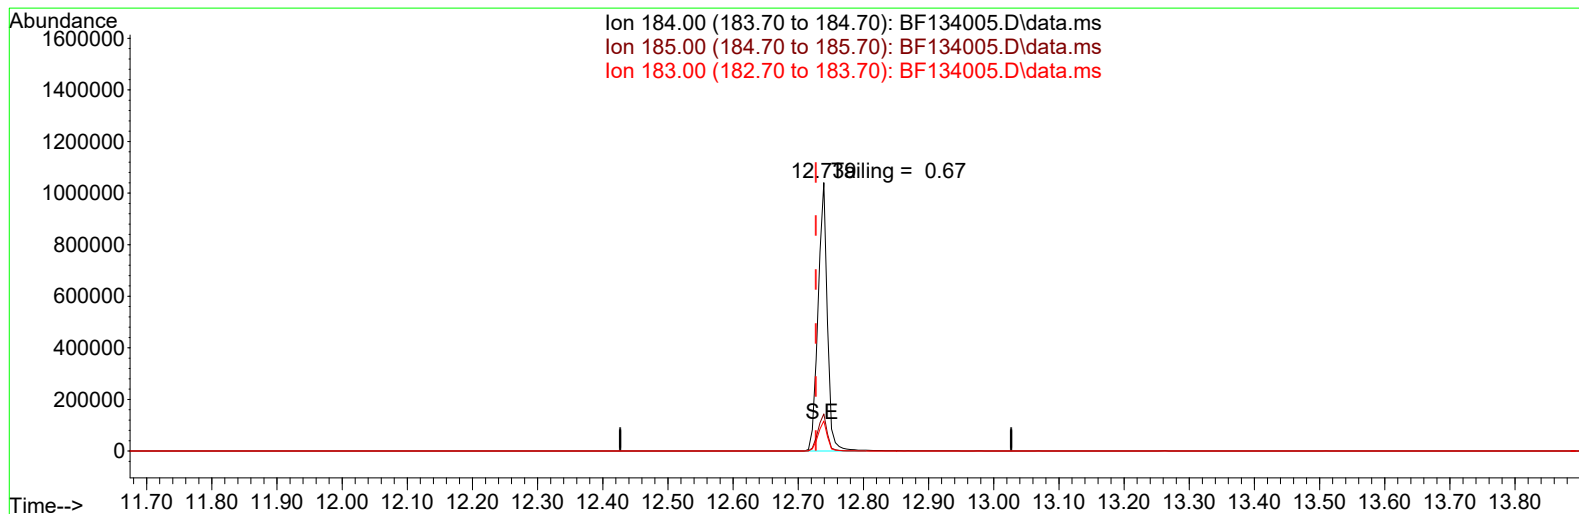

TIC: BF134005.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 667205.55 ng

response 1000170

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.86
183.00	11.00	11.22
0.00	0.00	0.00