

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
 Data File : BF133992.D
 Acq On : 27 Jun 2023 15:39
 Operator : CG\JU
 Sample : 03366-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF133992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	8	15	24	rVB	1409078	1790824	68.10%	6.769%
2	2.287	30	34	44	rVB	34411	48587	1.85%	0.184%
3	2.387	47	51	57	rVB2	21503	30775	1.17%	0.116%
4	5.093	508	511	521	rVB	197502	246275	9.36%	0.931%
5	5.487	573	578	581	rBV	2758352	2629770	100.00%	9.940%
6	6.487	743	748	751	rBV	2506252	2487720	94.60%	9.403%
7	6.851	806	810	813	rBV	987427	808107	30.73%	3.054%
8	7.410	900	905	909	rBV	1711851	1704332	64.81%	6.442%
9	8.128	1023	1027	1030	rBV	1240330	991078	37.69%	3.746%
10	9.204	1206	1210	1214	rBV	2856648	2605991	99.10%	9.850%
11	9.745	1299	1302	1305	rVB	36264	30340	1.15%	0.115%
12	9.886	1322	1326	1330	rBV	1256213	992466	37.74%	3.751%
13	9.916	1330	1331	1337	rVB	41801	34455	1.31%	0.130%
14	10.439	1416	1420	1424	rBV	34938	38388	1.46%	0.145%
15	10.604	1444	1448	1454	rVB	294658	239479	9.11%	0.905%
16	10.680	1457	1461	1464	rBV	1978073	1634480	62.15%	6.178%
17	10.792	1476	1480	1486	rVB	91455	101308	3.85%	0.383%
18	11.239	1551	1556	1560	rBV5	16465	34622	1.32%	0.131%
19	11.380	1576	1580	1582	rBV	1102899	944101	35.90%	3.568%
20	11.404	1582	1584	1588	rVV	465934	381115	14.49%	1.440%
21	11.457	1590	1593	1596	rVV	90646	75770	2.88%	0.286%
22	11.486	1596	1598	1602	rVV2	28634	28150	1.07%	0.106%
23	11.616	1613	1620	1627	rBV2	54330	82210	3.13%	0.311%
24	11.886	1662	1666	1668	rBV	64708	58207	2.21%	0.220%
25	11.910	1668	1670	1676	rVV	346416	348967	13.27%	1.319%
26	11.963	1676	1679	1682	rVV2	40585	46566	1.77%	0.176%
27	11.998	1682	1685	1687	rVV2	117117	124962	4.75%	0.472%
28	12.022	1687	1689	1694	rVB	52701	45894	1.75%	0.173%
29	12.186	1715	1717	1719	rVV	37652	29287	1.11%	0.111%
30	12.210	1719	1721	1724	rVB	49080	40818	1.55%	0.154%
31	12.439	1757	1760	1763	rBV2	56274	64202	2.44%	0.243%
32	12.474	1763	1766	1769	rVV3	34812	39902	1.52%	0.151%
33	12.527	1772	1775	1780	rVB2	41693	49225	1.87%	0.186%
34	12.604	1784	1788	1791	rBV	838925	671457	25.53%	2.538%
35	12.704	1801	1805	1807	rBV2	70705	68972	2.62%	0.261%
36	12.833	1821	1827	1833	rBV	659146	685649	26.07%	2.592%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
 Data File : BF133992.D
 Acq On : 27 Jun 2023 15:39
 Operator : CG\JU
 Sample : 03366-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	12.886	1833	1836	1839	rVV2	29731	34223	1.30%	0.129%
38	12.916	1839	1841	1844	rVB	103418	83845	3.19%	0.317%
39	12.951	1844	1847	1848	rBV3	38811	32426	1.23%	0.123%
40	12.980	1848	1852	1859	rVB	1977257	1734168	65.94%	6.555%
41	13.057	1860	1865	1868	rVV2	46693	70842	2.69%	0.268%
42	13.139	1876	1879	1881	rBV4	41482	46875	1.78%	0.177%
43	13.163	1881	1883	1887	rVB2	119689	105833	4.02%	0.400%
44	13.210	1887	1891	1892	rBV3	27740	34764	1.32%	0.131%
45	13.233	1892	1895	1897	rVB	72357	60863	2.31%	0.230%
46	13.257	1897	1899	1904	rBV3	91478	122915	4.67%	0.465%
47	13.363	1914	1917	1920	rBV	42229	39880	1.52%	0.151%
48	13.392	1920	1922	1926	rVV	44589	42680	1.62%	0.161%
49	13.557	1947	1950	1954	rBV4	50358	58300	2.22%	0.220%
50	13.674	1968	1970	1975	rVB	75356	76173	2.90%	0.288%
51	13.786	1986	1989	1992	rBV2	51478	55464	2.11%	0.210%
52	13.816	1992	1994	1996	rVV	52131	42989	1.63%	0.162%
53	13.839	1996	1998	2003	rVV2	42163	60554	2.30%	0.229%
54	13.886	2003	2006	2014	rVB	224640	270263	10.28%	1.022%
55	14.039	2025	2032	2035	rBV2	691252	972400	36.98%	3.675%
56	14.068	2035	2037	2043	rVB	324329	289899	11.02%	1.096%
57	14.145	2048	2050	2053	rVB	42217	34591	1.32%	0.131%
58	14.333	2079	2082	2084	rVB3	34427	28471	1.08%	0.108%
59	14.433	2096	2099	2102	rVB	65841	57163	2.17%	0.216%
60	14.468	2102	2105	2108	rVB2	33017	29569	1.12%	0.112%
61	14.533	2110	2116	2118	rBV4	77895	140344	5.34%	0.530%
62	14.833	2164	2167	2169	rBV	38259	38393	1.46%	0.145%
63	14.910	2177	2180	2183	rBV	46787	50777	1.93%	0.192%
64	14.986	2190	2193	2199	rVB5	53710	73179	2.78%	0.277%
65	15.104	2209	2213	2216	rBV	243705	363544	13.82%	1.374%
66	15.186	2224	2227	2229	rBV	53932	49674	1.89%	0.188%
67	15.215	2229	2232	2240	rVB4	63634	97551	3.71%	0.369%
68	15.415	2263	2266	2273	rVB	127110	181165	6.89%	0.685%
69	15.480	2273	2277	2283	rBV	188988	244958	9.31%	0.926%
70	15.551	2284	2289	2292	rBV	361449	466041	17.72%	1.761%
71	17.092	2545	2551	2558	rBV3	62499	132154	5.03%	0.499%




Sum of corrected areas: 26457381

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF133992.D
Acq On : 27 Jun 2023 15:39
Operator : CG\JU
Sample : 03366-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC37

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

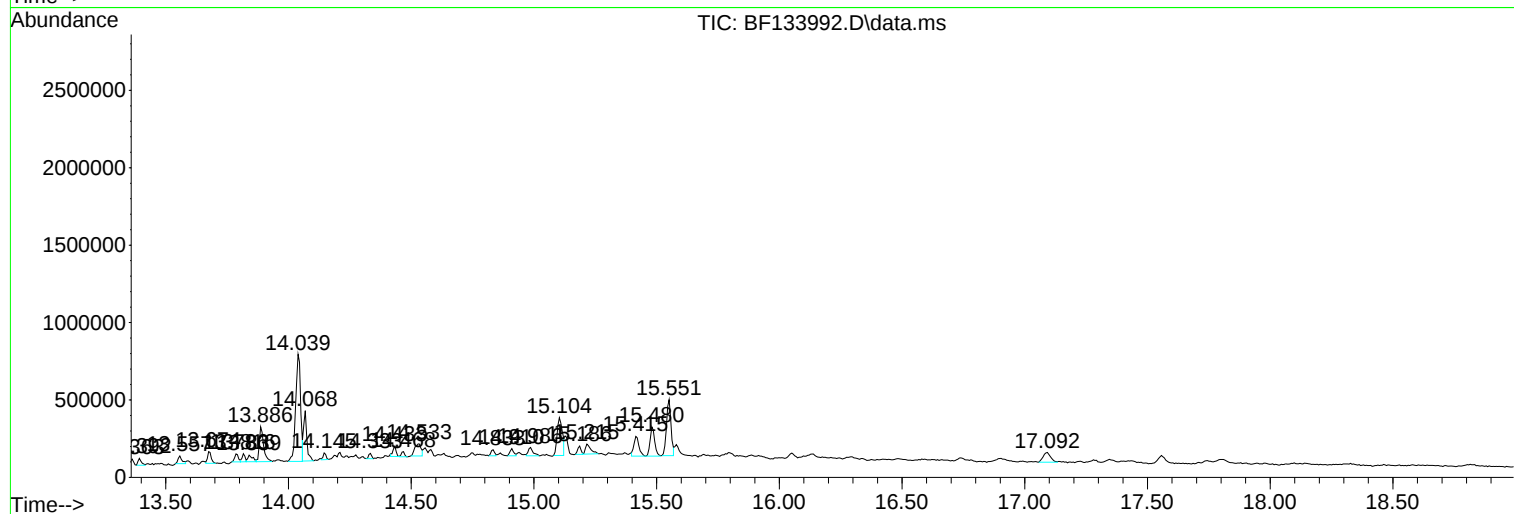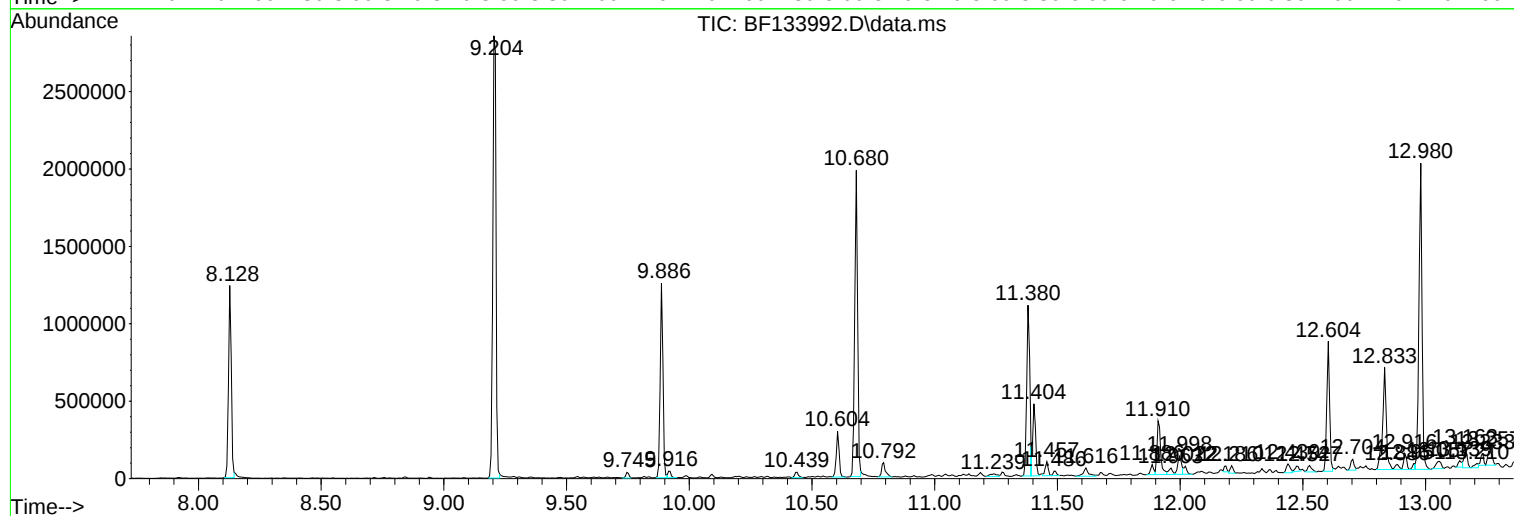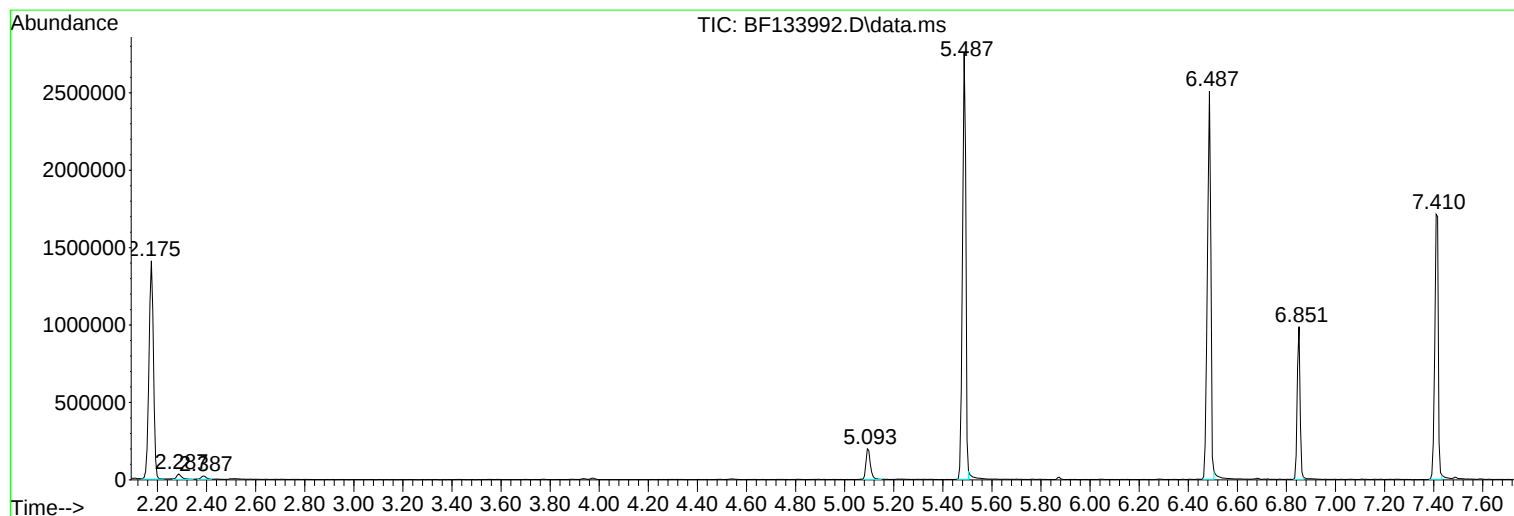

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF133992.D
Acq On : 27 Jun 2023 15:39
Operator : CG\JU
Sample : 03366-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC37

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF133992.D
Acq On : 27 Jun 2023 15:39
Operator : CG\JU
Sample : 03366-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC37

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------