
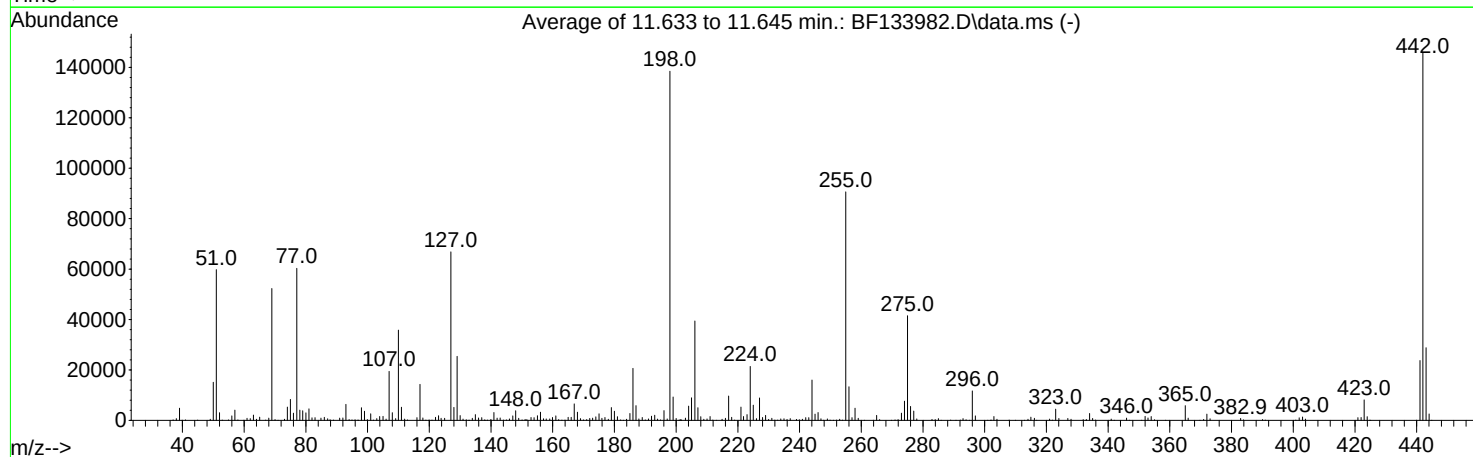


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF133982.D
Acq On : 27 Jun 2023 09:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 26 23:12:04 2023

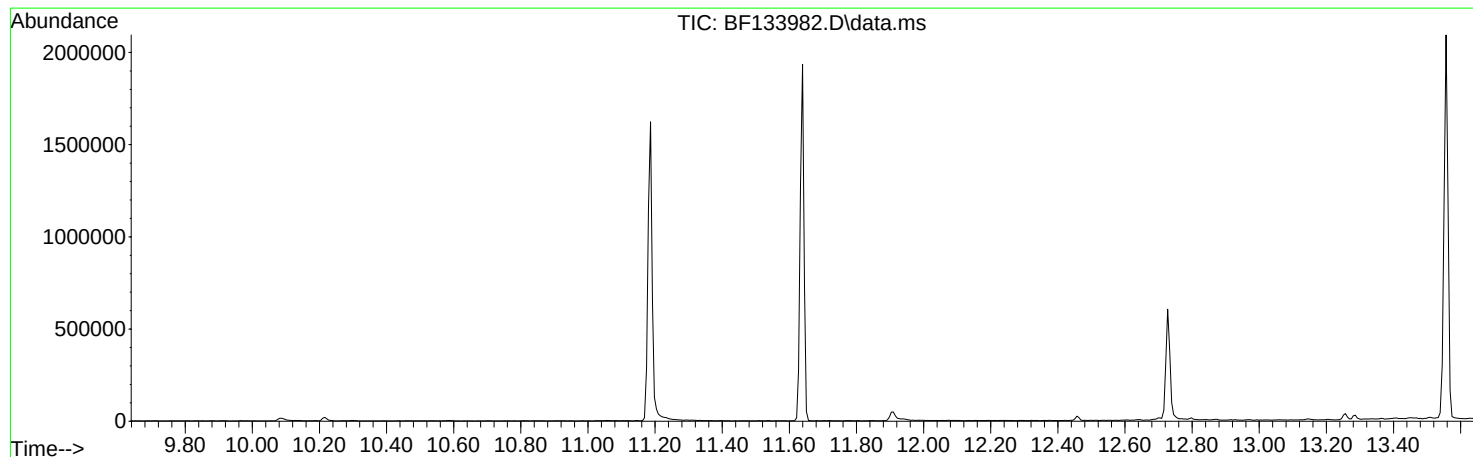

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	59787	PASS
68	69	0.00	2	1.7	876	PASS
69	198	0.00	100	37.8	52291	PASS
70	69	0.00	2	0.6	329	PASS
127	198	10	80	48.2	66811	PASS
197	198	0.00	2	0.4	553	PASS
198	198	100	100	100.0	138499	PASS
199	198	5	9	6.7	9288	PASS
275	198	10	60	30.0	41528	PASS
365	198	1	100	4.2	5822	PASS
441	198	0.01	100	17.1	23729	PASS
442	442	50	100	100.0	145907	PASS
443	442	15	24	19.8	28831	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/27/2023	BNA_F	<u>BF133982.D</u>
Compound Name	Response	Retention Time
DDT	335892	13.557
DDD	10050	13.257
DDE	284	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10334	346226	2.98

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\  
Data File : BF133982.D  
Acq On    : 27 Jun 2023  09:56  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 28 07:31:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

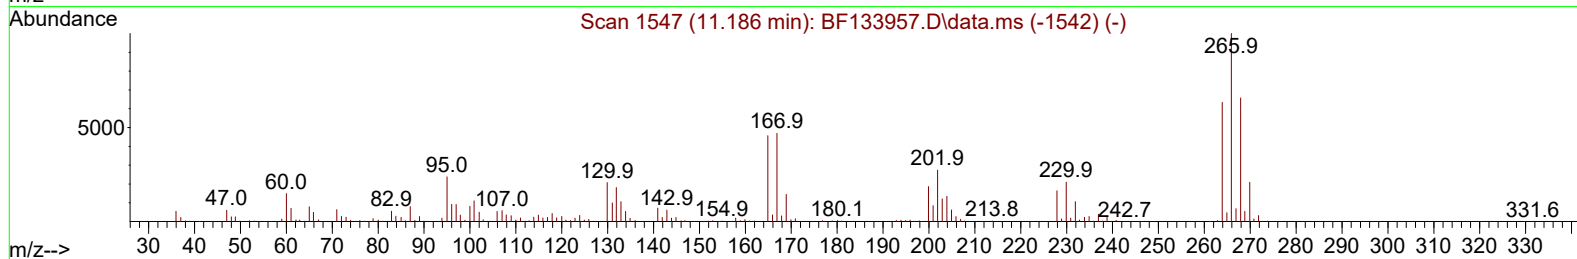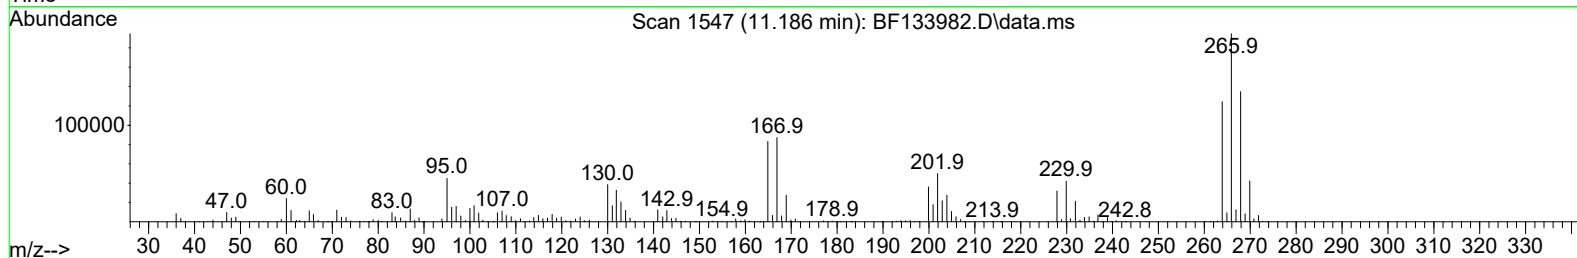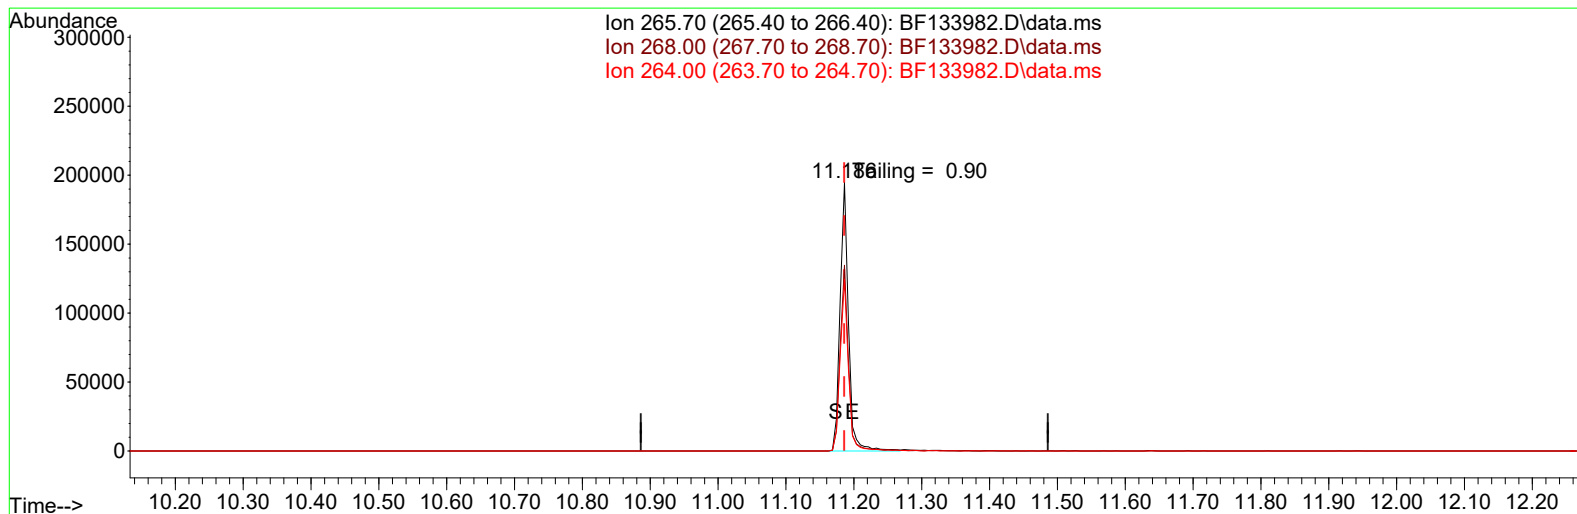

TIC: BF133982.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 102134.34 ng




response	167468
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	69.22
264.00	63.30	63.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF133982.D
Acq On : 27 Jun 2023 09:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 28 07:31:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

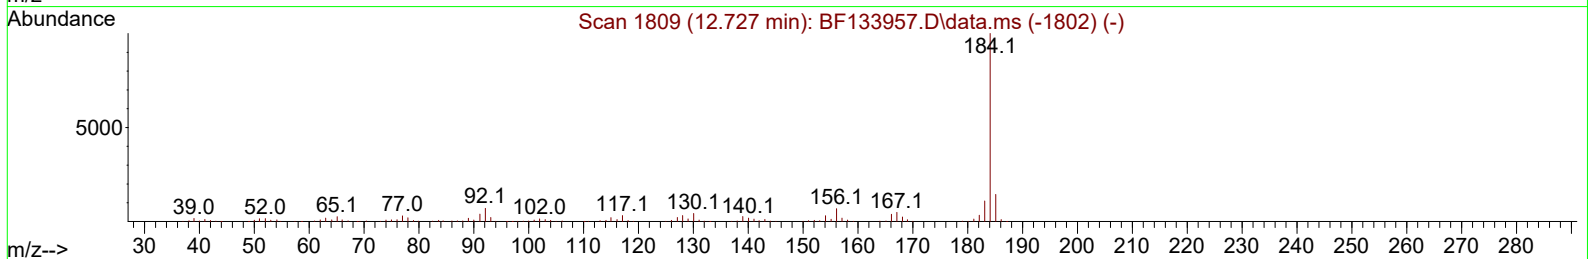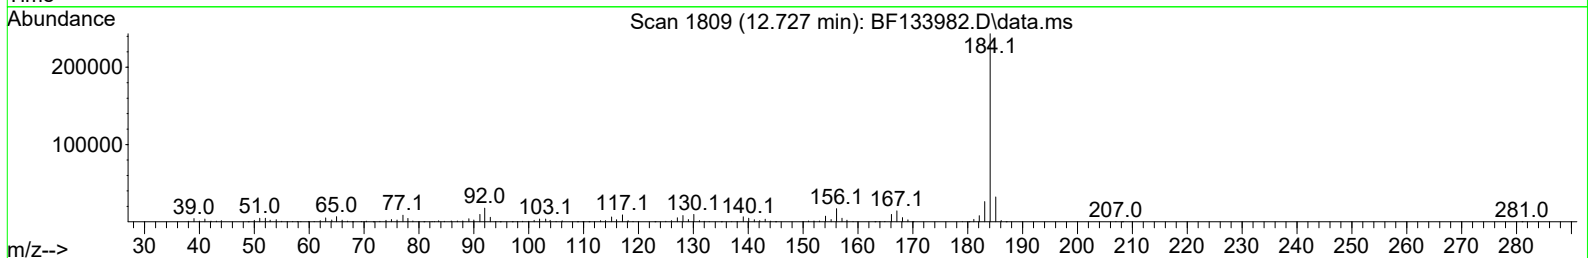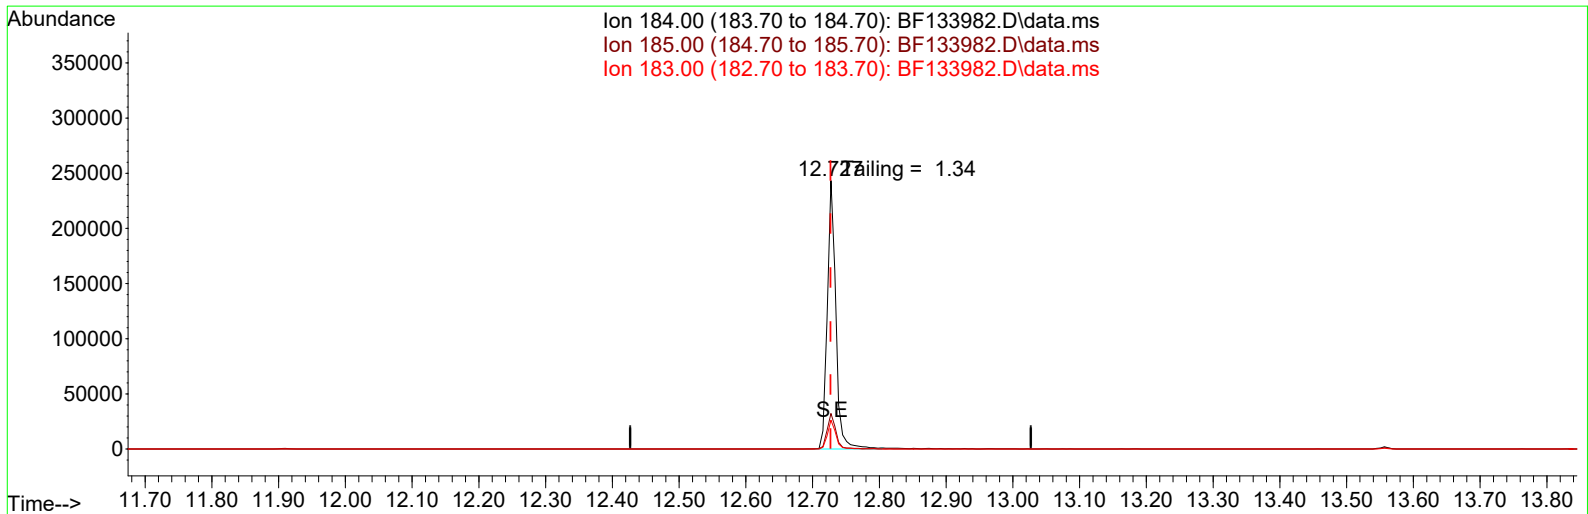

TIC: BF133982.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 54768.68 ng

response 218935

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.28
183.00	11.00	10.75
0.00	0.00	0.00