


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF134005.D
Acq On : 28 Jun 2023 00:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 26 23:12:04 2023

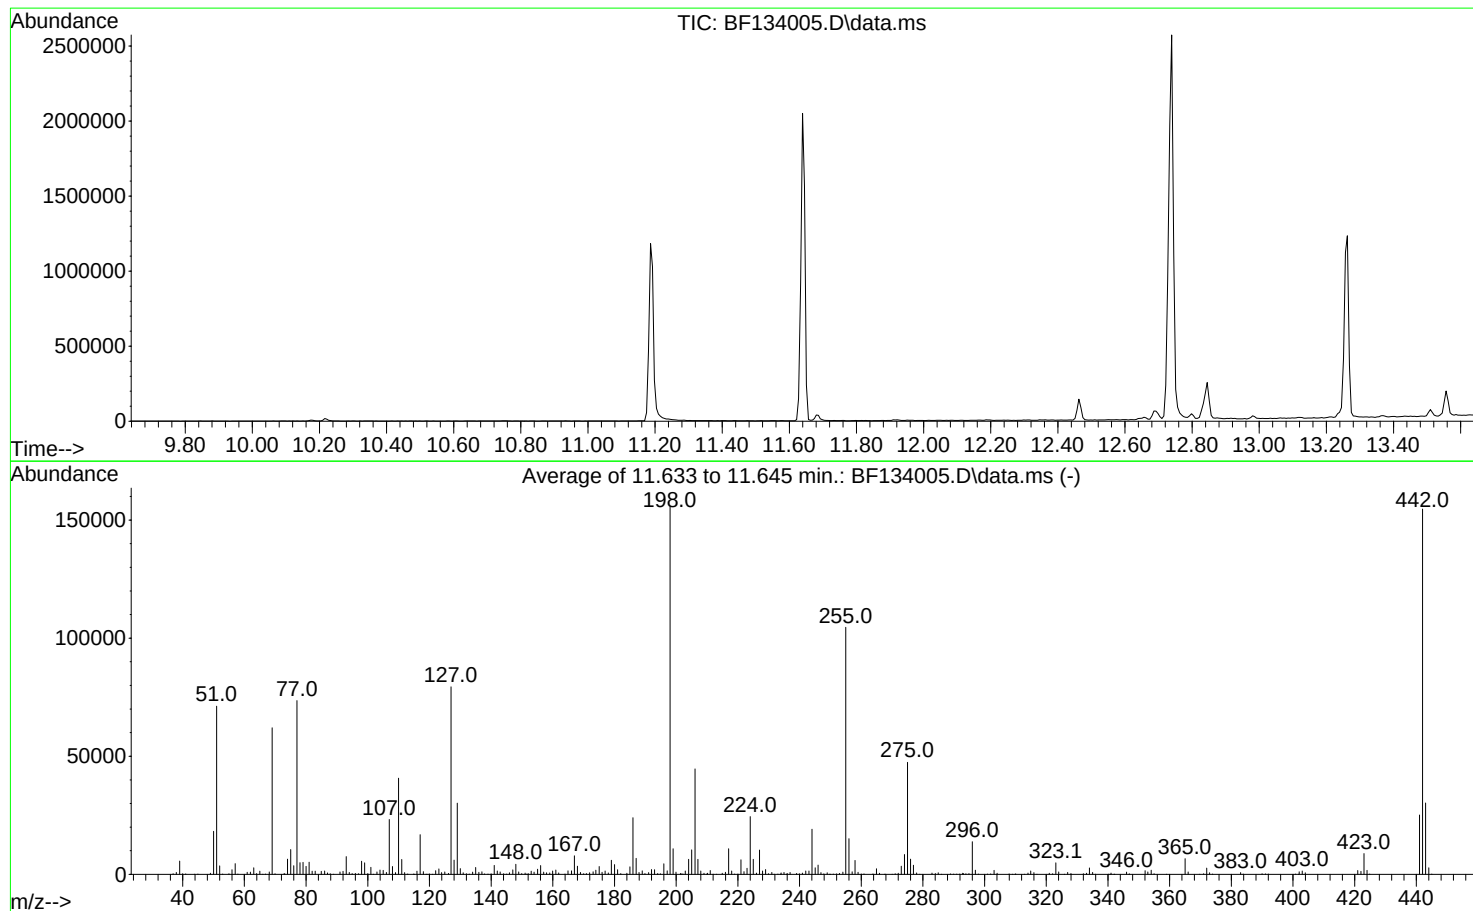

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	71227	PASS
68	69	0.00	2	1.7	1051	PASS
69	198	0.00	100	39.9	62069	PASS
70	69	0.00	2	0.4	258	PASS
127	198	10	80	51.0	79424	PASS
197	198	0.00	2	1.0	1480	PASS
198	198	100	100	100.0	155747	PASS
199	198	5	9	7.0	10829	PASS
275	198	10	60	30.5	47443	PASS
365	198	1	100	4.3	6678	PASS
441	198	0.01	100	16.1	25104	PASS
442	442	50	100	100.0	154624	PASS
443	442	15	24	19.6	30246	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/27/2023	BNA_F	<u>BF134005.D</u>
Compound Name	Response	Retention Time
DDT	24859	13.557
DDD	224393	13.263
DDE	408	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
224801	249660	90.04

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
 Data File : BF134005.D
 Acq On : 28 Jun 2023 00:00
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 07:32:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 23:12:04 2023
 Response via : Initial Calibration

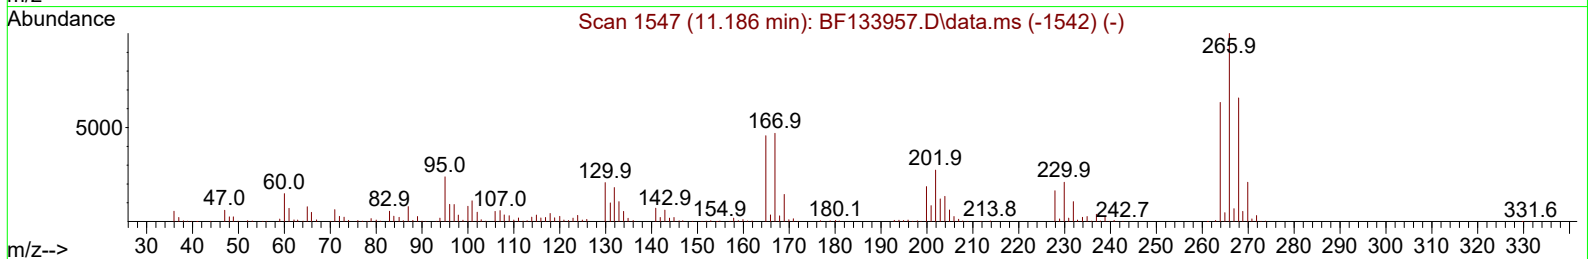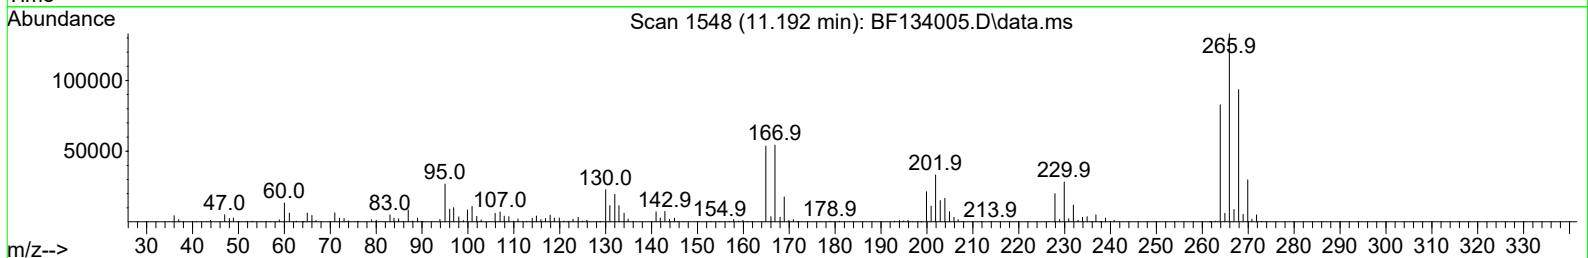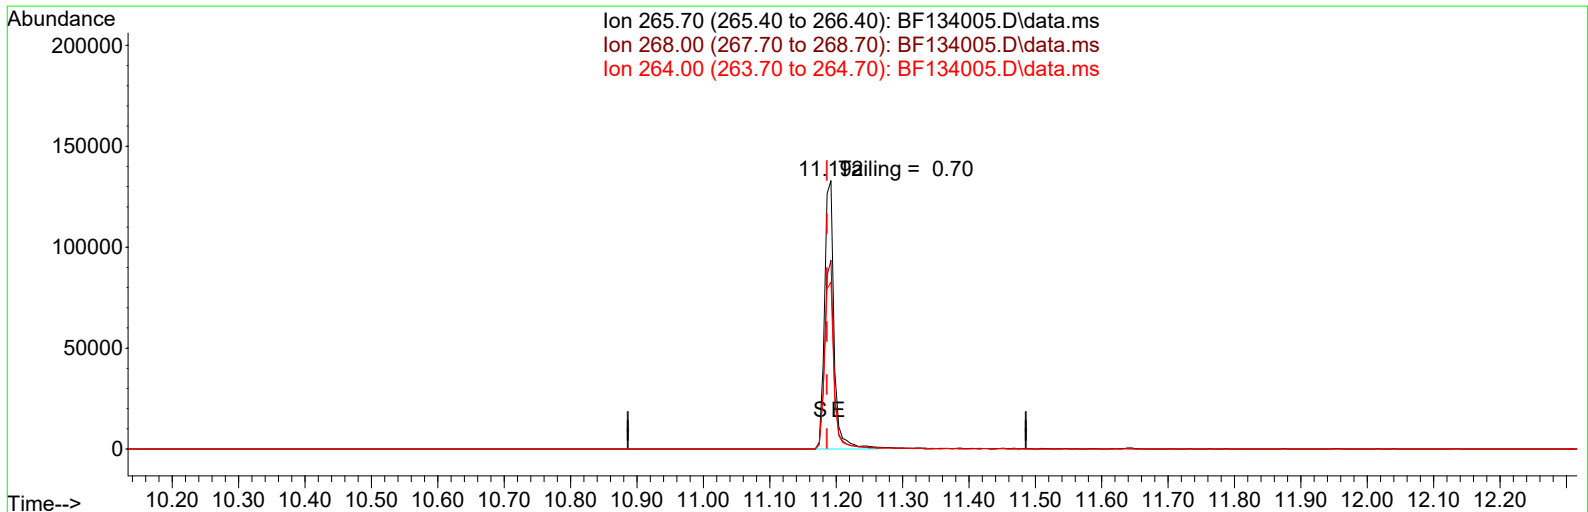

TIC: BF134005.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.006) 22292.73 ng




response 134479

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	70.30
264.00	63.30	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062723\
Data File : BF134005.D
Acq On : 28 Jun 2023 00:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 28 07:32:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

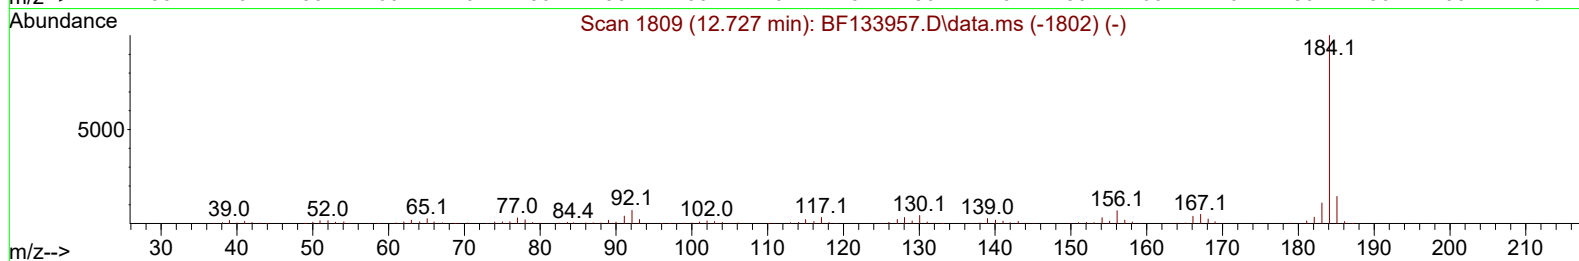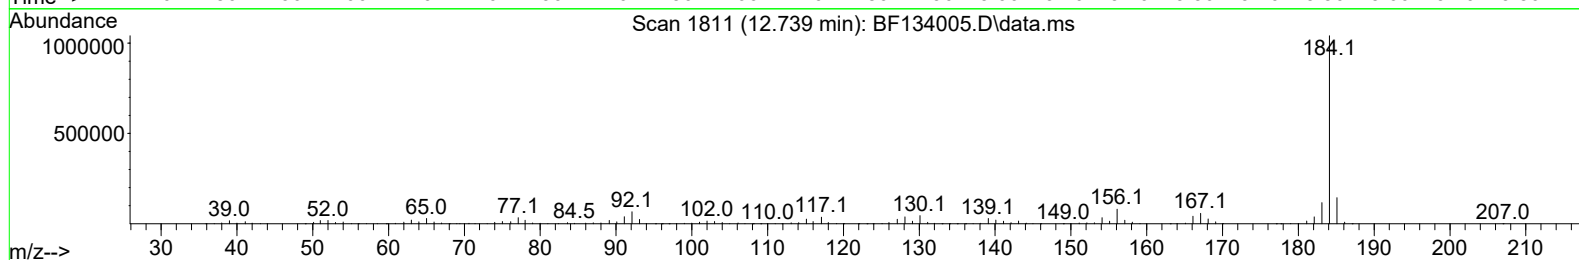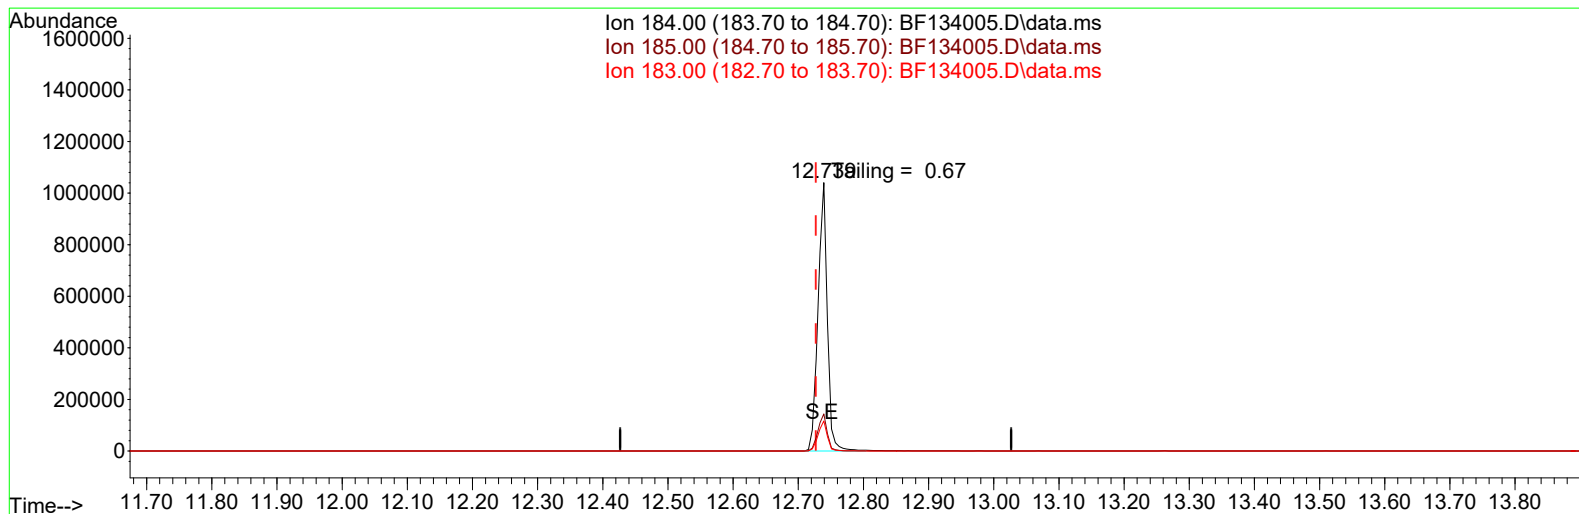

TIC: BF134005.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 667205.55 ng

response 1000170

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.86
183.00	11.00	11.22
0.00	0.00	0.00