


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062818\
Data File : BF106912.D
Acq On : 28 Jun 2018 10:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 25 18:50:17 2018

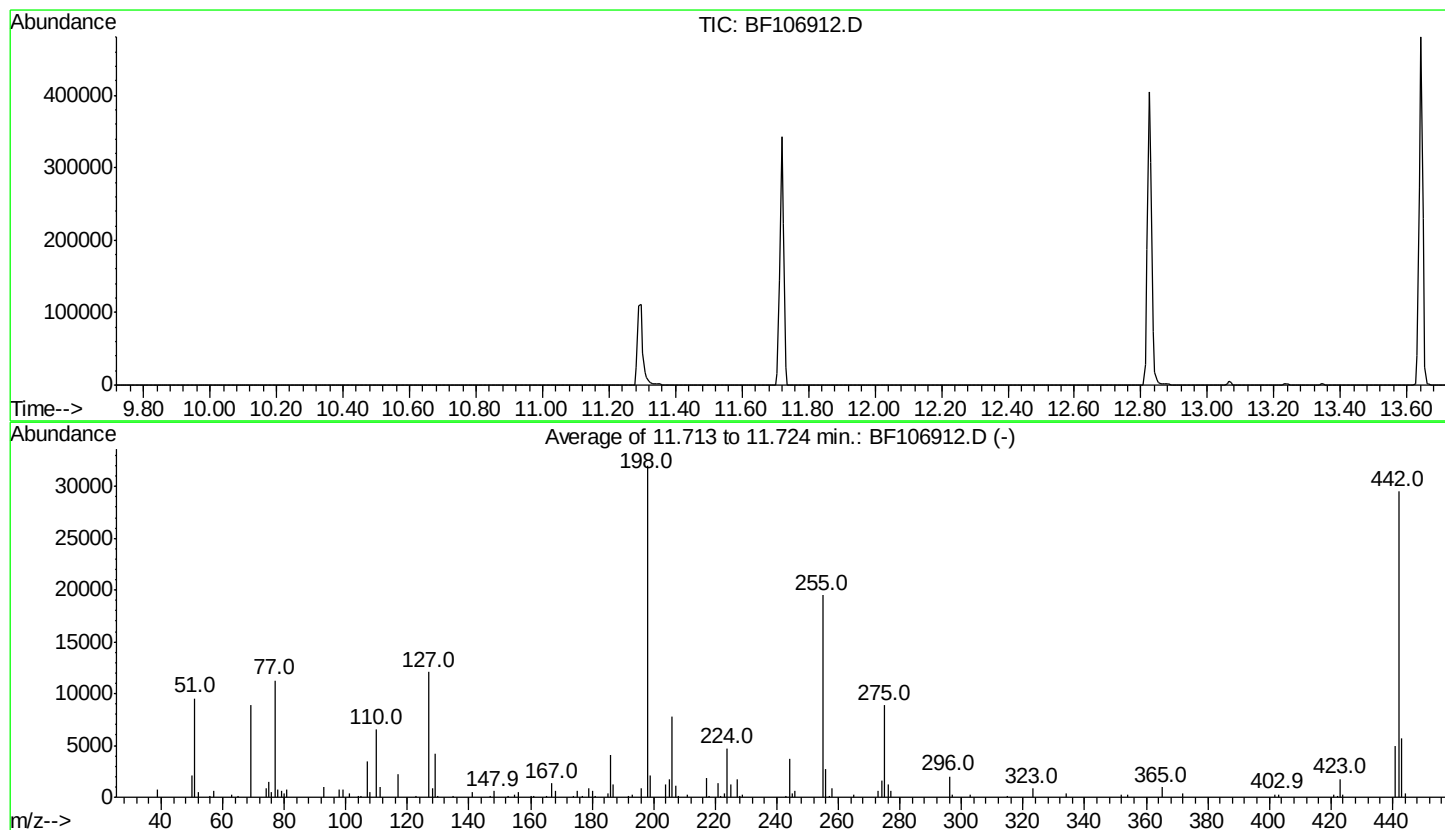

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	9522	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.9	8933	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.8	12088	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32008	PASS
199	198	5	9	6.6	2128	PASS
275	198	10	60	27.7	8864	PASS
365	198	1	100	3.0	967	PASS
441	443	0.01	100	85.3	4903	PASS
442	198	50	100	92.2	29526	PASS
443	442	15	24	19.5	5749	PASS