


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062818\
 Data File : BF106924.D
 Acq On : 28 Jun 2018 16:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 25 18:50:17 2018

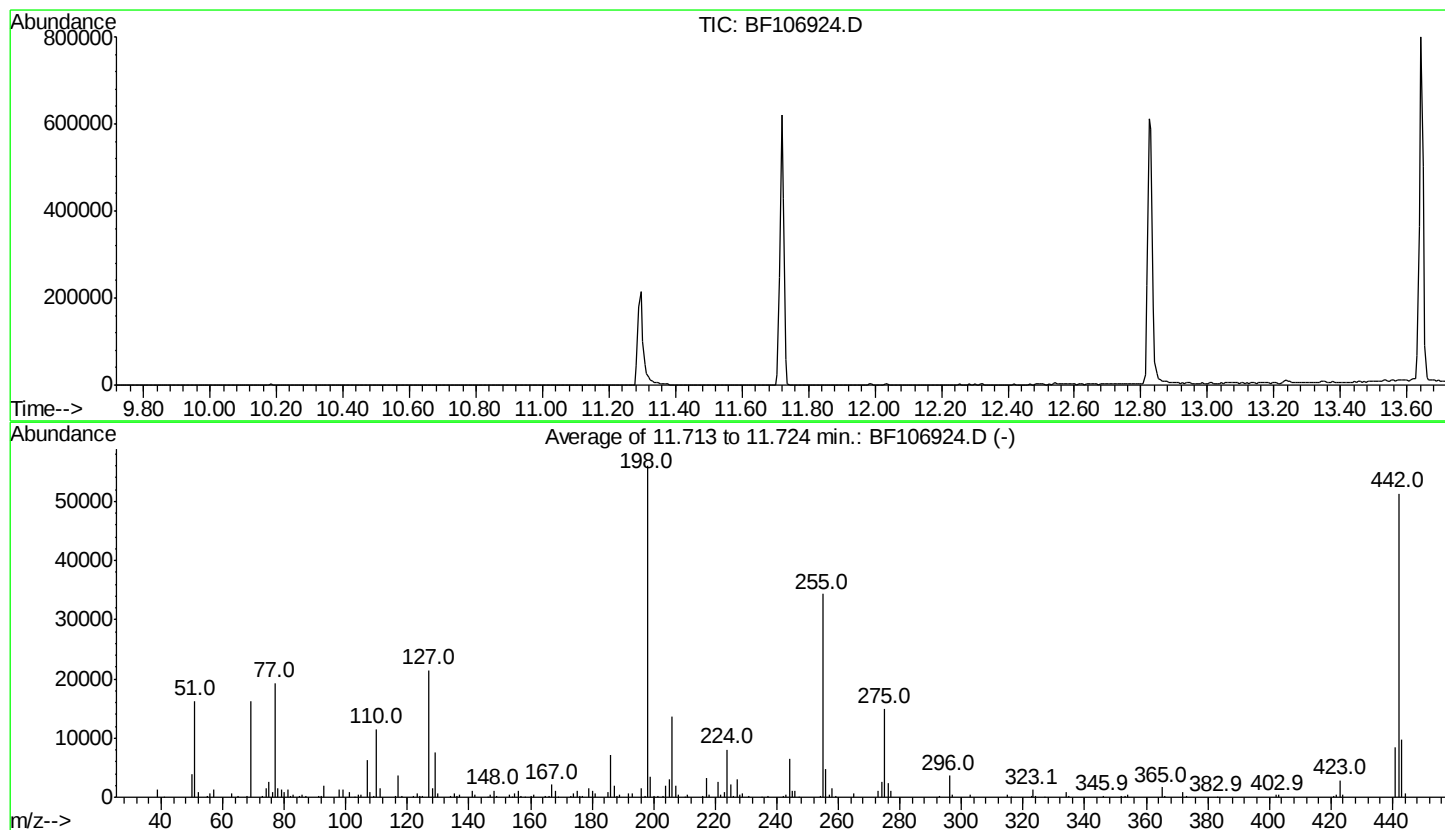

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	16314	PASS
68	69	0.00	2	0.9	149	PASS
69	198	0.00	100	28.8	16152	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.4	21486	PASS
197	198	0.00	2	0.5	298	PASS
198	198	100	100	100.0	56013	PASS
199	198	5	9	6.4	3562	PASS
275	198	10	60	26.8	15009	PASS
365	198	1	100	3.1	1716	PASS
441	443	0.01	100	85.3	8333	PASS
442	198	50	100	91.5	51257	PASS
443	442	15	24	19.1	9773	PASS