


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062824\
Data File : BF138383.D
Acq On : 28 Jun 2024 12:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 29 02:44:30 2024

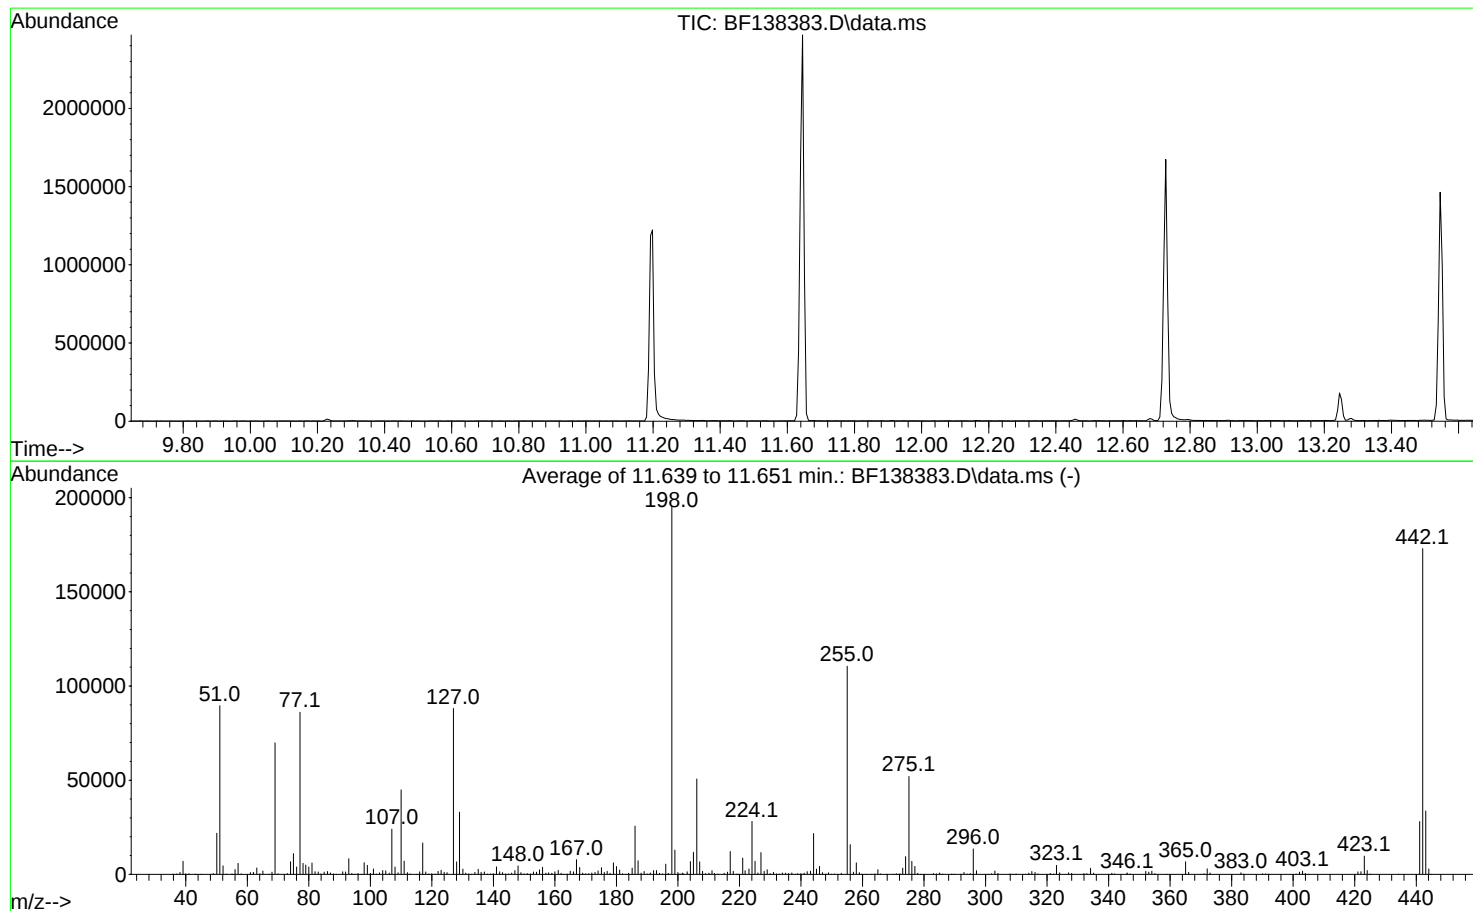

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	89588	PASS
68	69	0.00	2	1.8	1227	PASS
69	198	0.00	100	35.8	69867	PASS
70	69	0.00	2	0.5	332	PASS
127	198	10	80	45.1	88077	PASS
197	198	0.00	2	0.3	497	PASS
198	198	100	100	100.0	195325	PASS
199	198	5	9	6.6	12954	PASS
275	198	10	60	26.6	52013	PASS
365	198	1	100	3.4	6694	PASS
441	198	0.01	100	14.4	28047	PASS
442	442	50	100	100.0	172979	PASS
443	442	15	24	19.5	33645	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/28/2024	BNA_F	<u>BF138383.D</u>
Compound Name	Response	Retention Time
DDT	227849	13.545
DDD	30724	13.245
DDE	431	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31155	259004	12.03

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062824\
Data File : BF138383.D
Acq On : 28 Jun 2024 12:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 29 02:51:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

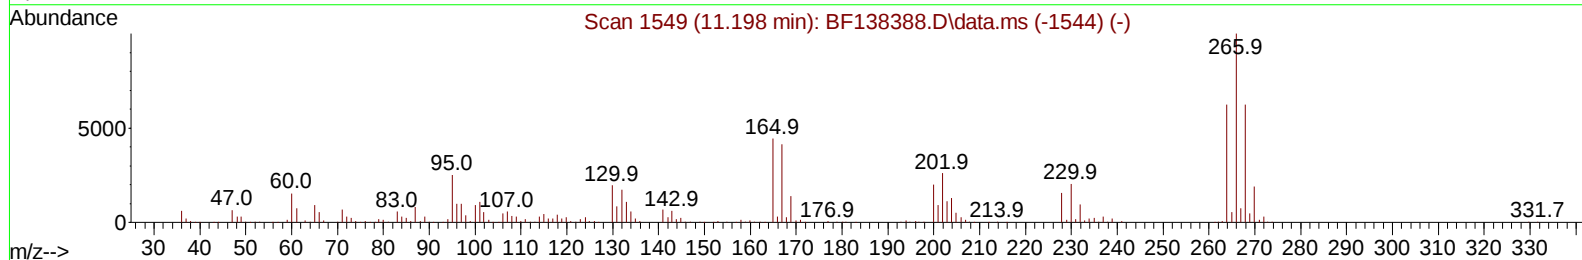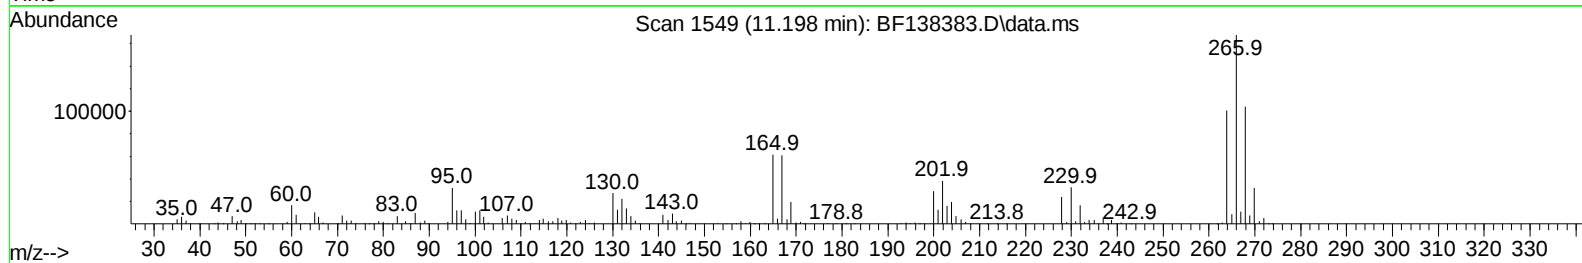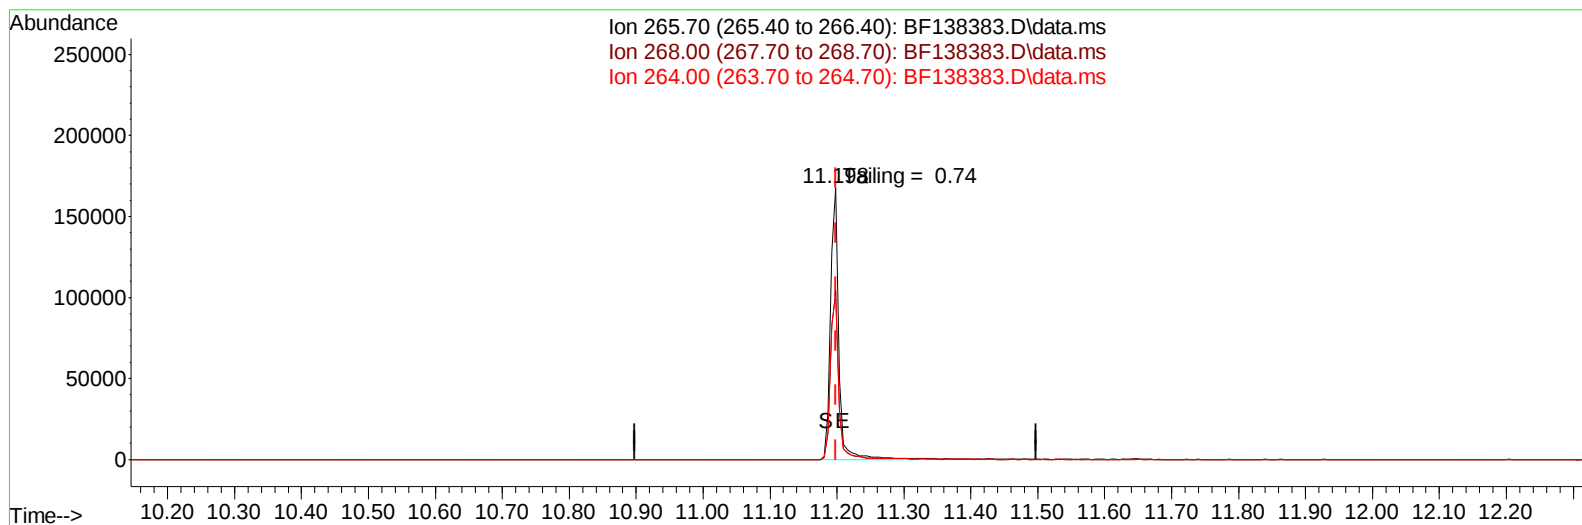

TIC: BF138383.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 31003.33 ng




response 146902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.23
264.00	62.50	60.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062824\
Data File : BF138383.D
Acq On : 28 Jun 2024 12:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 29 02:51:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

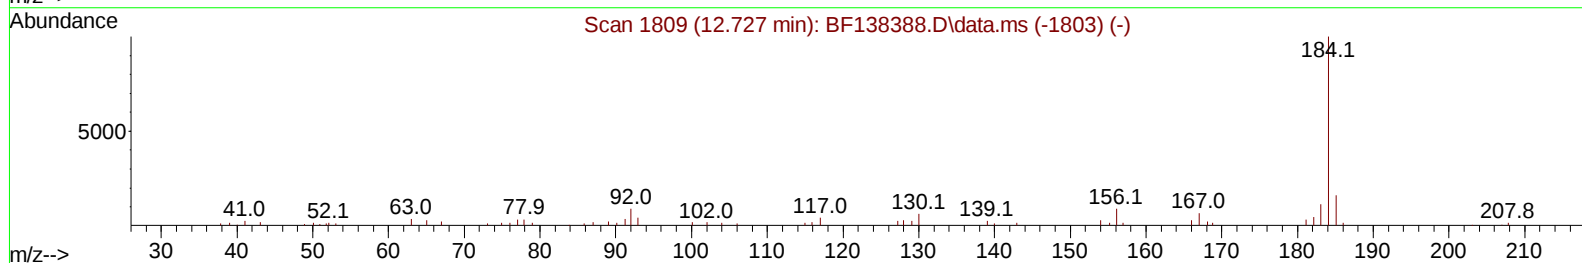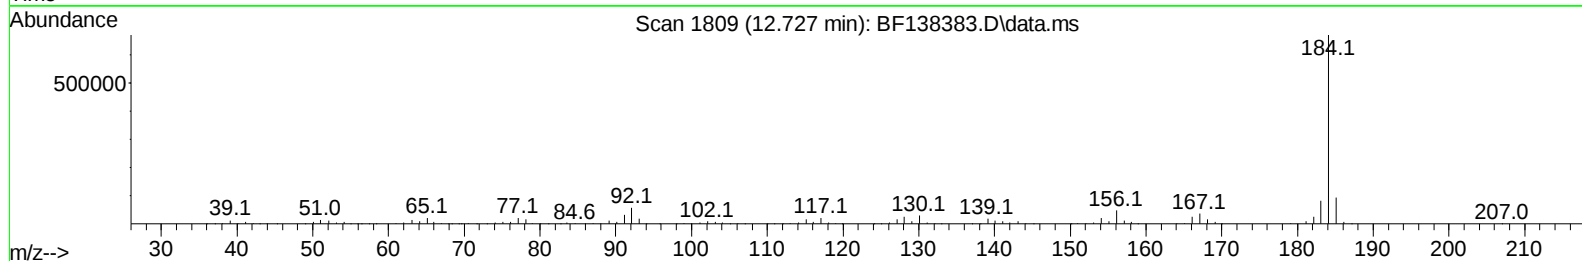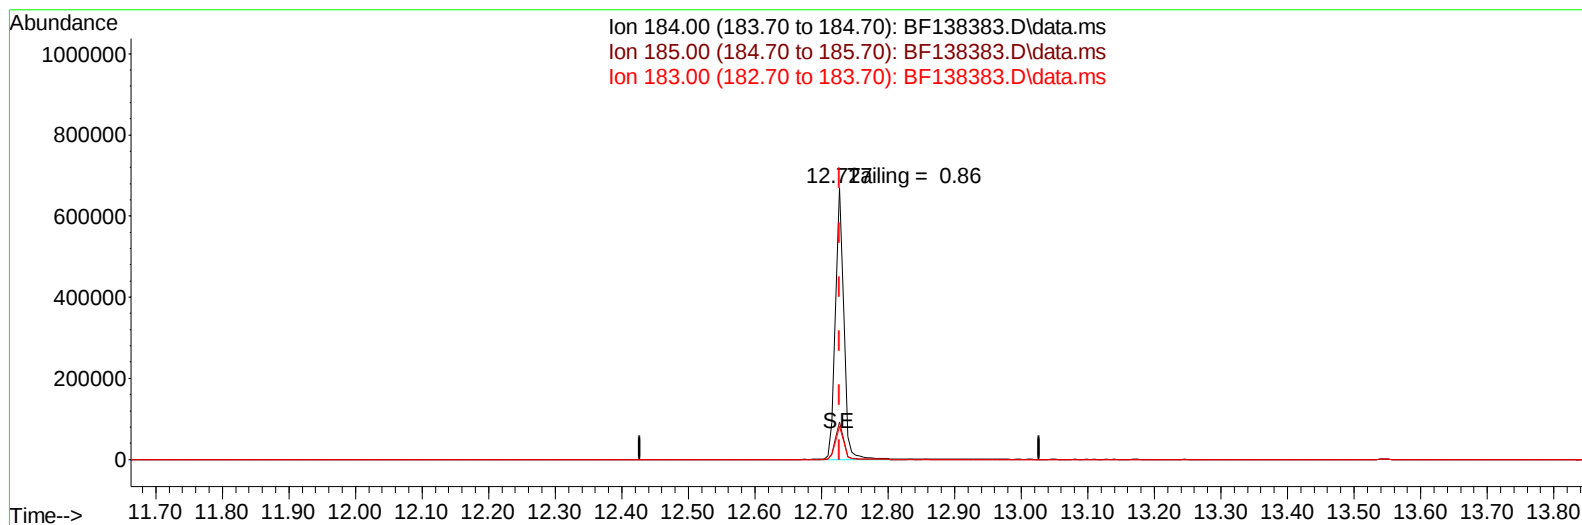

TIC: BF138383.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 0.00 ng

response 577198

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	13.93
183.00	11.30	12.10
0.00	0.00	0.00