
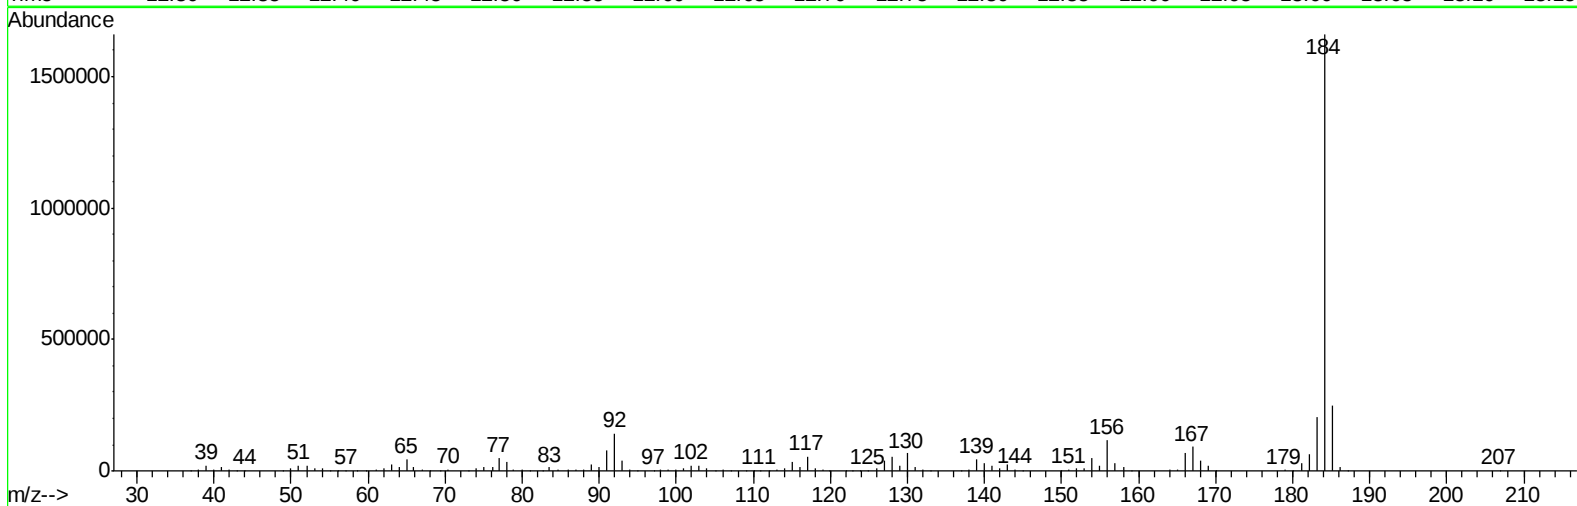


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062919\
Data File : BF115307.D
Acq On : 29 Jun 2019 7:54
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 04:40:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

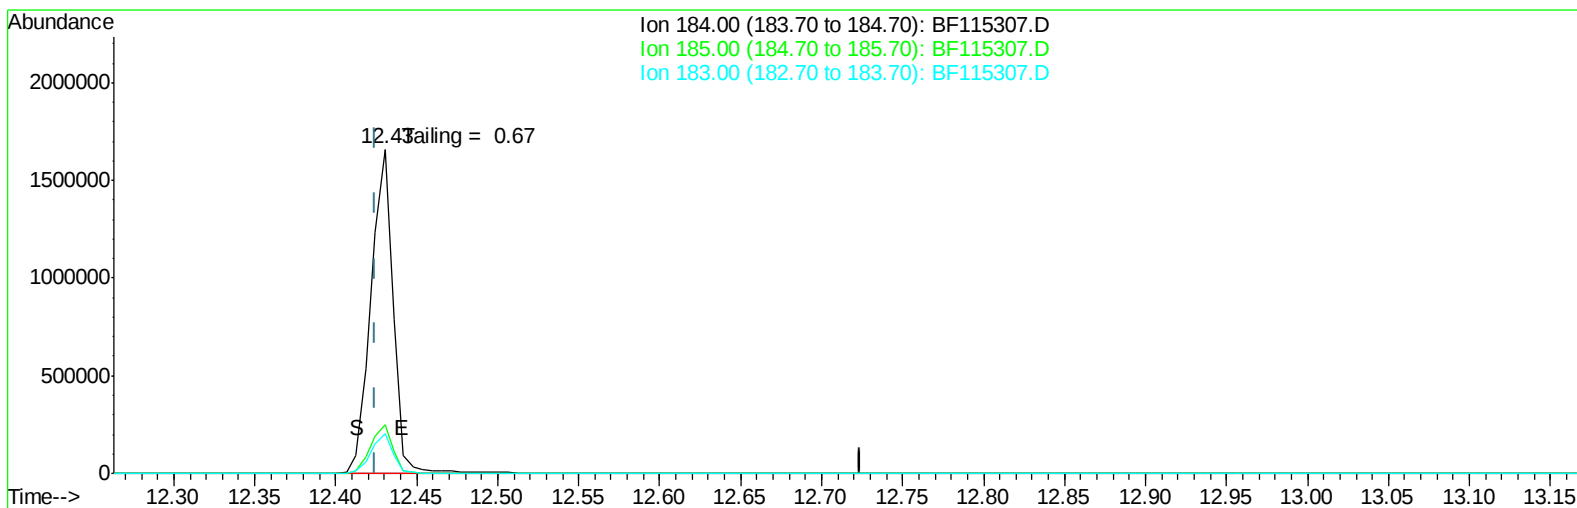

TIC: BF115307.D

(77) Benzidine



12.430min (+0.006) 116611.34ng

response 1610361

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.86
183.00	12.00	12.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062919\
Data File : BF115307.D
Acq On : 29 Jun 2019 7:54
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 04:40:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

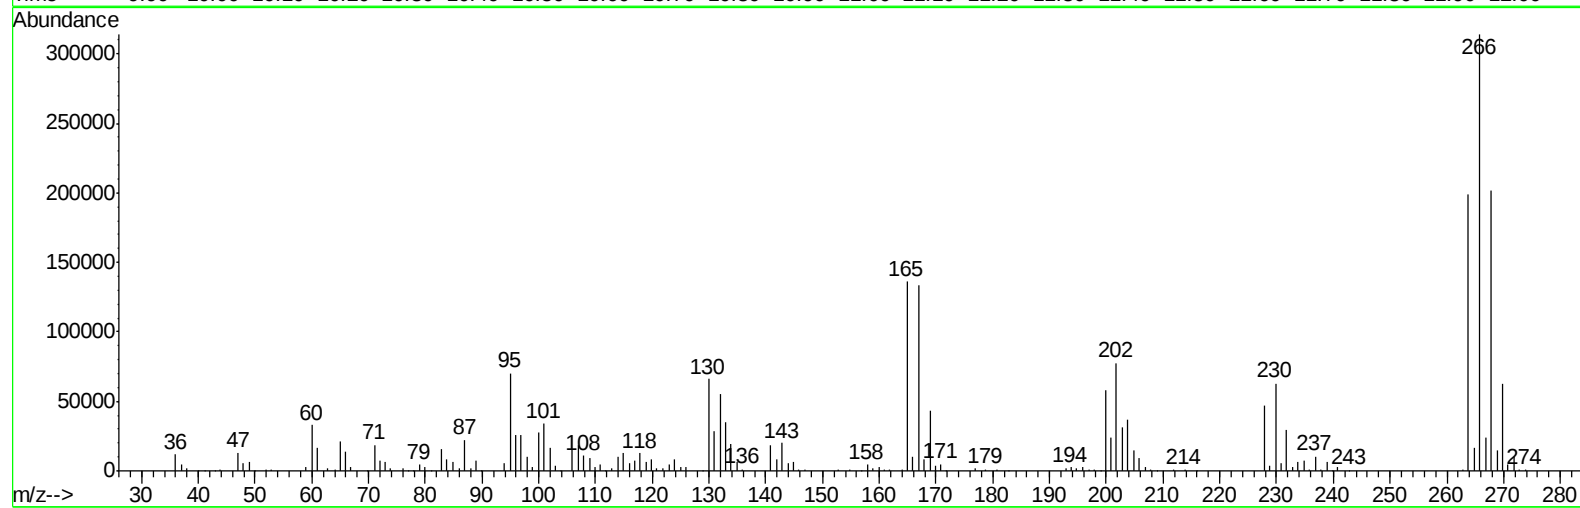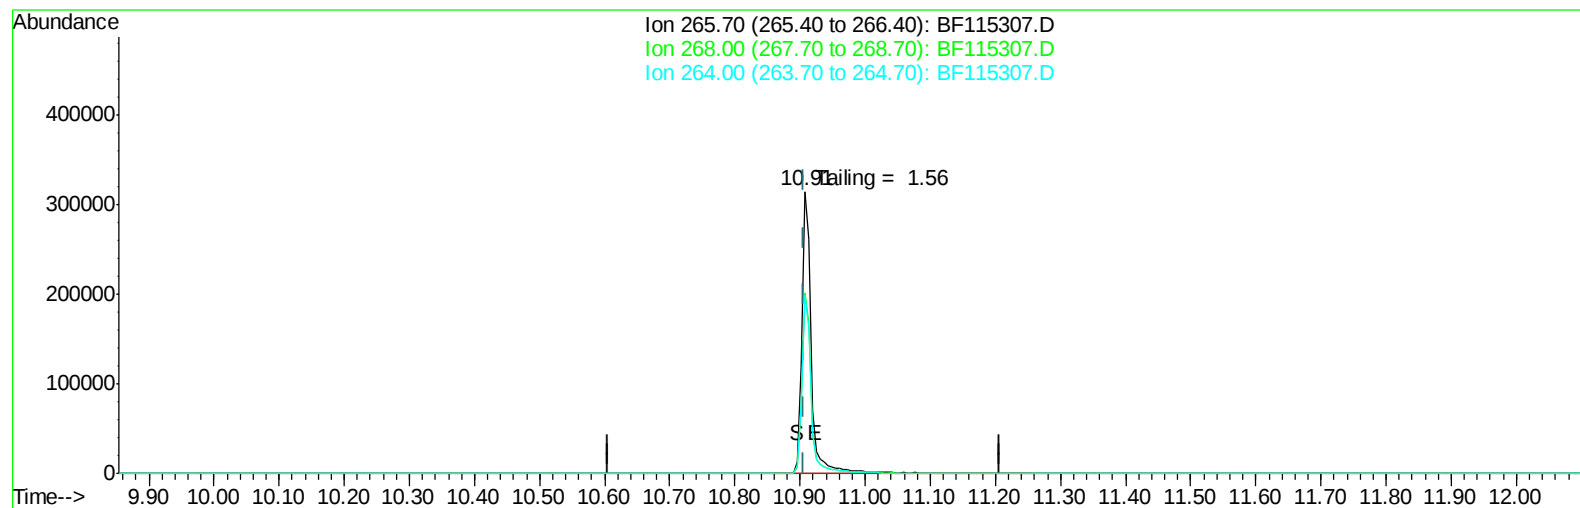

TIC: BF115307.D

(70) Pentachlorophenol (C)

10.907min (+0.000) 154830.24ng

response 315740

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	64.25
264.00	61.60	63.25
0.00	0.00	0.00