

Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_F\DATA\BF062919\
 Data File : BF115311.D
 Acq On : 29 Jun 2019 9:41
 Operator : HP/JU
 Sample : PB121004BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121004BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.207	550	556	559	rBV	4802380	5266170	75.15%	9.765%
2	6.242	726	732	735	rBV	4852881	5342859	76.24%	9.908%
3	6.366	748	753	757	rBV	5213315	5639488	80.48%	10.458%
4	6.595	789	792	796	rBV	1574143	1323507	18.89%	2.454%
5	6.754	815	819	822	rBV	5117441	4662887	66.54%	8.647%
6	7.160	882	888	891	rBV	3543575	3648058	52.06%	6.765%
7	7.878	1005	1010	1014	rBV	1886659	1673652	23.88%	3.104%
8	8.960	1188	1194	1197	rBV	6601866	6796165	96.98%	12.603%
9	9.624	1302	1307	1319	rBV	2202190	1987392	28.36%	3.685%
10	10.407	1435	1440	1456	rBV	4102038	4227756	60.33%	7.840%
11	11.095	1553	1557	1561	rBV	2407890	2094341	29.89%	3.884%
12	12.683	1822	1827	1830	rBV	6628421	7007606	100.00%	12.995%
13	13.712	1998	2002	2011	rBV	2106892	1901366	27.13%	3.526%
14	15.077	2229	2234	2241	rBV	1604494	1959139	27.96%	3.633%
15	15.142	2242	2245	2251	rVB	81892	111312	1.59%	0.206%
16	15.524	2306	2310	2316	rVB	76175	111574	1.59%	0.207%
17	15.959	2379	2384	2391	rVB	60405	98098	1.40%	0.182%
18	16.471	2466	2471	2479	rVB2	36255	75039	1.07%	0.139%


Sum of corrected areas: 53926409

Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_F\DATA\BF062919\
Data File : BF115311.D
Acq On : 29 Jun 2019 9:41
Operator : HP/JU
Sample : PB121004BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121004BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

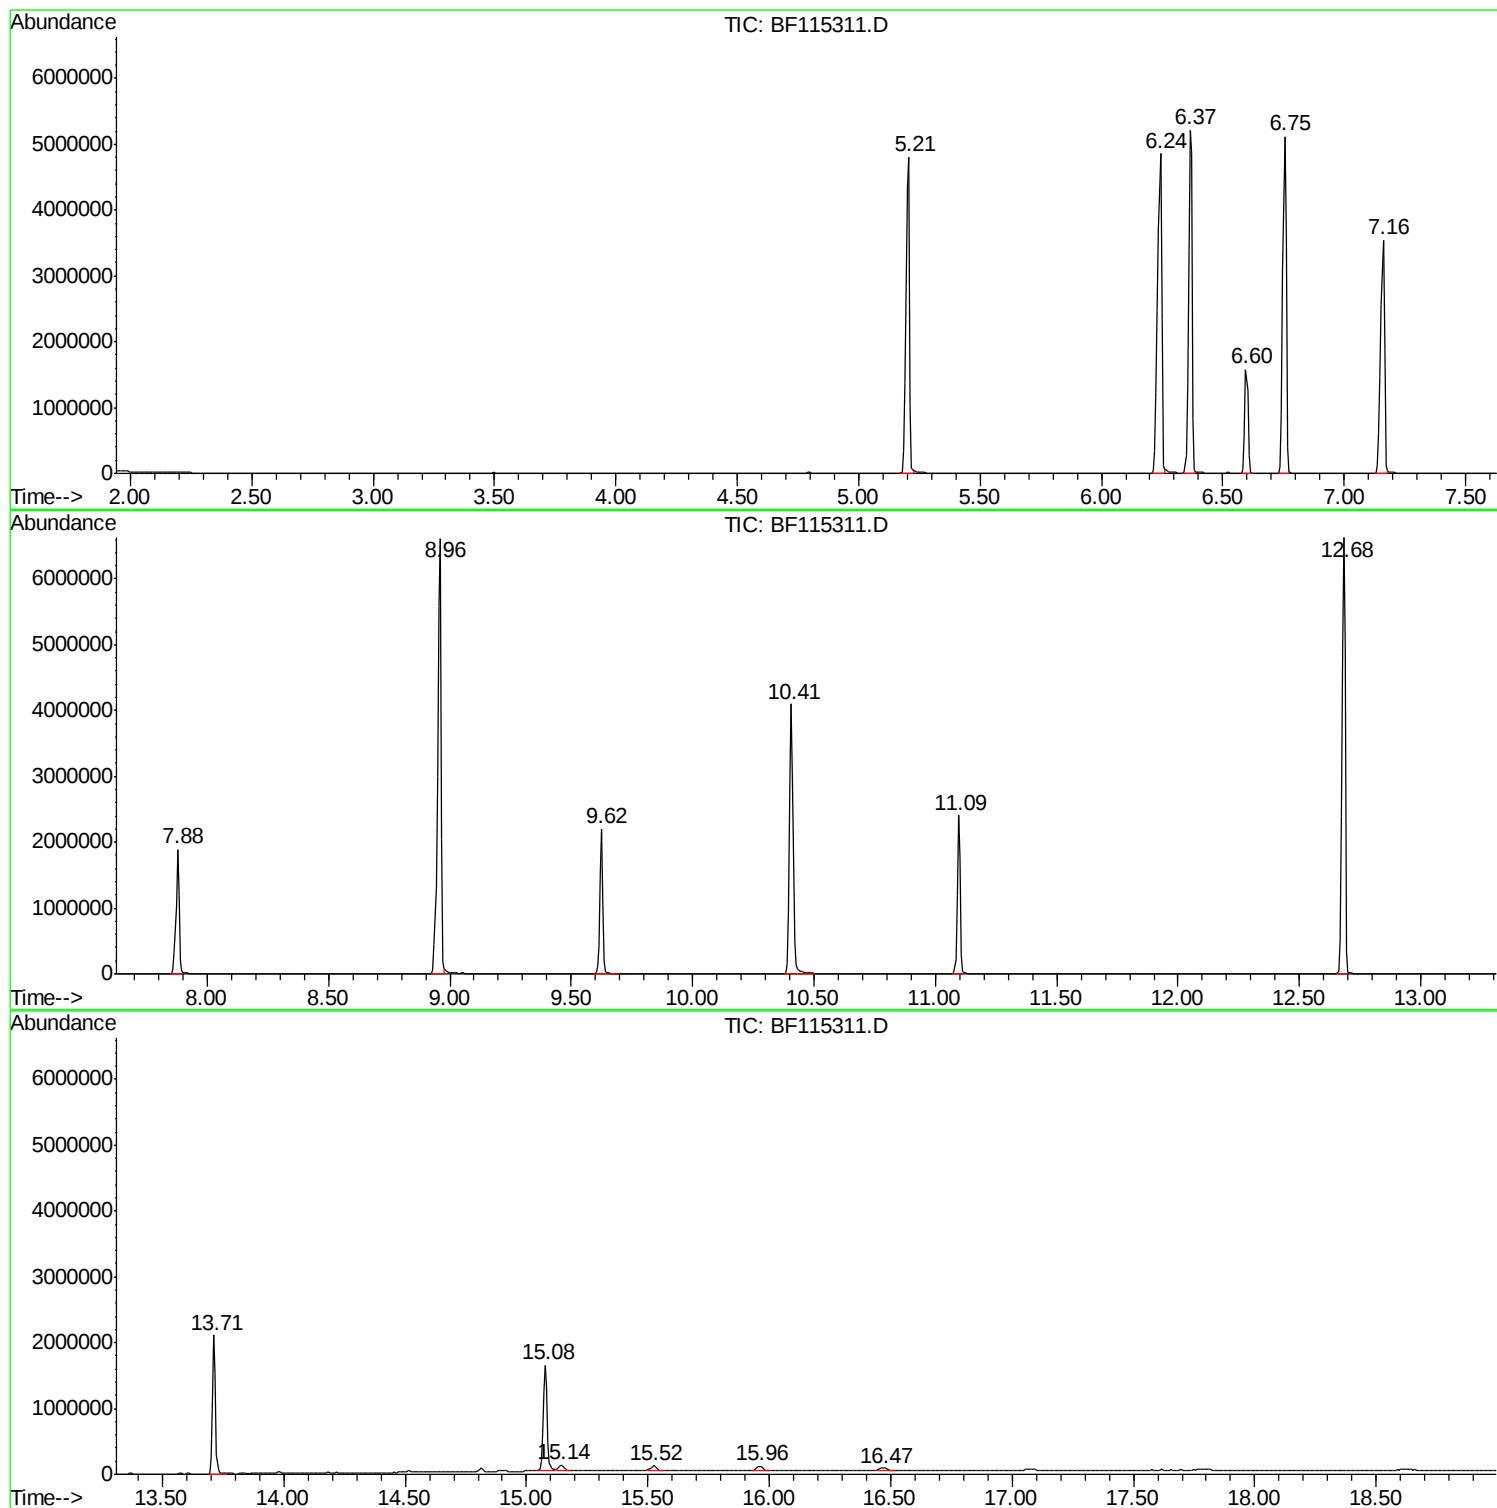

Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_F\DATA\BF062919\
Data File : BF115311.D
Acq On : 29 Jun 2019 9:41
Operator : HP/JU
Sample : PB121004BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121004BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	85.22 ng	5639490	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Amphetaminil	250	C17H18N2	017590-01-1	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

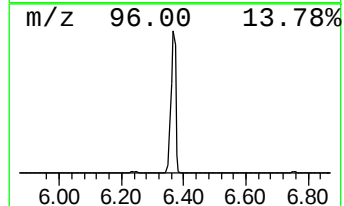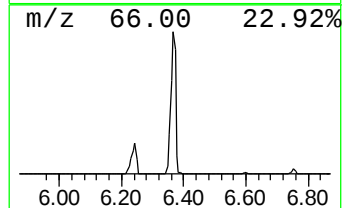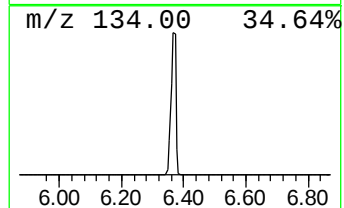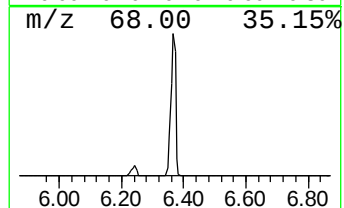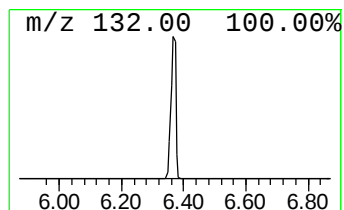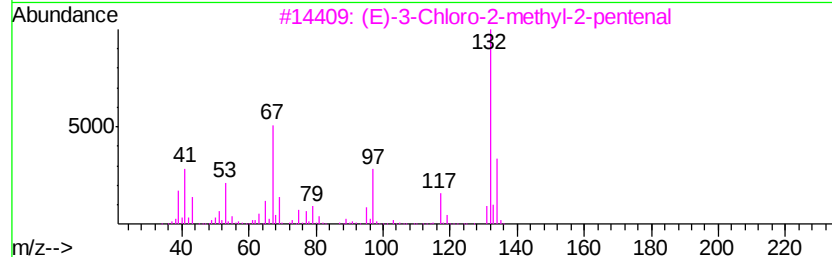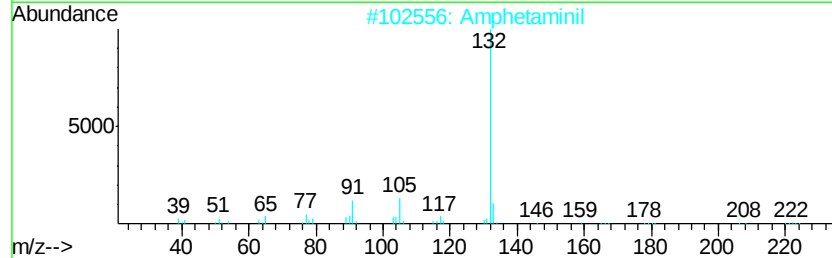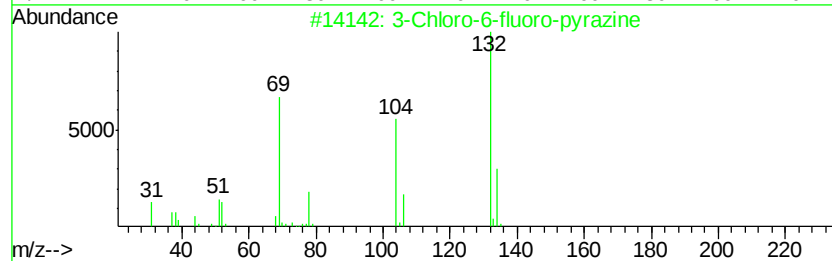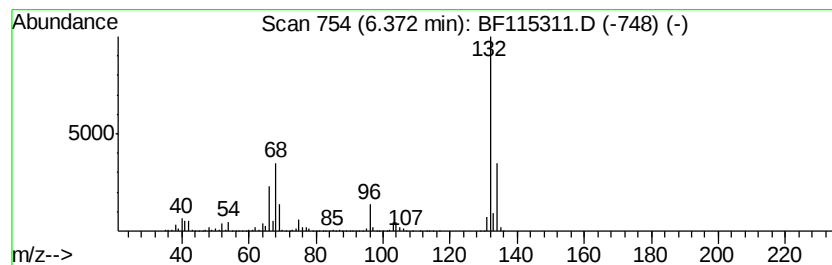

Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_F\DATA\BF062919\
Data File : BF115311.D
Acq On : 29 Jun 2019 9:41
Operator : HP/JU
Sample : PB121004BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121004BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.37	6.37	85.2	ng	5639490	1	6.60	1323510	20.0