


Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_F\DATA\BF062919\
 Data File : BF115307.D
 Acq On : 29 Jun 2019 7:54
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:26:43 2019

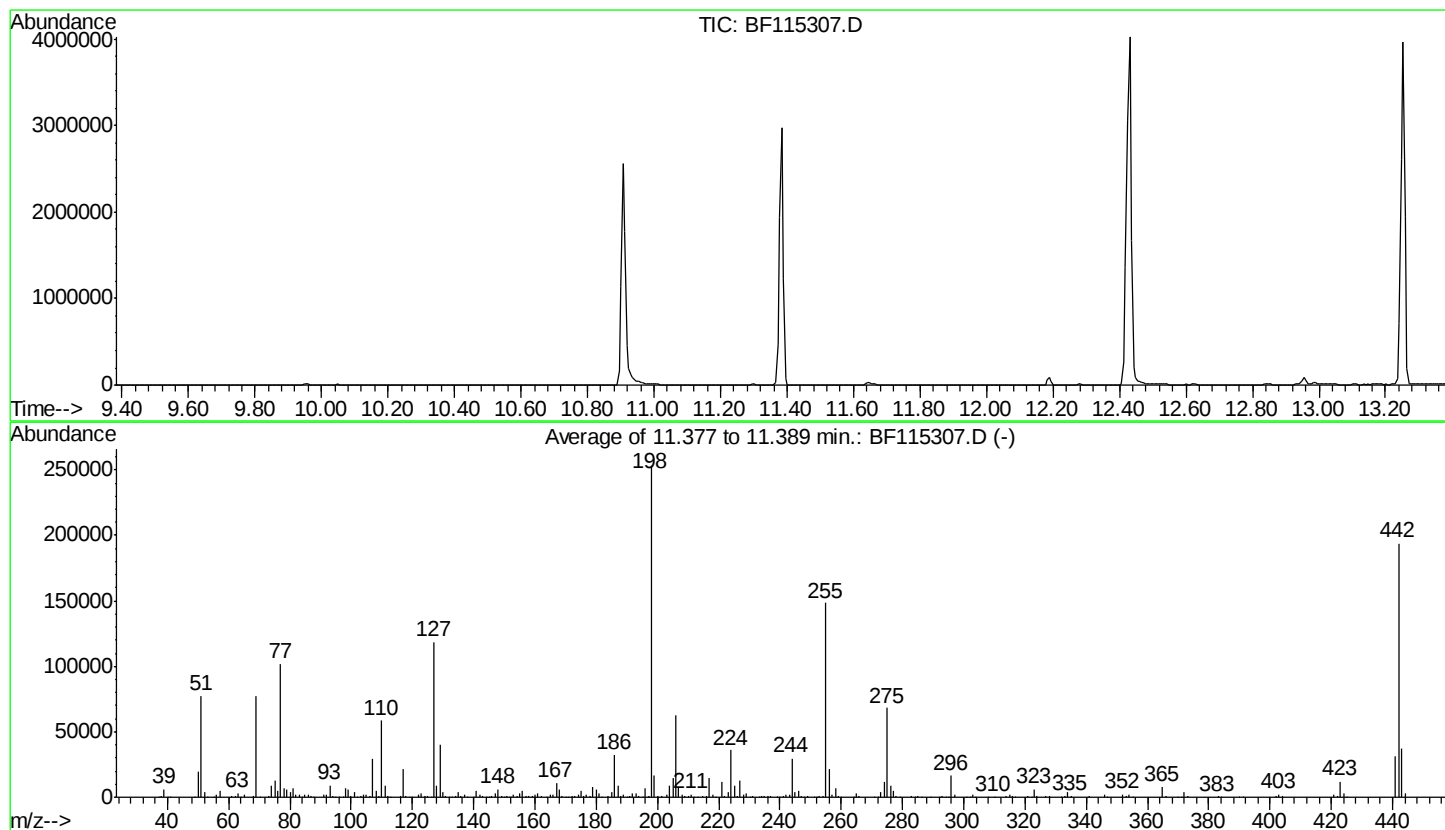

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	77322	PASS
68	69	0.00	2	1.6	1226	PASS
69	198	0.00	100	30.7	77658	PASS
70	69	0.00	2	0.4	348	PASS
127	198	10	80	46.8	118466	PASS
197	198	0.00	2	0.4	1070	PASS
198	198	100	100	100.0	253290	PASS
199	198	5	9	6.7	16983	PASS
275	198	10	60	27.0	68360	PASS
365	198	1	100	3.1	7838	PASS
441	198	0.01	100	12.4	31357	PASS
442	198	50	100	76.5	193741	PASS
443	442	15	24	19.0	36880	PASS