
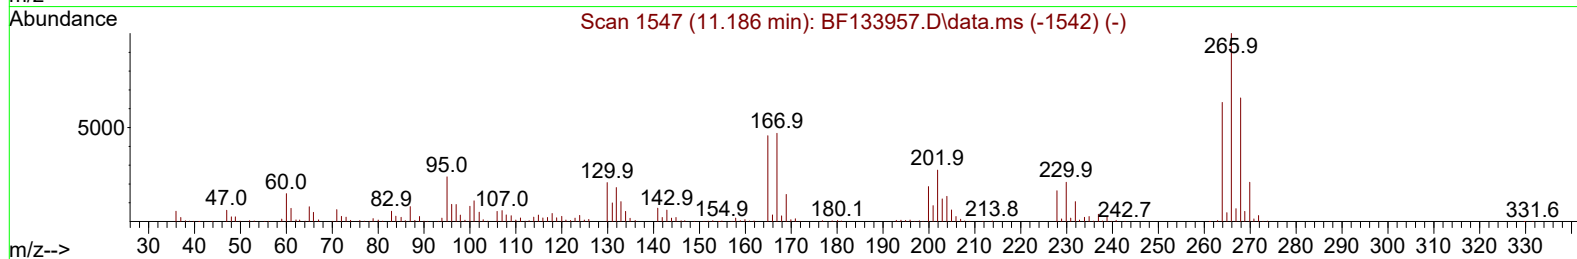
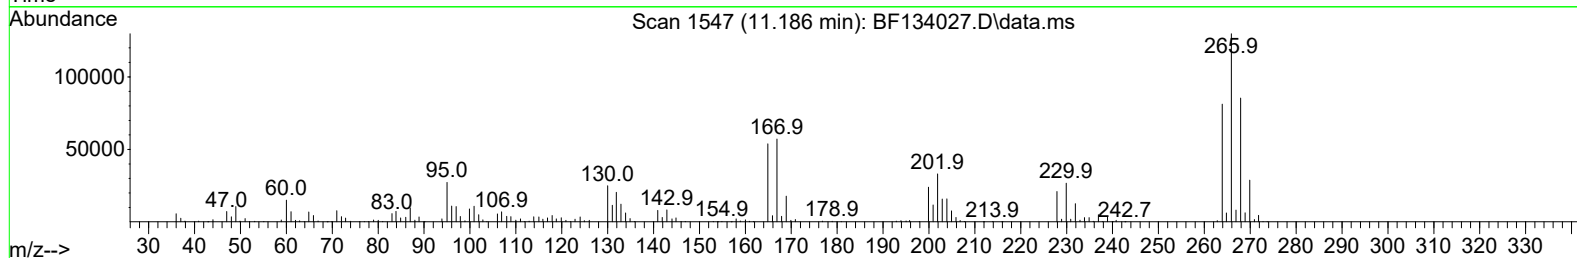


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062923\
 Data File : BF134027.D
 Acq On : 29 Jun 2023 09:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:25:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 23:12:04 2023
 Response via : Initial Calibration

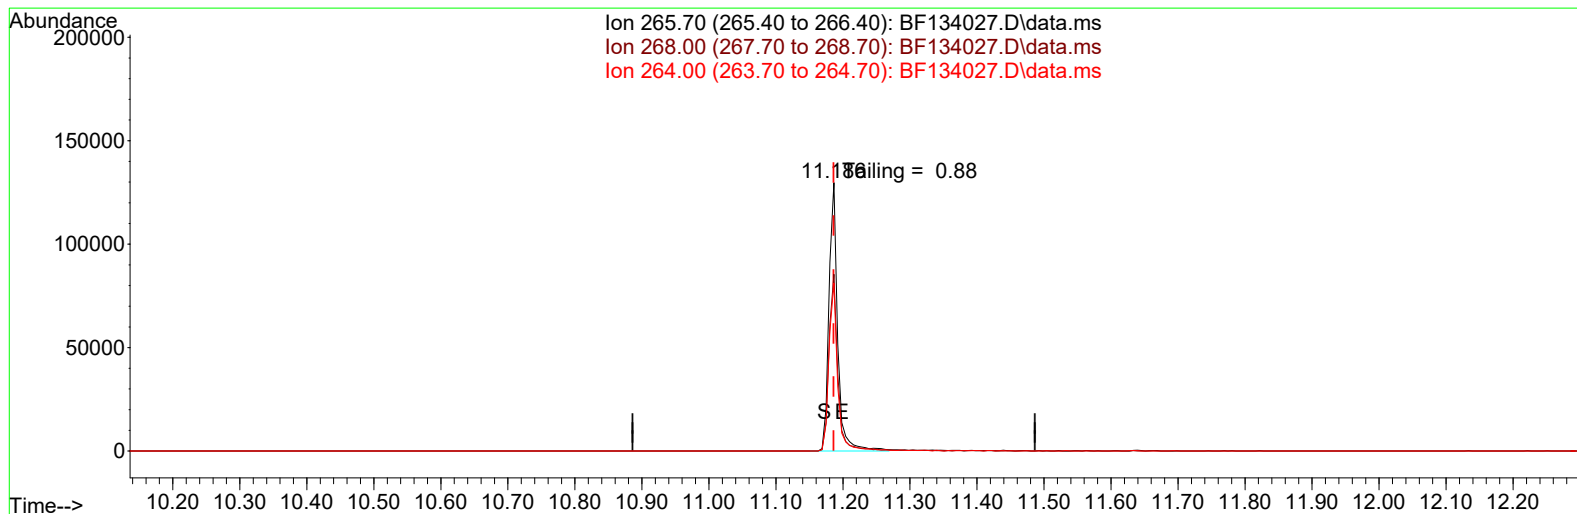

TIC: BF134027.D\data.ms

(70) Pentachlorophenol (C)




11.186min (+ 0.000) 55218.14 ng

response 119230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	65.83
264.00	63.30	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062923\
Data File : BF134027.D
Acq On : 29 Jun 2023 09:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:25:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

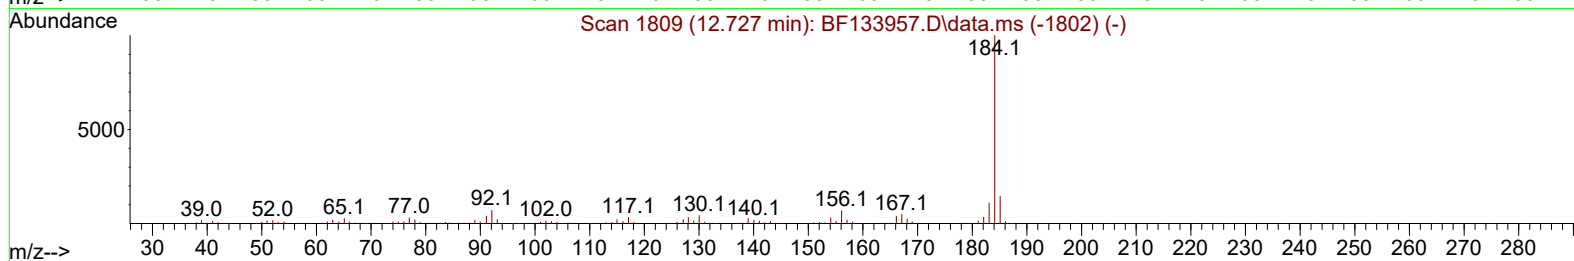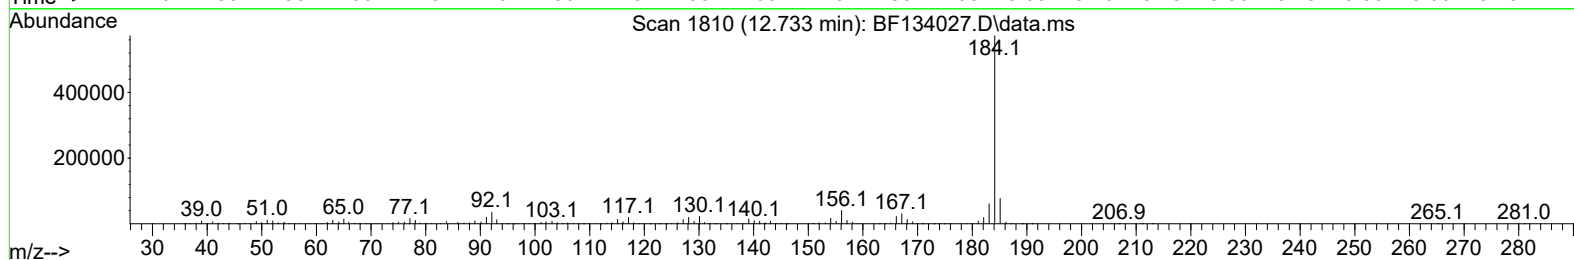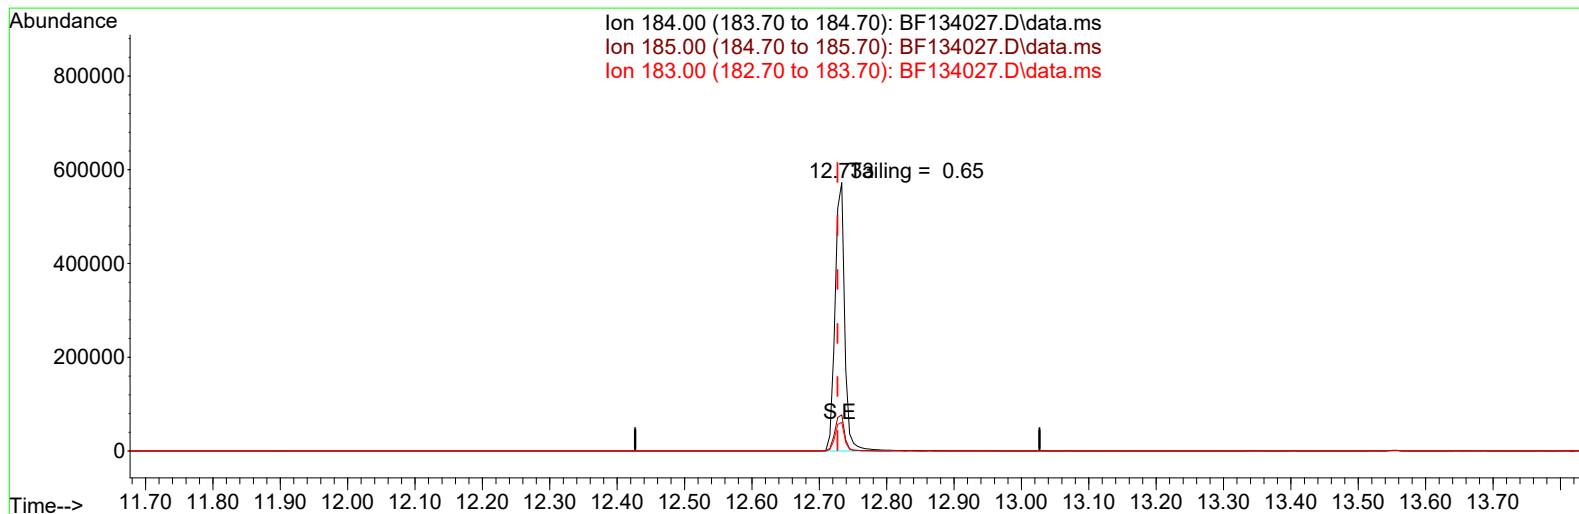

TIC: BF134027.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 41031.47 ng

response 567240

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.48
183.00	11.00	10.69
0.00	0.00	0.00