
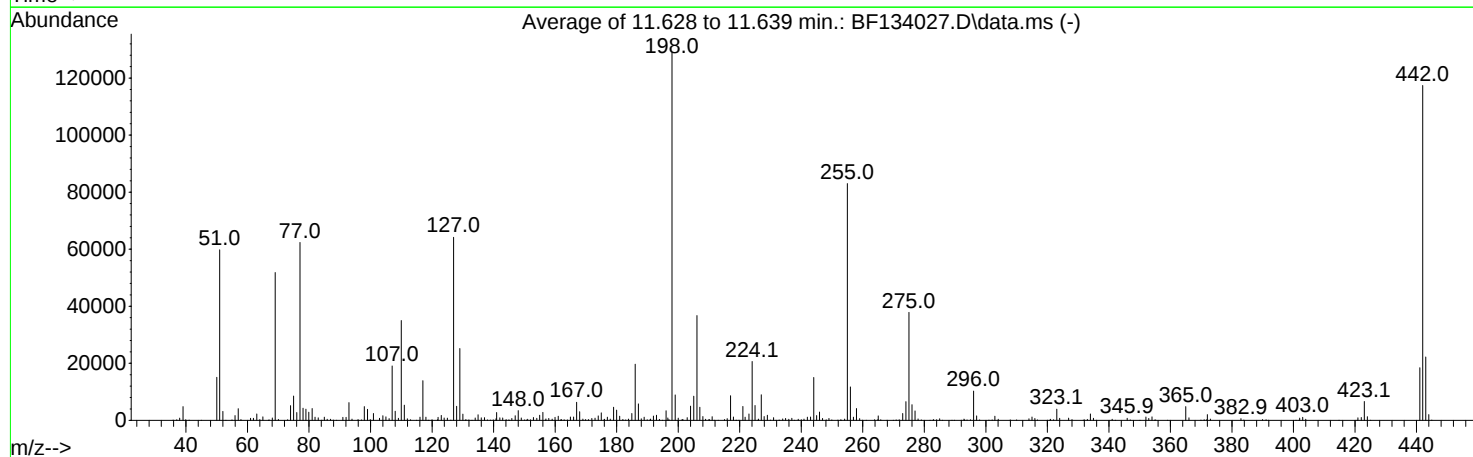


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062923\
 Data File : BF134027.D
 Acq On : 29 Jun 2023 09:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 26 23:12:04 2023

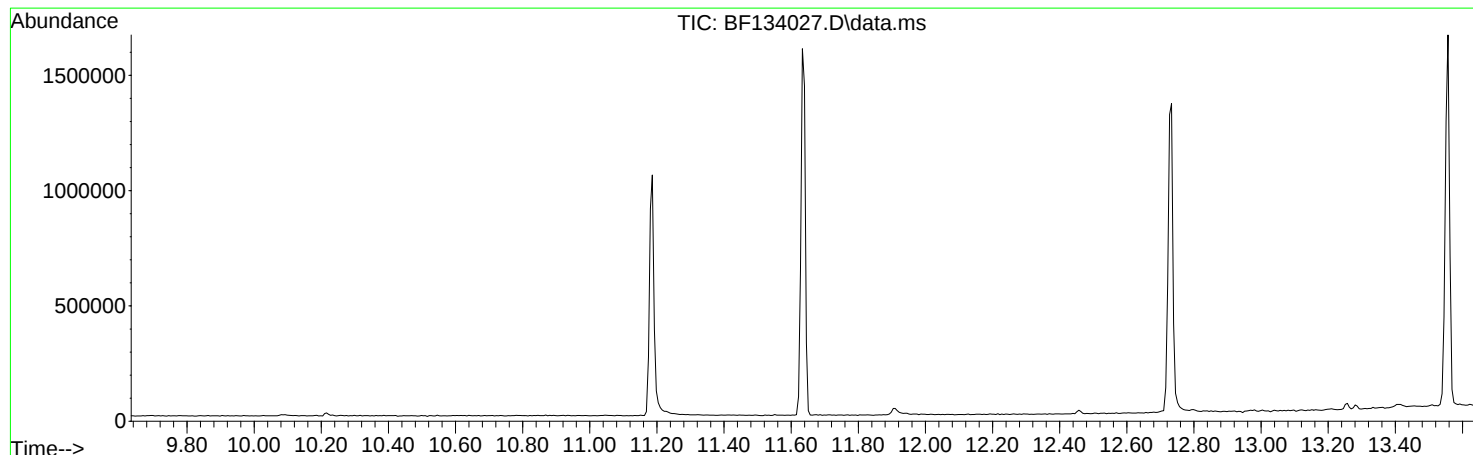

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	59786	PASS
68	69	0.00	2	1.7	859	PASS
69	198	0.00	100	40.2	51824	PASS
70	69	0.00	2	0.6	324	PASS
127	198	10	80	49.8	64179	PASS
197	198	0.00	2	0.2	262	PASS
198	198	100	100	100.0	128965	PASS
199	198	5	9	6.9	8905	PASS
275	198	10	60	29.4	37862	PASS
365	198	1	100	3.8	4847	PASS
441	198	0.01	100	14.3	18472	PASS
442	442	50	100	100.0	117416	PASS
443	442	15	24	18.9	22207	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/29/2023	BNA_F	<u>BF134027.D</u>
Compound Name	Response	Retention Time
DDT	271627	13.557
DDD	7938	13.257
DDE	479	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8417	280044	3.01

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062923\
 Data File : BF134027.D
 Acq On : 29 Jun 2023 09:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 30 08:25:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 23:12:04 2023
 Response via : Initial Calibration

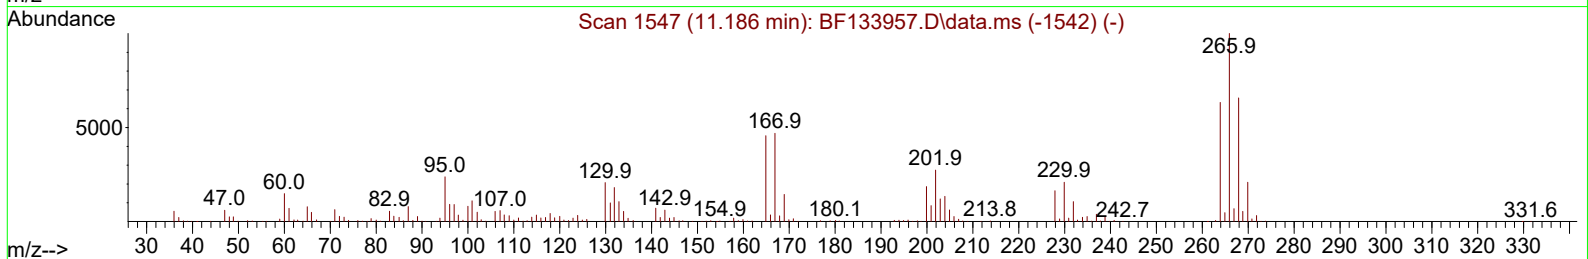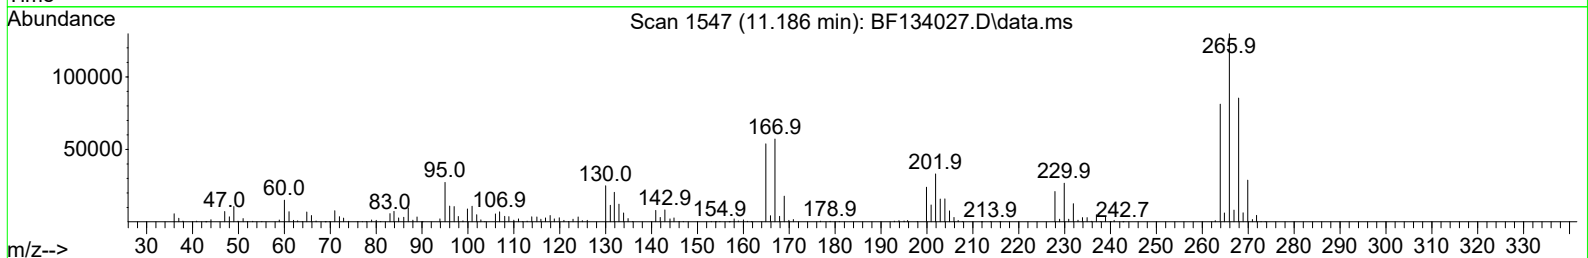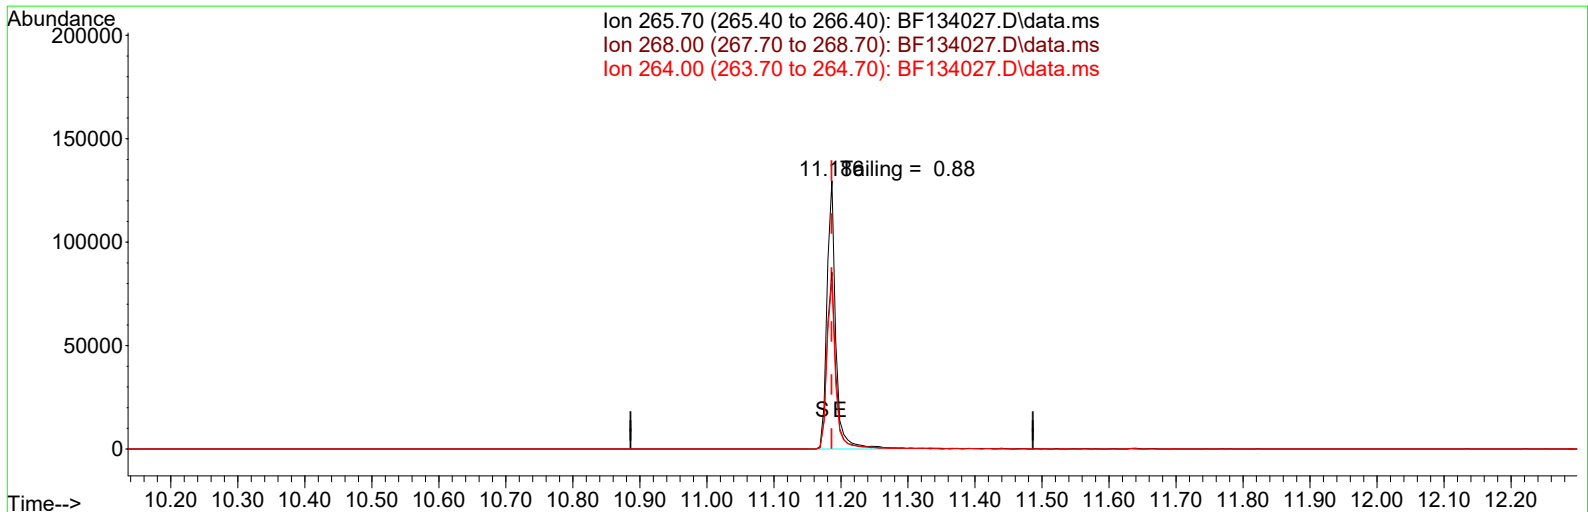

TIC: BF134027.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 55218.14 ng




response 119230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	65.83
264.00	63.30	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062923\
Data File : BF134027.D
Acq On : 29 Jun 2023 09:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 08:25:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

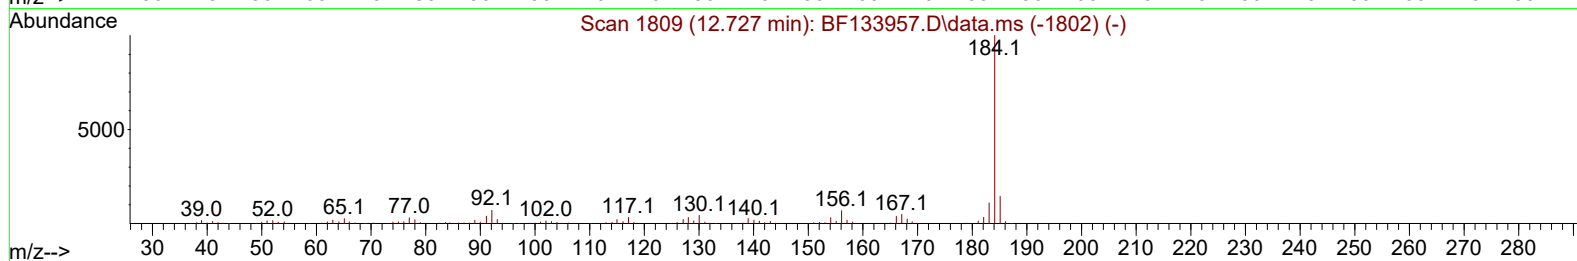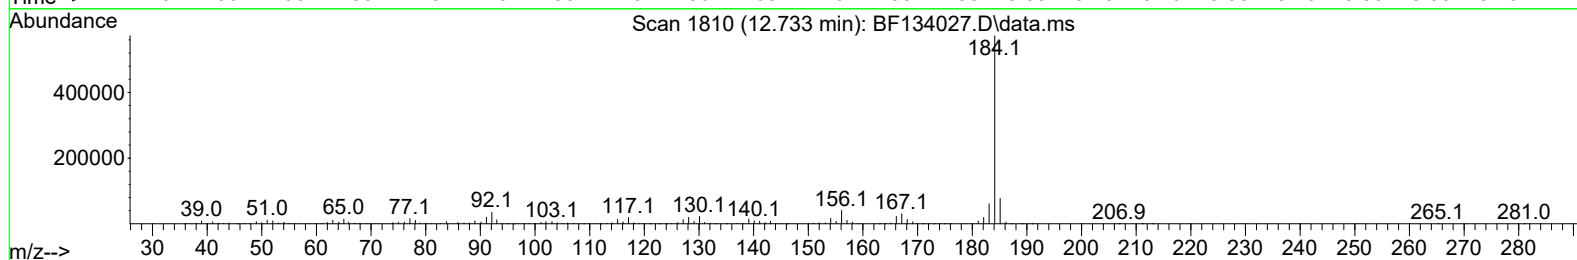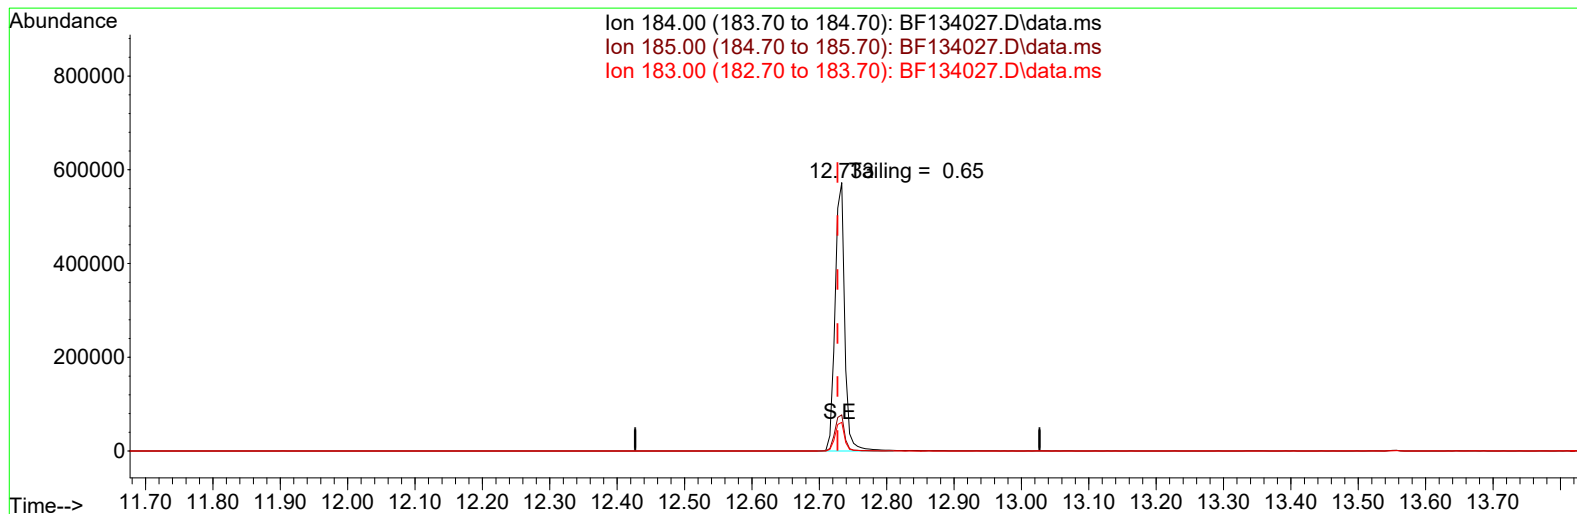

TIC: BF134027.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 41031.47 ng

response 567240

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.48
183.00	11.00	10.69
0.00	0.00	0.00