

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF063018\
 Data File : BF107012.D
 Acq On : 30 Jun 2018 14:09
 Operator : JU/SJ
 Sample : J3600-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jul 02 04:05:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	64581	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	242308	20.00	ng	-0.01
38) Acenaphthene-d10	10.00	164	105828	20.00	ng	-0.01
63) Phenanthrene-d10	11.49	188	196462	20.00	ng	-0.01
75) Chrysene-d12	14.15	240	211732	20.00	ng	-0.02
86) Perylene-d12	15.69	264	162117	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	82689	21.68	ng	-0.01
7) Phenol-d6	6.60	99	99567	20.91	ng	-0.02
23) Nitrobenzene-d5	7.51	82	57654	13.22	ng	-0.02
41) 2,4,6-Tribromophenol	10.79	330	23379	19.06	ng	-0.01
44) 2-Fluorobiphenyl	9.31	172	116216	4.64	ng	-0.02
78) Terphenyl-d14	13.07	244	129805	14.85	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.51	70	7070	2.252	ng	Qvalue # 78
25) Isophorone	7.51	82	57653	7.504	ng	# 64
50) 2,6-Dinitrotoluene	10.00	165	13304	7.916	ng	# 24
51) Acenaphthene	10.02	154	15235	2.308	ng	97
55) 4-Nitrophenol	10.20	139	4329	3.207	ng	# 9
56) 2,4-Dinitrotoluene	10.00	165	13304	6.064	ng	# 21
57) Fluorene	10.54	166	20746	2.893	ng	99
70) Phenanthrene	11.51	178	272668	28.775	ng	99
71) Anthracene	11.57	178	80473	8.320	ng	97
72) Carbazole	11.72	167	27092	2.992	ng	99
74) Fluoranthene	12.71	202	496782	47.565	ng	96
77) Pylene	12.94	202	472351	33.831	ng	99
80) Benzo(a)anthracene	14.14	228	278315	21.567	ng	98
82) Chrysene	14.17	228	247501	20.847	ng	98
85) Indeno(1,2,3-cd)pyrene	17.27	276	92187	9.150	ng	# 87
87) Benzo(b)fluoranthene	15.23	252	366331	36.376	ng	# 95
88) Benzo(k)fluoranthene	15.35	252	45250	4.718	ng	95
89) Benzo(a)pyrene	15.55	252	126373	14.116	ng	97
90) Dibenzo(a,h)anthracene	17.45	278	19305	2.544	ng	92
91) Benzo(a,h,i)perylene	17.75	276	93681	12.633	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF063018\
Data File : BF107012.D
Acq On : 30 Jun 2018 14:09
Operator : JU/SJ
Sample : J3600-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 02 04:05:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

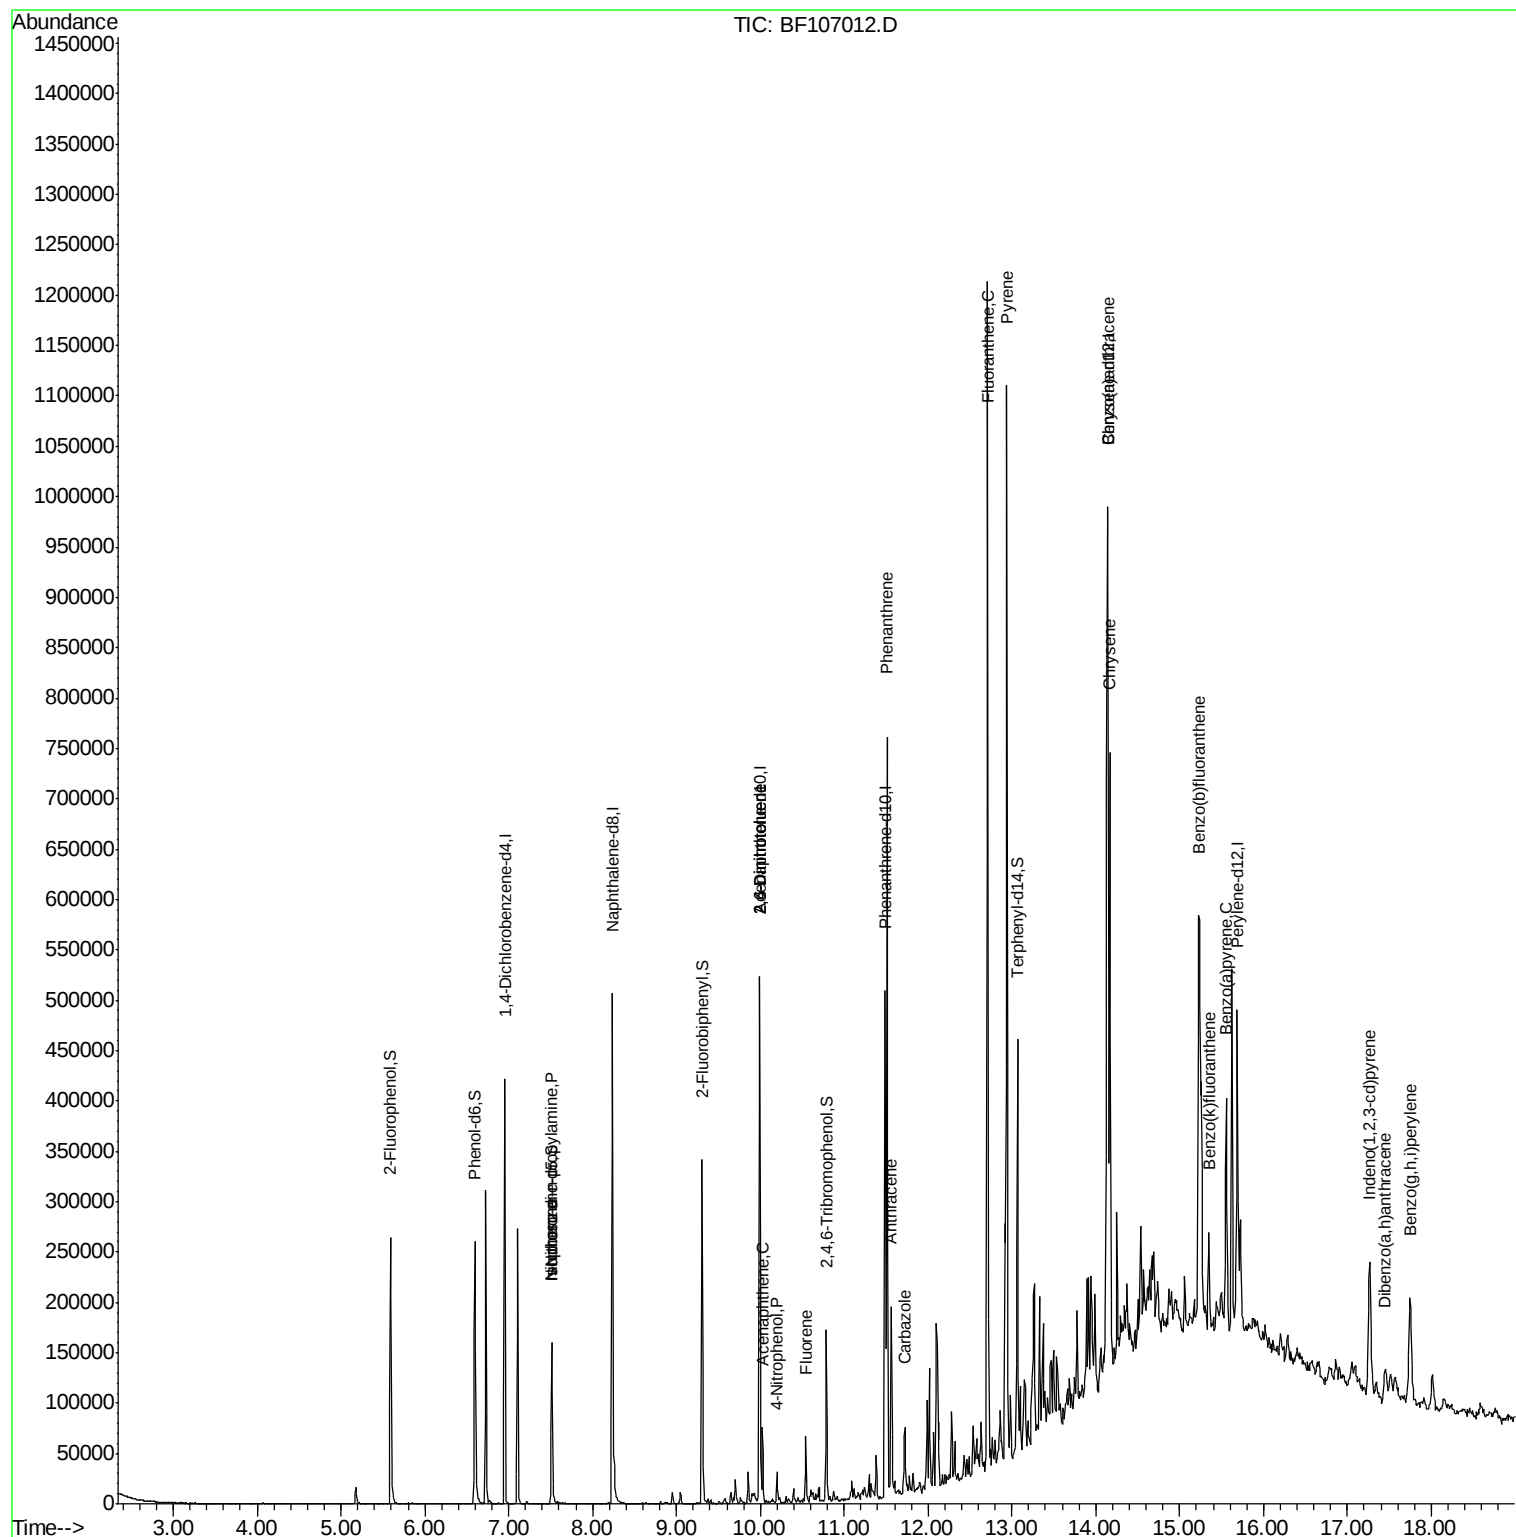




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 64581
Ion Ratio Lower Upper
152 100
150 159.3 124.6 186.8
115 56.4 50.1 75.1

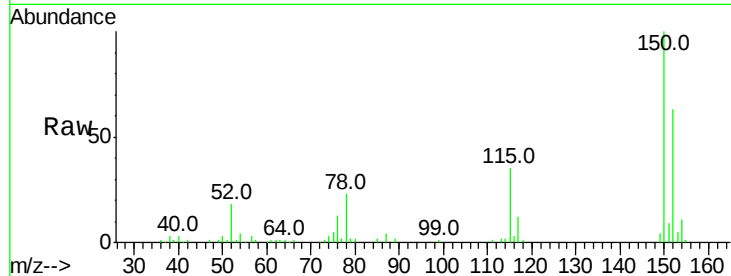


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

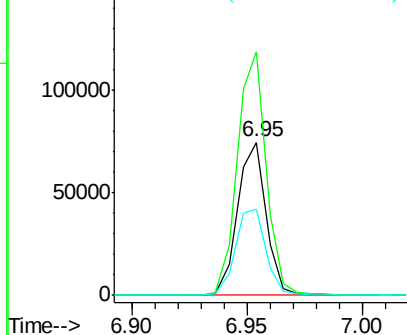



#5

2-Fluorophenol
Concen: 21.681 ng
RT: 5.59 min Scan# 553
Delta R.T. -0.01 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Tgt Ion:112 Resp: 82689
Ion Ratio Lower Upper
112 100
64 59.8 47.9 71.9
63 27.6 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

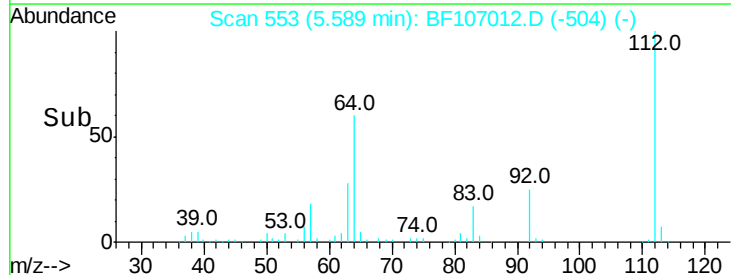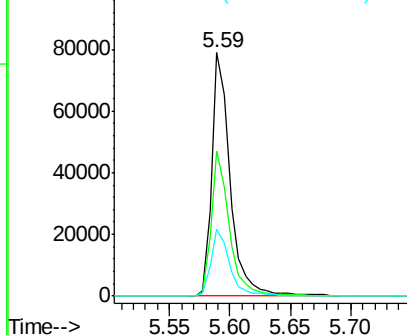



#7

Phenol-d6

Concen: 20.905 ng

RT: 6.60 min Scan# 724

Delta R.T. -0.02 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 99567

Ion Ratio Lower Upper




99 100

42 16.2 14.5 21.7

71 32.7 25.4 38.0

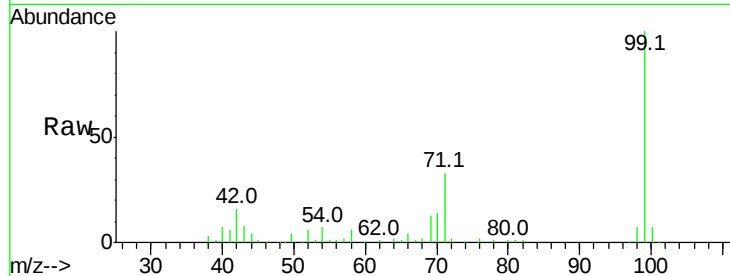

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

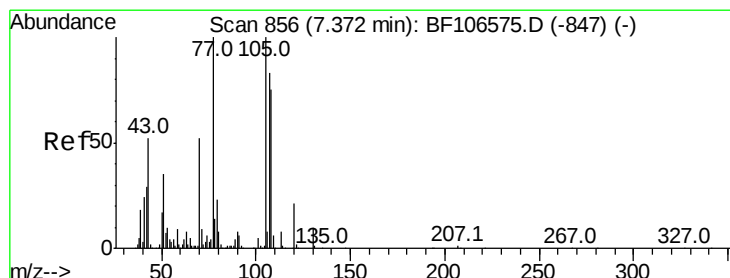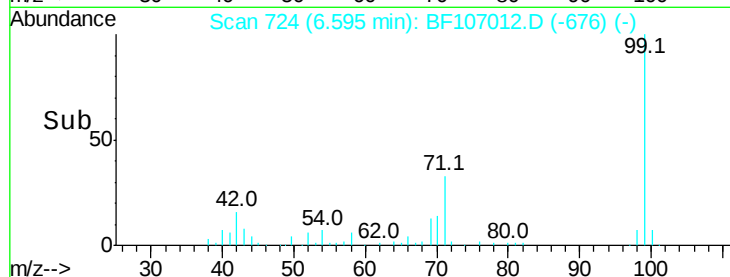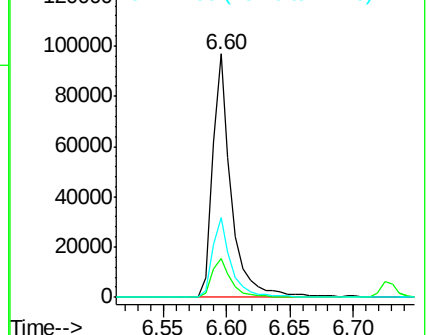

#19

n-Nitroso-di-n-propylamine

Concen: 2.252 ng

RT: 7.51 min Scan# 880

Delta R.T. 0.13 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Tgt Ion: 70 Resp: 7070


Ion Ratio Lower Upper

70 100



42 48.7 47.5 71.3

101 0.0 7.4 11.2#

130 0.0 16.6 25.0#

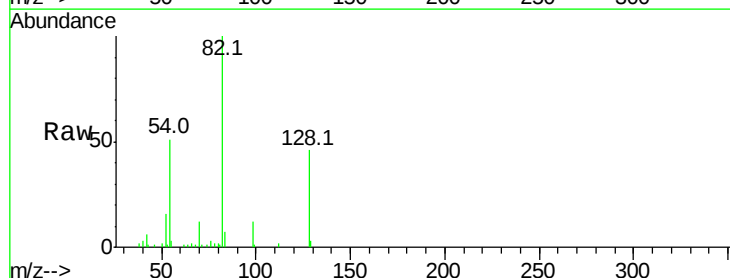

Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1

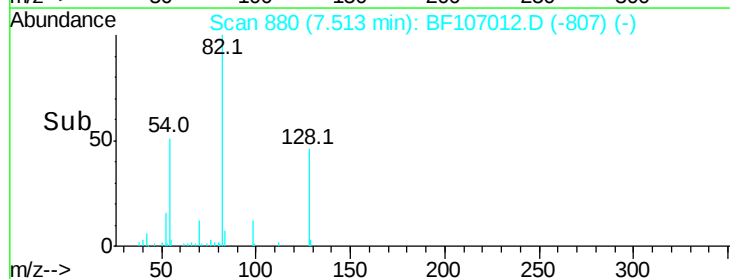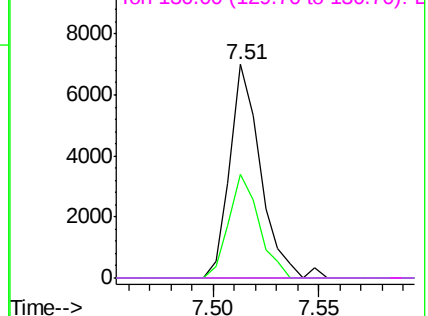







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.24 min Scan# 1003
Delta R.T. -0.01 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	136	Resp:	242308
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	8.0	6.6	9.8
68	5.7	5.0	7.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

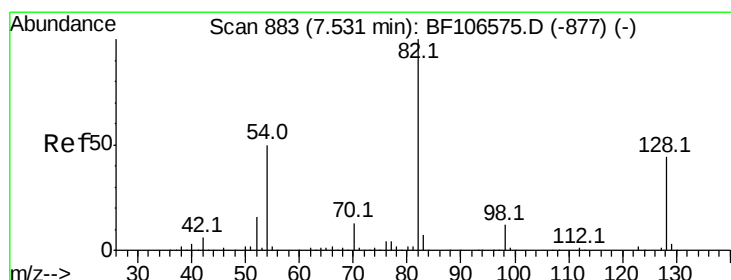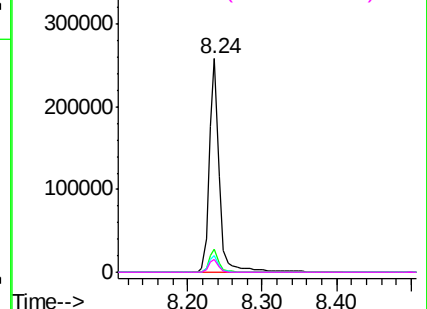




#23
Nitrobenzene-d5
Concen: 13.223 ng
RT: 7.51 min Scan# 880
Delta R.T. -0.02 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Tgt Ion:	82	Resp:	57654
Ion	Ratio	Lower	Upper
82	100		
128	45.6	36.1	54.1
54	50.9	41.4	62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

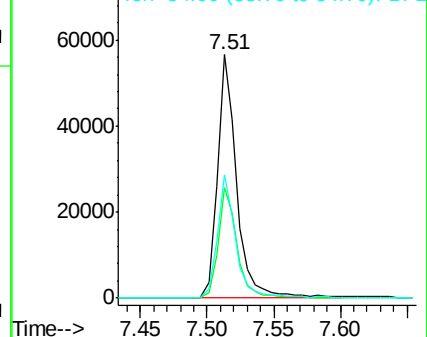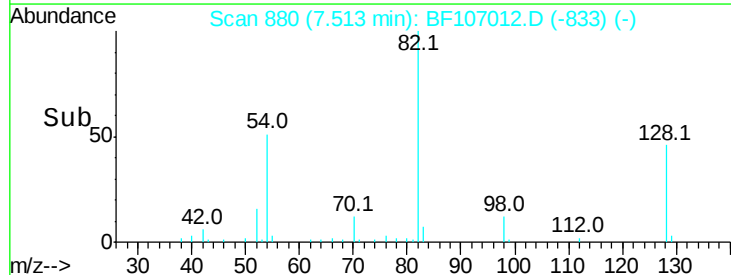

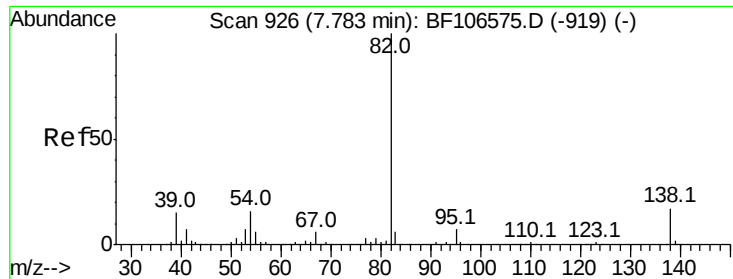

#25

Isophorone

Concen: 7.504 ng

RT: 7.51 min Scan# 880

Delta R.T. -0.28 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 57653

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

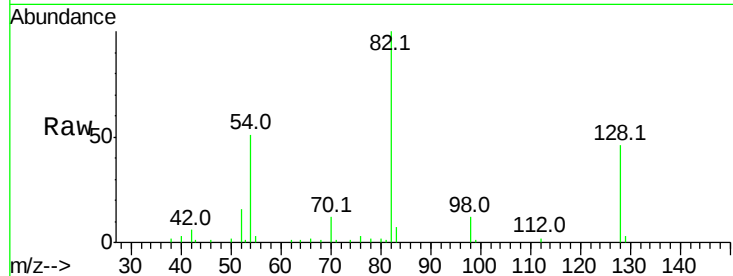

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

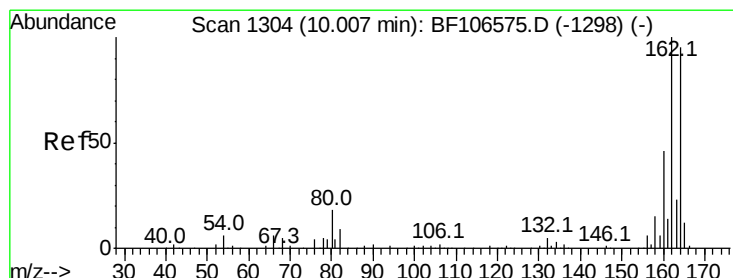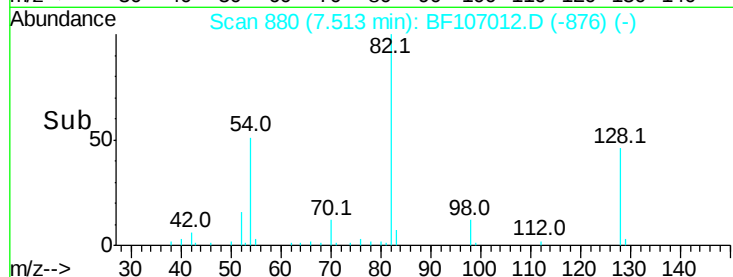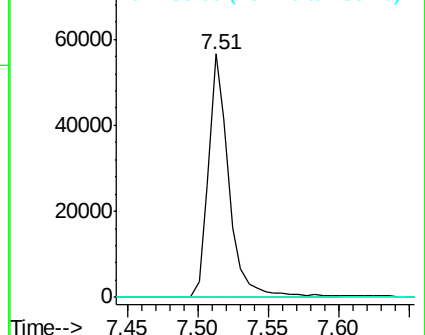

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.00 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09


Tgt Ion: 164 Resp: 105828

Ion Ratio Lower Upper

164 100

162 98.8 86.1 129.1



160 43.0 38.3 57.5

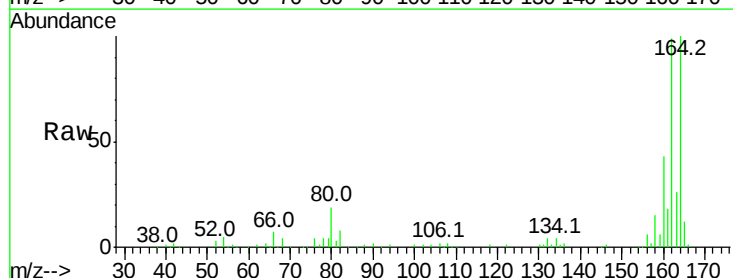

Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

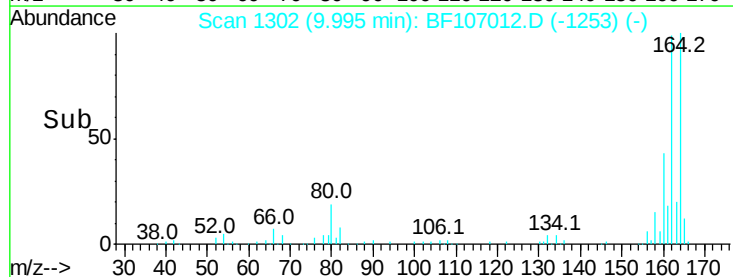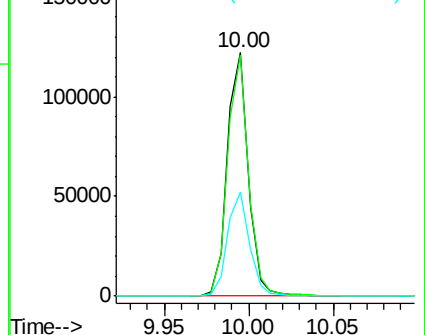







#41
 2,4,6-Tribromophenol
 Concen: 19.060 ng
 RT: 10.79 min Scan# 1437
 Delta R.T. -0.01 min
 Lab File: BF107012.D
 Acq: 30 Jun 2018 14:09

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 23379
 Ion Ratio Lower Upper
 330 100
 332 95.2 77.0 115.6
 141 24.6 29.9 44.9#

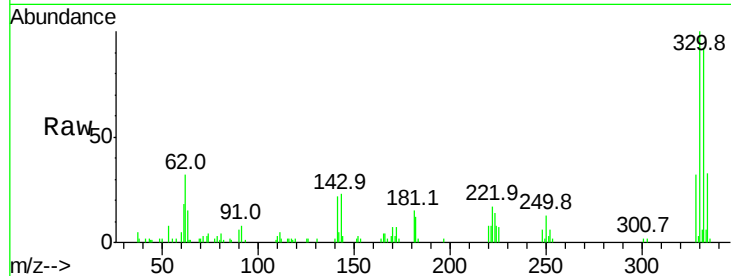


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

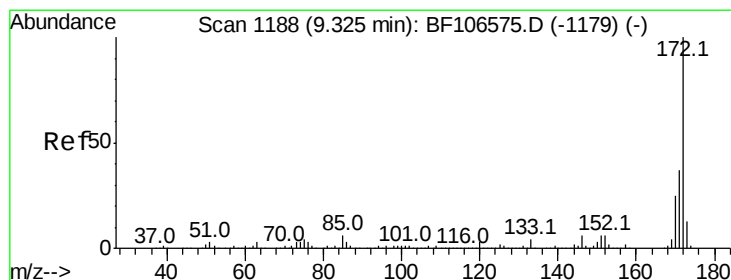
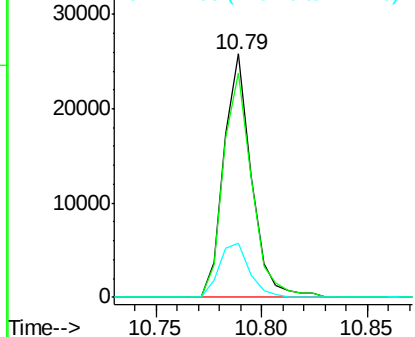



#44
 2-Fluorobiphenyl
 Concen: 4.642 ng
 RT: 9.31 min Scan# 1185
 Delta R.T. -0.02 min
 Lab File: BF107012.D
 Acq: 30 Jun 2018 14:09

Tgt Ion:172 Resp: 116216
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.7 44.5
 170 23.5 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

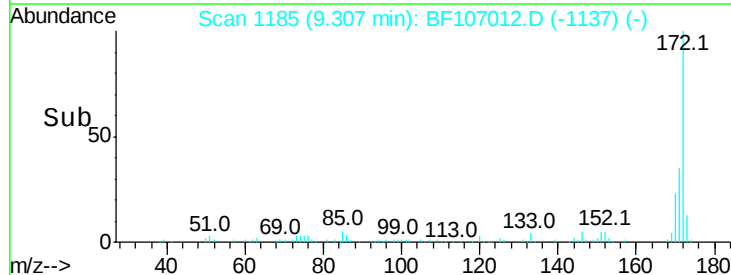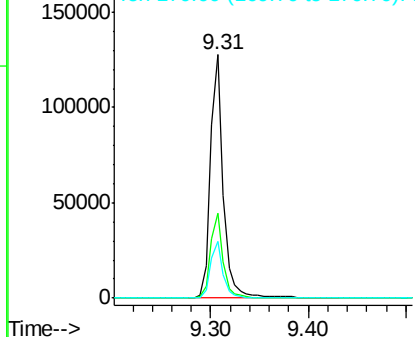


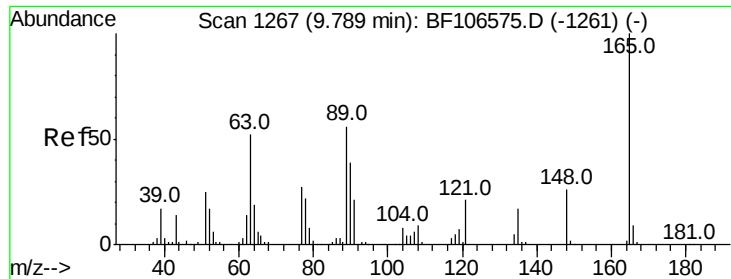




#50
2,6-Dinitrotoluene
Concen: 7.916 ng
RT: 10.00 min Scan# 1302
Delta R.T. 0.20 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:165 Resp: 13304
Ion Ratio Lower Upper
165 100
63 0.0 44.7 67.1#
89 0.0 44.0 66.0#




Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

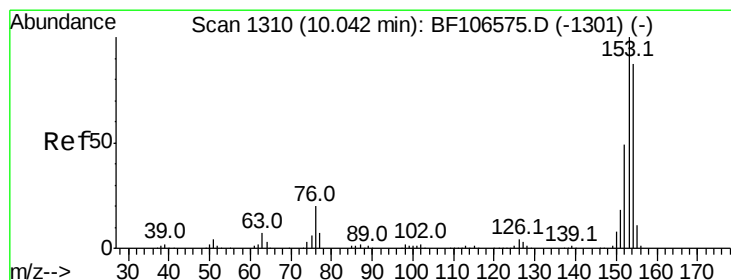
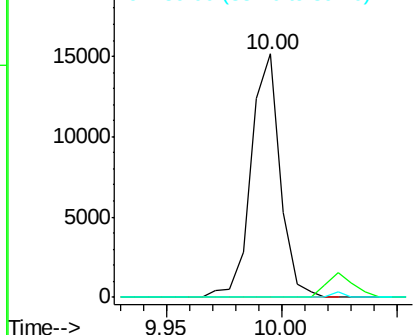



#51
Acenaphthene
Concen: 2.308 ng
RT: 10.02 min Scan# 1307
Delta R.T. -0.02 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Tgt Ion:154 Resp: 15235
Ion Ratio Lower Upper
154 100
153 116.8 91.2 136.8
152 51.7 43.8 65.8



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E

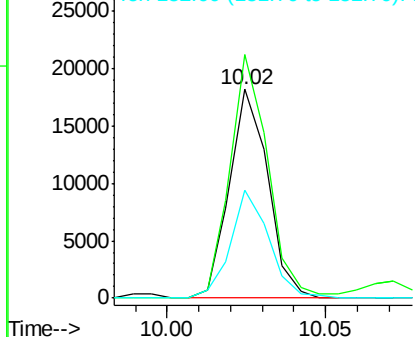







#55
4-Nitrophenol
Concen: 3.207 ng
RT: 10.20 min Scan# 1337
Delta R.T. 0.06 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Instrument :
BNA_F
ClientSampleId :

Tot Ion:139 Resp: 4329
Ion Ratio Lower Upper
139 100
109 0.0 48.4 88.4#
65 0.0 72.6 112.6#

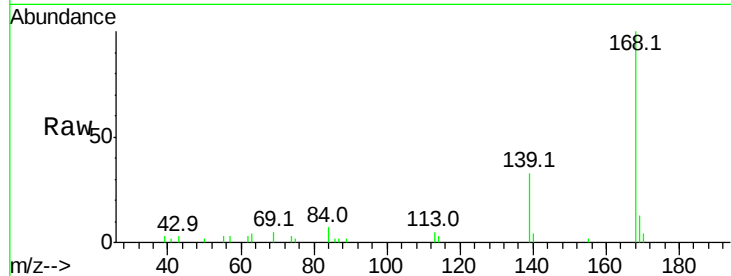


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF1

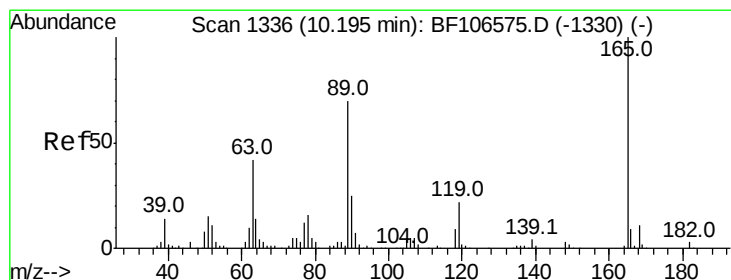
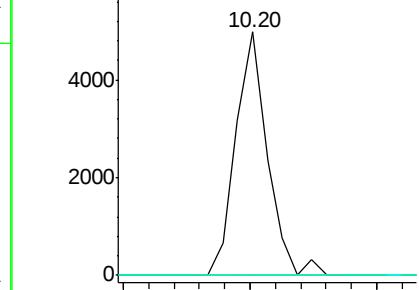



#56
2,4-Dinitrotoluene
Concen: 6.064 ng
RT: 10.00 min Scan# 1302
Delta R.T. -0.21 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Tgt Ion:165 Resp: 13304
Ion Ratio Lower Upper
165 100
63 0.0 36.4 54.6#
89 0.0 57.8 86.6#
182 0.0 1.6 2.4#



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): E



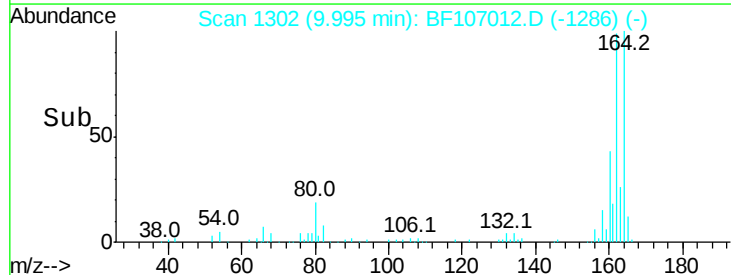
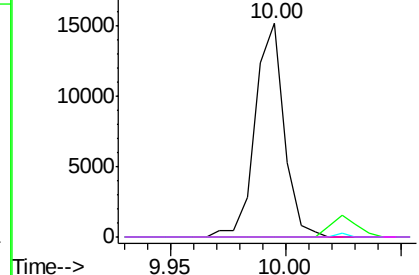




#57
 Fluorene
 Concen: 2.893 ng
 RT: 10.54 min Scan# 1395
 Delta R.T. -0.02 min
 Lab File: BF107012.D
 Acq: 30 Jun 2018 14:09




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
166	100		
165	100.4	79.8	119.8
167	15.3	10.6	16.0

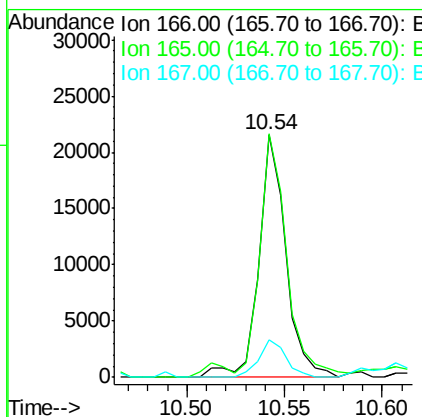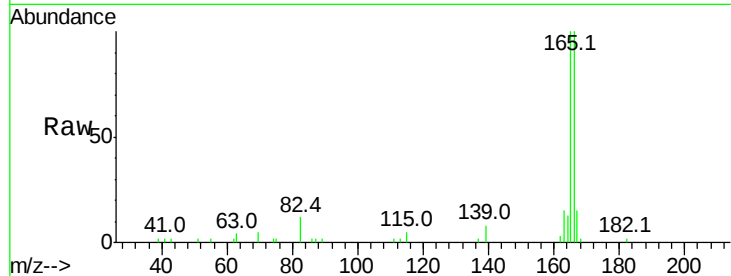

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.49 min Scan# 1556
 Delta R.T. -0.01 min
 Lab File: BF107012.D
 Acq: 30 Jun 2018 14:09

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.6	8.5	12.7#
80	8.6	9.2	13.8#


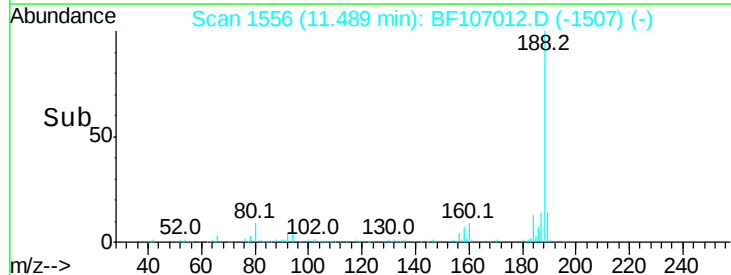
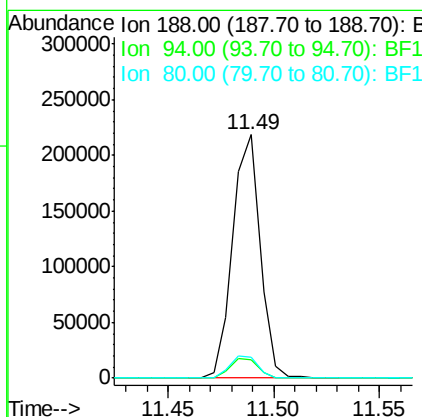





#70
Phenanthrene
Concen: 28.775 ng
RT: 11.51 min Scan# 1560
Delta R.T. -0.01 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09




Instrument :
BNA_F
ClientSampleId :


Tot Ion:178 Resp: 272668
Ion Ratio Lower Upper
178 100
176 19.6 15.8 23.8
179 15.4 13.0 19.6

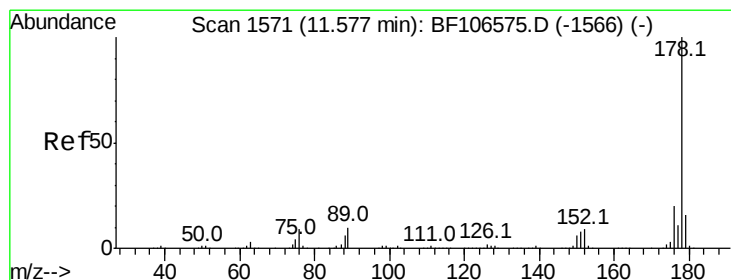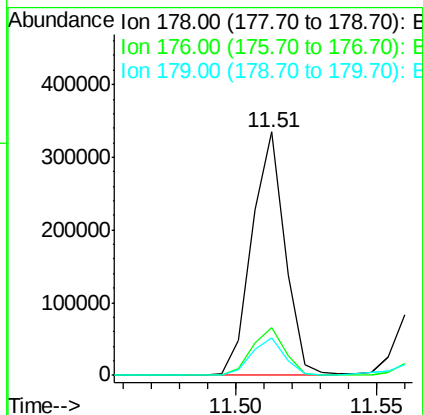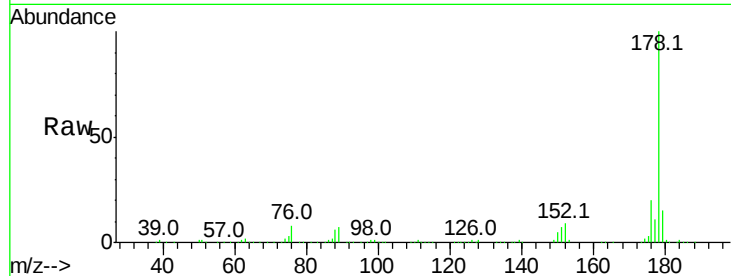

#71
Anthracene
Concen: 8.320 ng
RT: 11.57 min Scan# 1569
Delta R.T. -0.01 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Tgt Ion:178 Resp: 80473
Ion Ratio Lower Upper
178 100
176 18.0 15.4 23.2
179 14.6 12.6 19.0

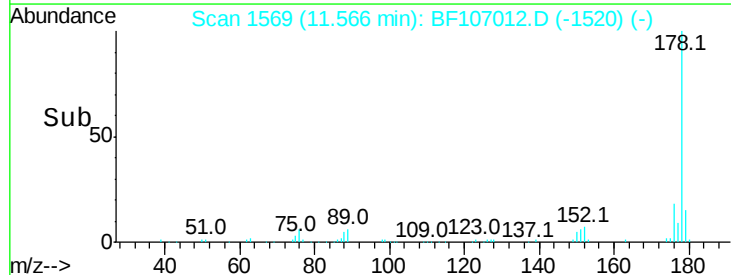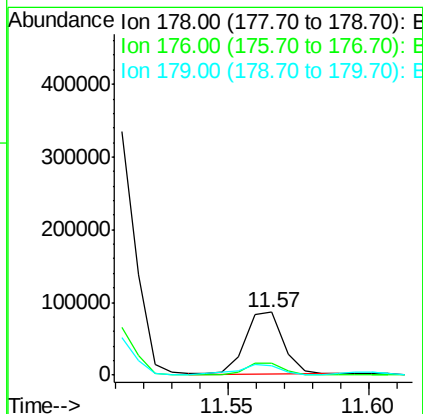



#72

Carbazole

Concen: 2.992 ng

RT: 11.72 min Scan# 1596

Delta R.T. -0.01 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion:167 Resp: 27092

Ion Ratio Lower Upper

167 100

166 21.9 17.6 26.4




139 12.3 10.9 16.3



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

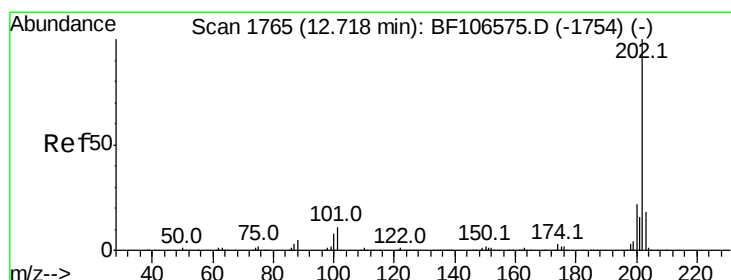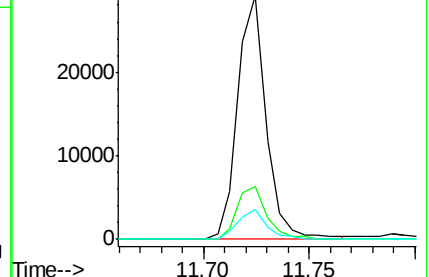

#74

Fluoranthene

Concen: 47.565 ng

RT: 12.71 min Scan# 1763

Delta R.T. -0.01 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09


Tgt Ion:202 Resp: 496782

Ion Ratio Lower Upper

202 100

101 10.9 0.0 34.1



203 17.9 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

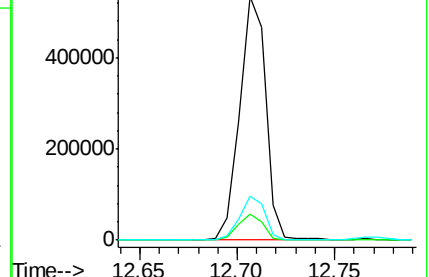



#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2008

Delta R.T. -0.02 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Instrument :

BNA_F

ClientSampled :


Tot Ion:240 Resp: 211732

Ion Ratio Lower Upper

240 100

120 7.4 9.5 14.3#




236 25.5 20.7 31.1

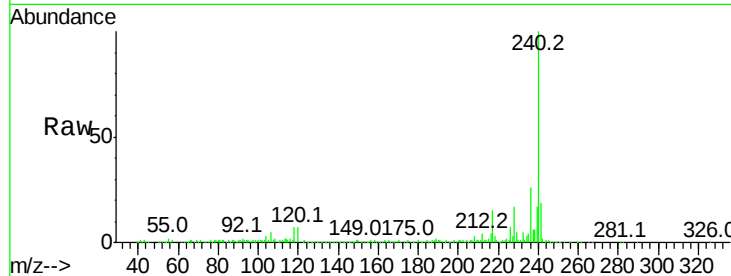

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

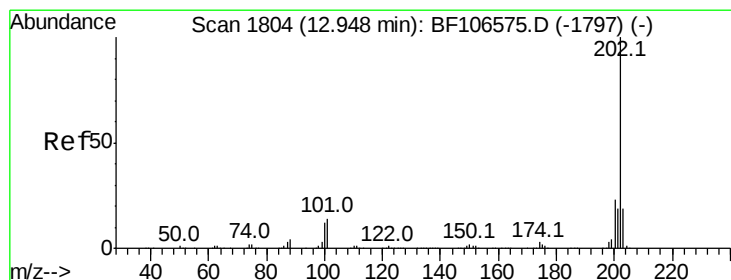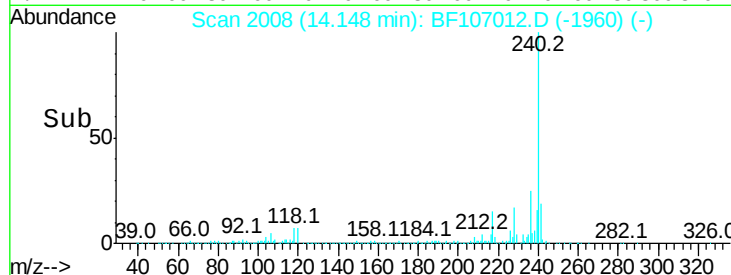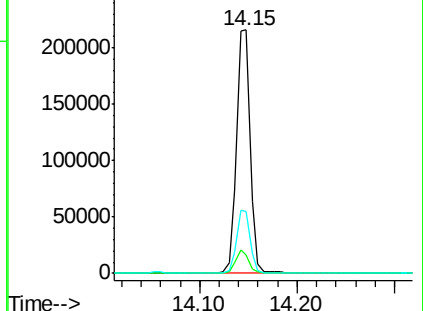

#77

Pyrene

Concen: 33.831 ng

RT: 12.94 min Scan# 1803

Delta R.T. -0.01 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09


Tgt Ion:202 Resp: 472351

Ion Ratio Lower Upper

202 100

200 21.5 17.4 26.2



203 17.6 14.3 21.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

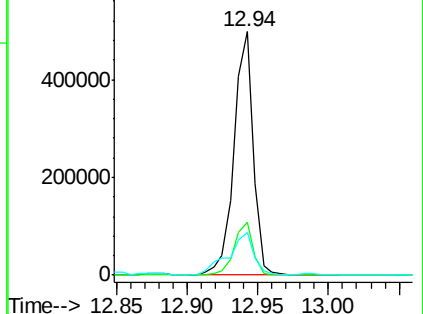



#78

Terphenyl-d14

Concen: 14.850 ng

RT: 13.07 min Scan# 1824

Delta R.T. -0.02 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 129805

Ion Ratio Lower Upper

244 100

212 6.0 5.4 8.0




122 9.2 11.0 16.4#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

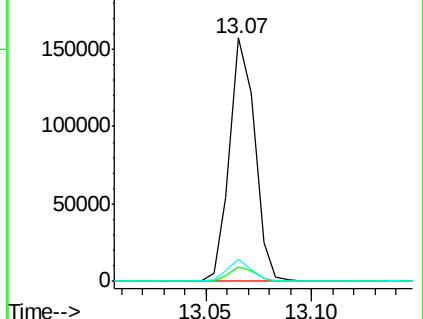

#80

Benzo(a)anthracene

Concen: 21.567 ng

RT: 14.14 min Scan# 2006

Delta R.T. -0.02 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09


Tgt Ion:228 Resp: 278315

Ion Ratio Lower Upper

228 100

226 29.3 22.6 33.8



229 20.6 15.8 23.6




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

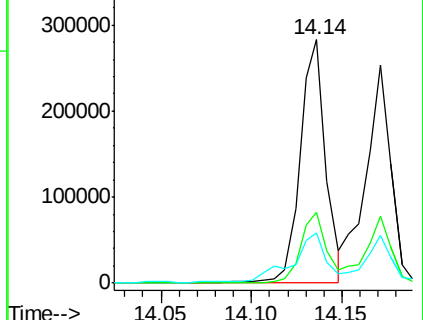



#82

Chrysene

Concen: 20.847 ng

RT: 14.17 min Scan# 2012

Delta R.T. -0.02 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Instrument :

BNA_F

ClientSampleId :


Tot Ion:228 Resp: 247501

Ion Ratio Lower Upper

228 100

226 30.5 25.0 37.6




229 21.7 16.2 24.4

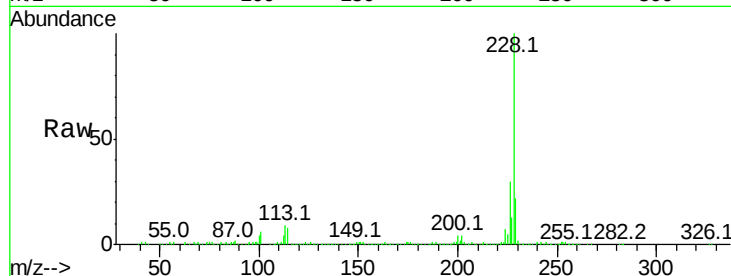

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

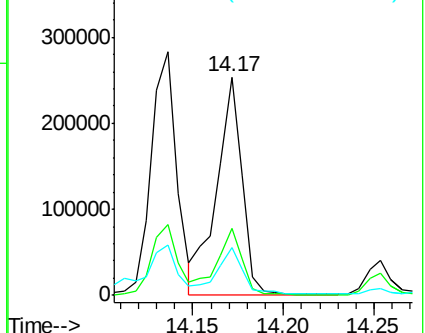

#85

Indeno(1,2,3-cd)pyrene

Concen: 9.150 ng

RT: 17.27 min Scan# 2538

Delta R.T. -0.04 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09


Tgt Ion:276 Resp: 92187

Ion Ratio Lower Upper

276 100

138 18.6 25.0 37.6#



277 24.5 20.1 30.1




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E




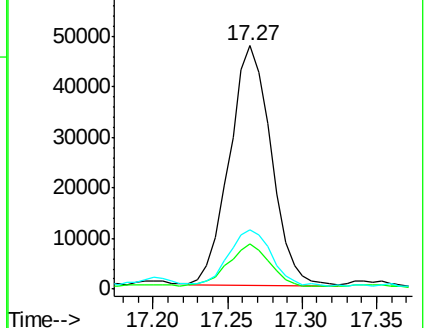




#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.69 min Scan# 2270
Delta R.T. -0.03 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.2	28.8
265	22.3	17.5	26.3

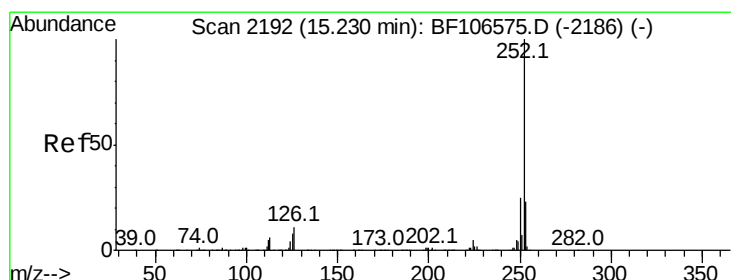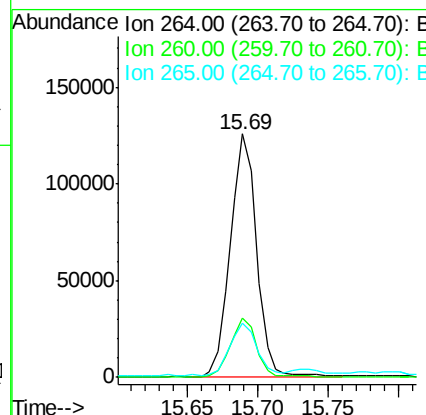

#87
Benzo(b)fluoranthene
Concen: 36.376 ng
RT: 15.23 min Scan# 2192
Delta R.T. -0.03 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.0	25.6
125	8.8	9.0	13.6



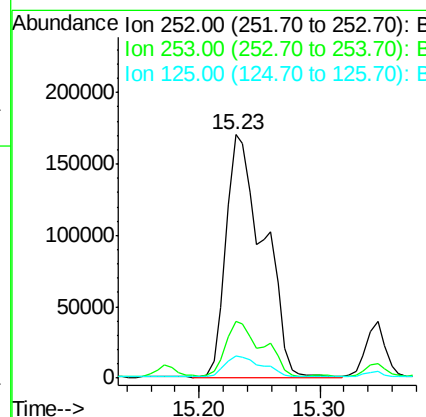





#88
Benzo(k)fluoranthene
Concen: 4.718 ng
RT: 15.35 min Scan# 2212
Delta R.T. 0.05 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
252	100		
253	25.6	17.9	26.9
125	11.7	10.2	15.2

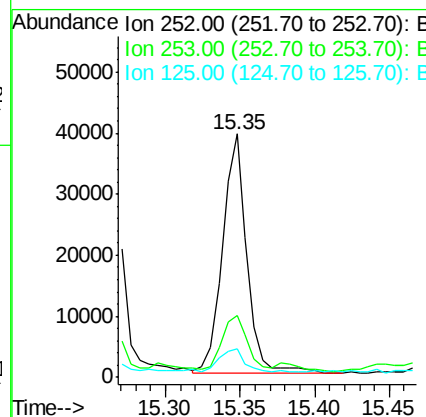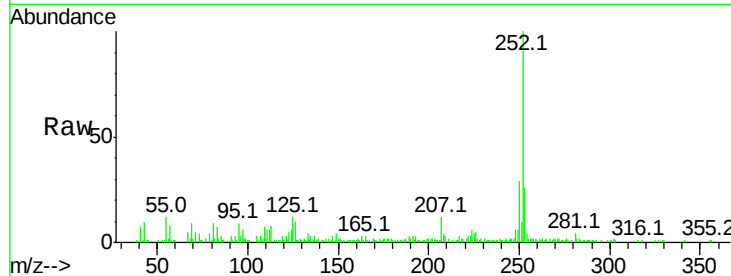

#89
Benzo(a)pyrene
Concen: 14.116 ng
RT: 15.55 min Scan# 2247
Delta R.T. -0.10 min
Lab File: BF107012.D
Acq: 30 Jun 2018 14:09

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.1	25.7
125	13.2	9.8	14.6

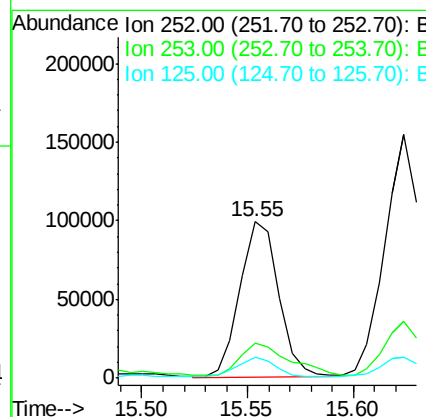

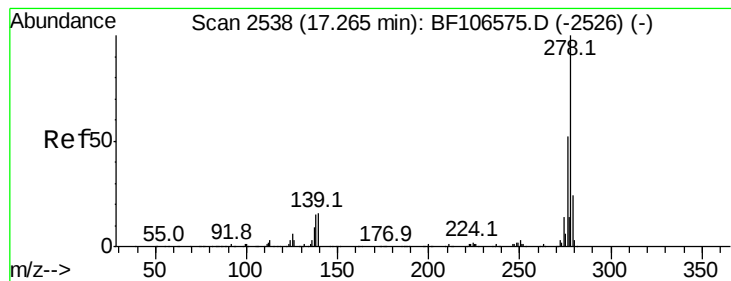

#90

Dibenzo(a,h)anthracene

Concen: 2.544 ng

RT: 17.45 min Scan# 2570

Delta R.T. 0.13 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09

Instrument :

BNA_F

ClientSampled :


Tot Ion:278 Resp: 19305

Ion	Ratio	Lower	Upper
278	100		
139	16.7	15.9	23.9
279	28.1	19.0	28.4

278 100

139 16.7 15.9 23.9




279 28.1 19.0 28.4



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

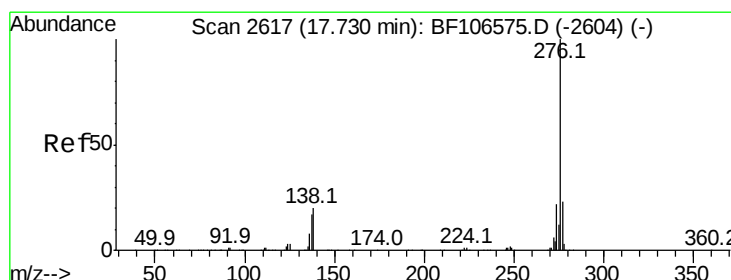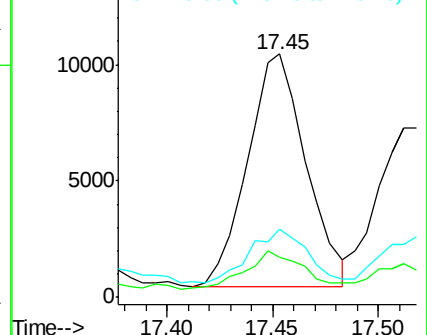

#91

Benzo(g,h,i)perylene

Concen: 12.633 ng

RT: 17.75 min Scan# 2620

Delta R.T. -0.04 min

Lab File: BF107012.D

Acq: 30 Jun 2018 14:09


Tgt Ion:276 Resp: 93681

Ion	Ratio	Lower	Upper
276	100		
277	25.6	17.9	26.9
138	19.4	21.8	32.8

276 100

277 25.6 17.9 26.9

138 19.4 21.8 32.8



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

