

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF063018\
 Data File : BF107016.D
 Acq On : 30 Jun 2018 15:56
 Operator : JU/SJ
 Sample : J3629-07 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Jul 02 04:05:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	58268	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	208587	20.00	ng	-0.01
38) Acenaphthene-d10	10.00	164	87513	20.00	ng	-0.01
63) Phenanthrene-d10	11.49	188	176936	20.00	ng	-0.01
75) Chrysene-d12	14.14	240	206070	20.00	ng	-0.02
86) Perylene-d12	15.69	264	137604	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	6467	1.88	ng	0.00
7) Phenol-d6	6.61	99	7704	1.79	ng	0.00
23) Nitrobenzene-d5	7.52	82	4271	1.14	ng	-0.01
41) 2,4,6-Tribromophenol	10.80	330	1805	1.78	ng	0.00
44) 2-Fluorobiphenyl	9.31	172	10490	-15.39	ng	-0.01
78) Terphenyl-d14	13.07	244	15277	1.80	ng	-0.02
Target Compounds						
50) 2,6-Dinitrotoluene	10.00	165	11026	7.933	ng	# 24
56) 2,4-Dinitrotoluene	10.00	165	11026	6.078	ng	# 21

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF063018\
Data File : BF107016.D
Acq On : 30 Jun 2018 15:56
Operator : JU/SJ
Sample : J3629-07 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Jul 02 04:05:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

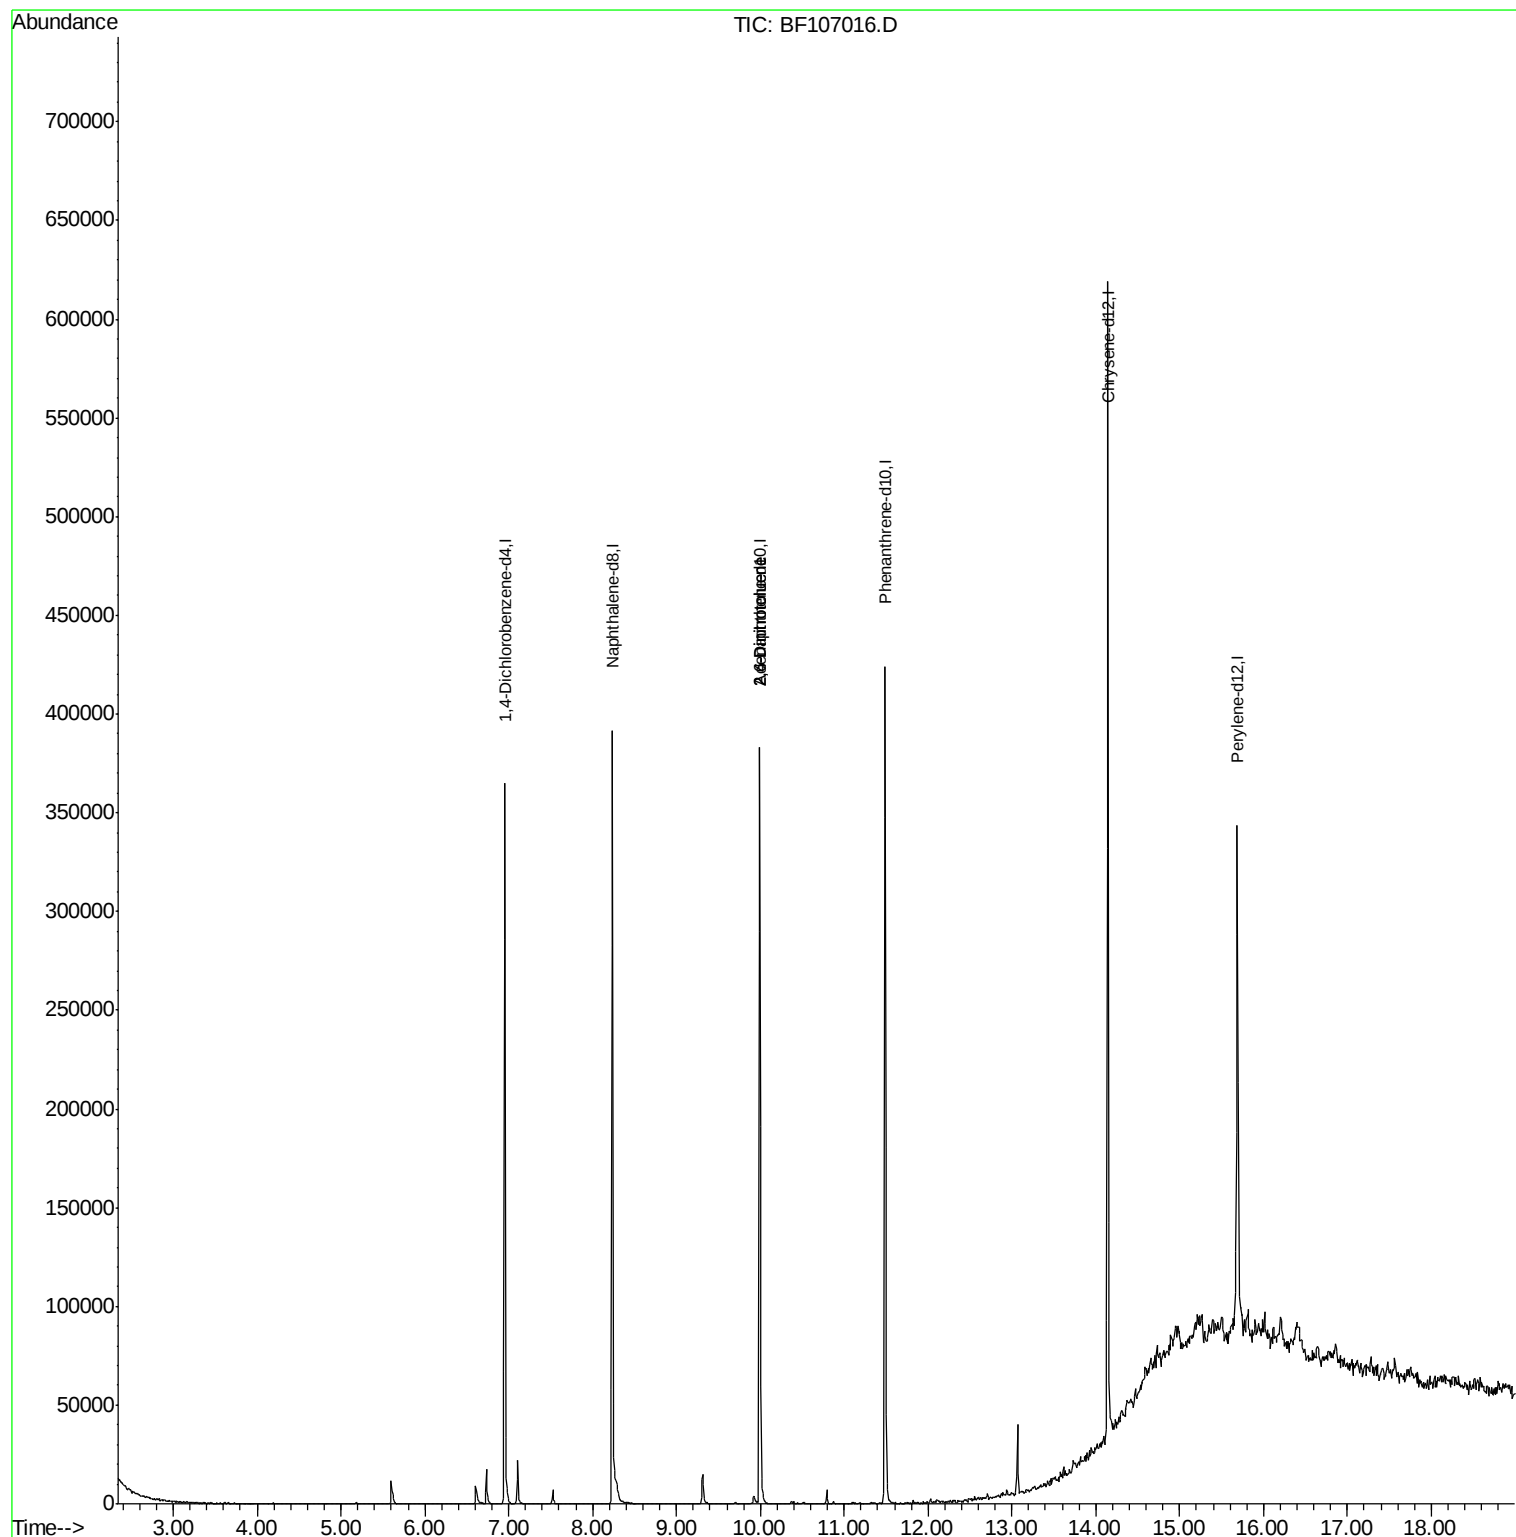




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF107016.D
Acq: 30 Jun 2018 15:56

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 58268
Ion Ratio Lower Upper
152 100
150 156.5 124.6 186.8
115 56.7 50.1 75.1

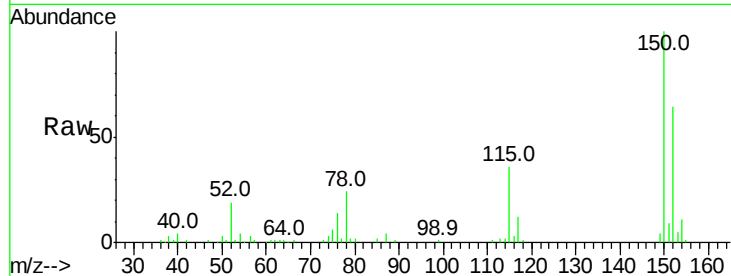


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

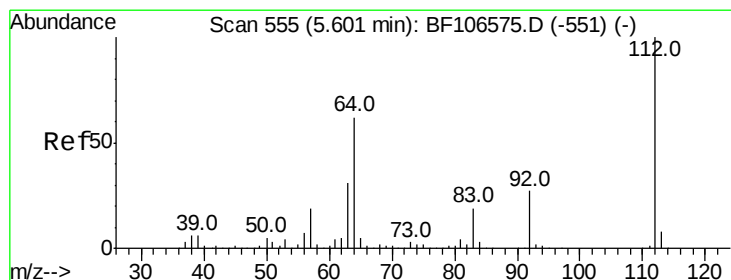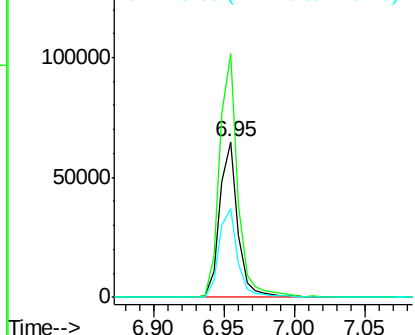



#5

2-Fluorophenol
Concen: 1.879 ng
RT: 5.60 min Scan# 555
Delta R.T. 0.00 min
Lab File: BF107016.D
Acq: 30 Jun 2018 15:56

Tgt Ion:112 Resp: 6467
Ion Ratio Lower Upper
112 100
64 59.1 47.9 71.9
63 29.9 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

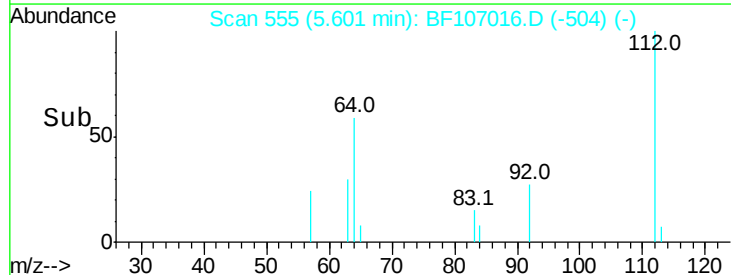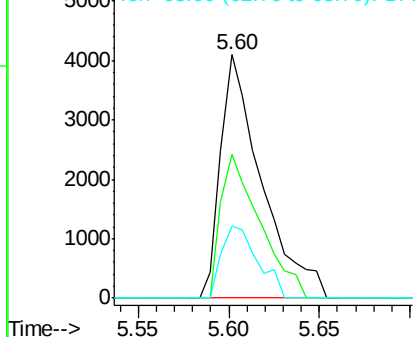



#7

Phenol-d6

Concen: 1.793 ng

RT: 6.61 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF107016.D

Acq: 30 Jun 2018 15:56

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 7704

Ion Ratio Lower Upper




99 100

42 20.4 14.5 21.7

71 34.5 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

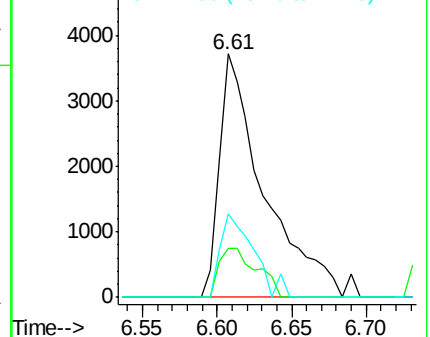

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF107016.D

Acq: 30 Jun 2018 15:56

Tgt Ion: 136 Resp: 208587


Ion Ratio Lower Upper

136 100



137 10.7 8.9 13.3

54 7.6 6.6 9.8

68 5.9 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

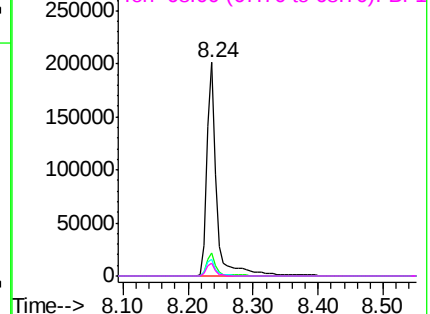






#23
 Nitrobenzene-d5
 Concen: 1.138 ng
 RT: 7.52 min Scan# 882
 Delta R.T. -0.01 min
 Lab File: BF107016.D
 Acq: 30 Jun 2018 15:56

Instrument :
 BNA_F
 ClientSampled :

Tot Ion: 82 Resp: 4271
 Ion Ratio Lower Upper
 82 100
 128 40.8 36.1 54.1
 54 43.6 41.4 62.2

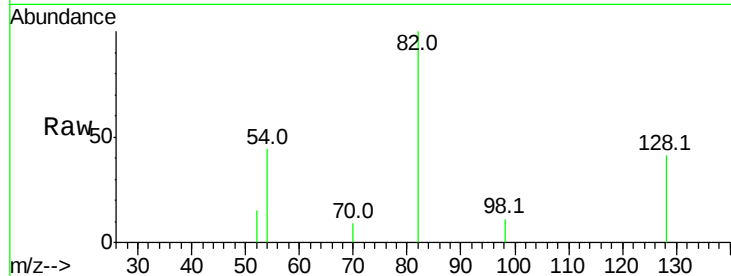


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1


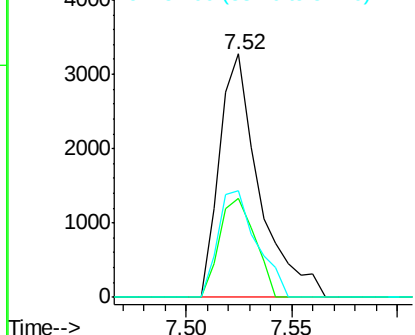


#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.00 min Scan# 1302
 Delta R.T. -0.01 min
 Lab File: BF107016.D
 Acq: 30 Jun 2018 15:56

Tgt Ion:164 Resp: 87513
 Ion Ratio Lower Upper
 164 100
 162 96.3 86.1 129.1
 160 44.8 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

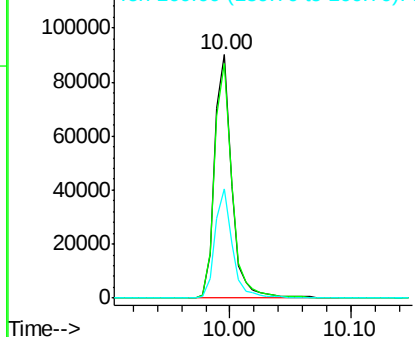






#41
 2,4,6-Tribromophenol
 Concen: 1.780 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF107016.D
 Acq: 30 Jun 2018 15:56

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 1805
 Ion Ratio Lower Upper
 330 100
 332 91.5 77.0 115.6
 141 17.8 29.9 44.9#

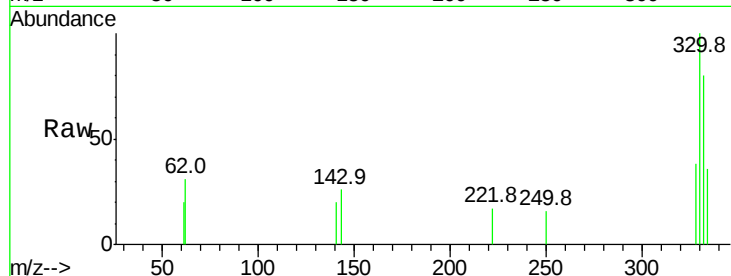


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


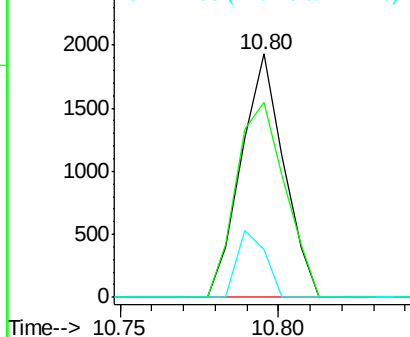



#44
 2-Fluorobiphenyl
 Concen: -15.394 ng
 RT: 9.31 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF107016.D
 Acq: 30 Jun 2018 15:56

Tgt Ion:172 Resp: 10490
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.7 44.5
 170 22.4 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

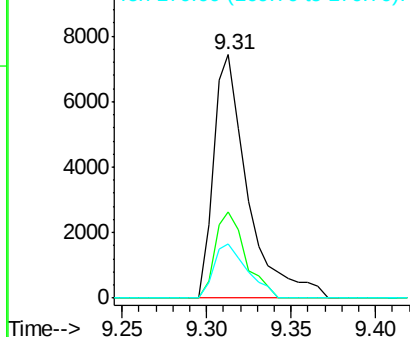


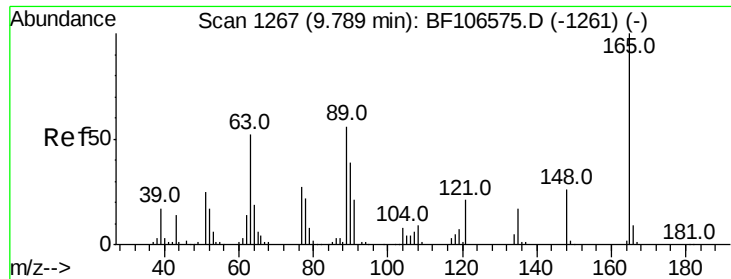

#50
 2,6-Dinitrotoluene
 Concen: 7.933 ng
 RT: 10.00 min Scan# 1302
 Delta R.T. 0.20 min
 Lab File: BF107016.D
 Acq: 30 Jun 2018 15:56

Instrument :
 BNA_F
 ClientSampleId :




Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	44.7	67.1#
89	0.0	44.0	66.0#

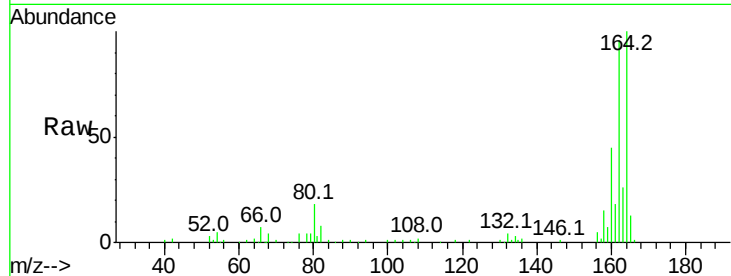

Abundance Ion 165.00 (164.70 to 165.70): E


Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

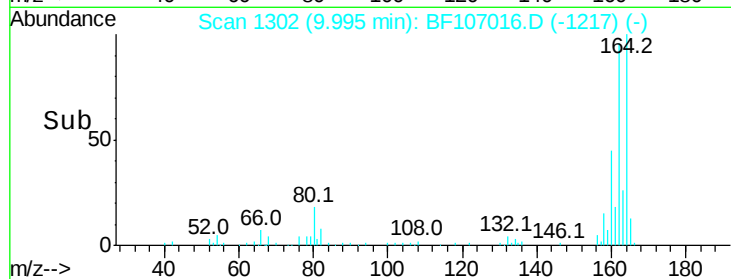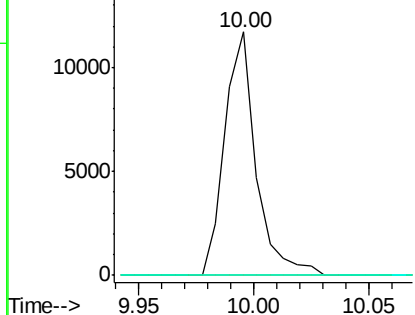

#56
 2,4-Dinitrotoluene
 Concen: 6.078 ng
 RT: 10.00 min Scan# 1302
 Delta R.T. -0.21 min
 Lab File: BF107016.D
 Acq: 30 Jun 2018 15:56

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#





Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E




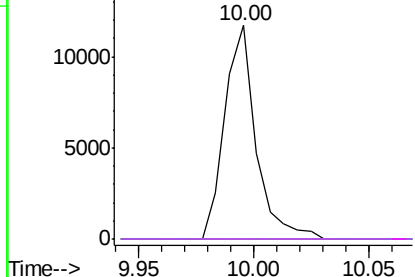




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.49 min Scan# 1556
Delta R.T. -0.01 min
Lab File: BF107016.D
Acq: 30 Jun 2018 15:56




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 176936
Ion Ratio Lower Upper
188 100
94 8.2 8.5 12.7#
80 8.5 9.2 13.8#

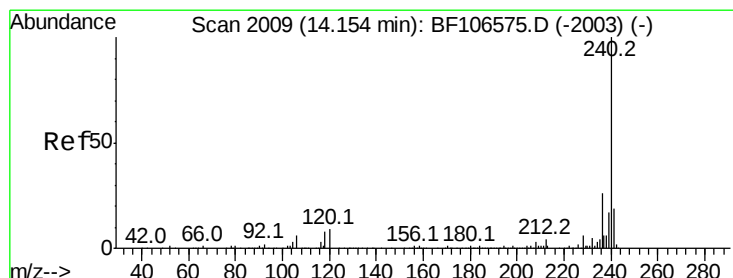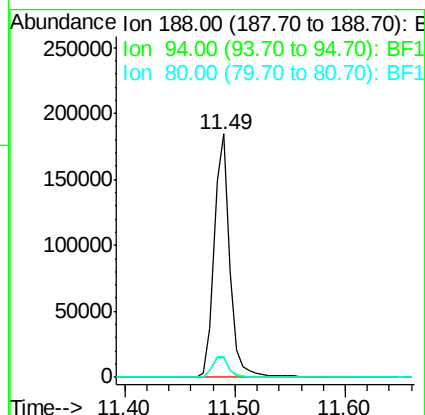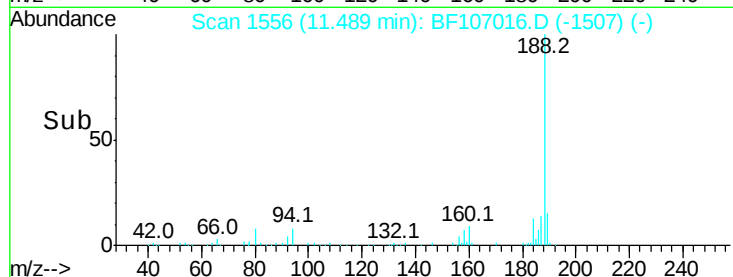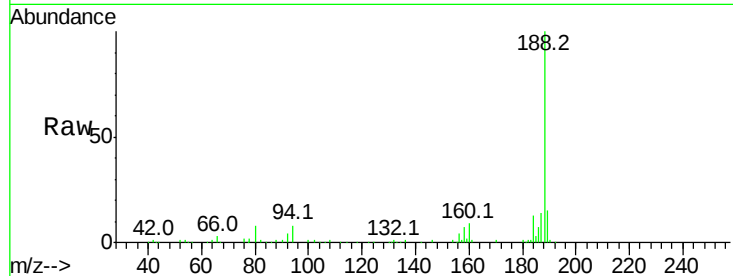

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.14 min Scan# 2007
Delta R.T. -0.02 min
Lab File: BF107016.D
Acq: 30 Jun 2018 15:56

Tgt Ion:240 Resp: 206070
Ion Ratio Lower Upper
240 100
120 9.4 9.5 14.3#
236 25.6 20.7 31.1

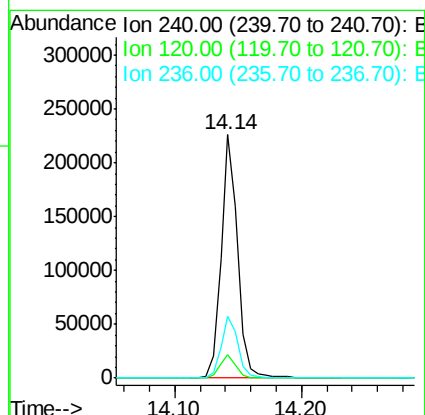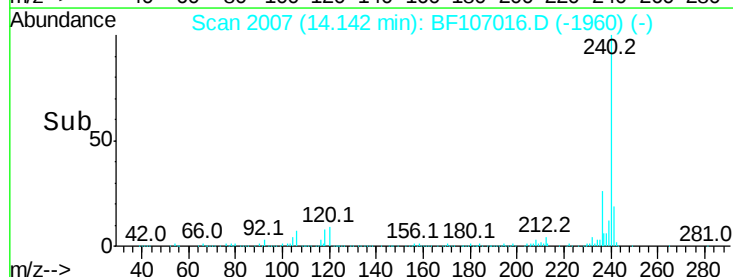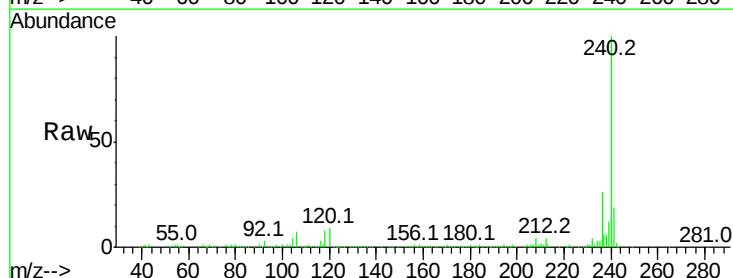

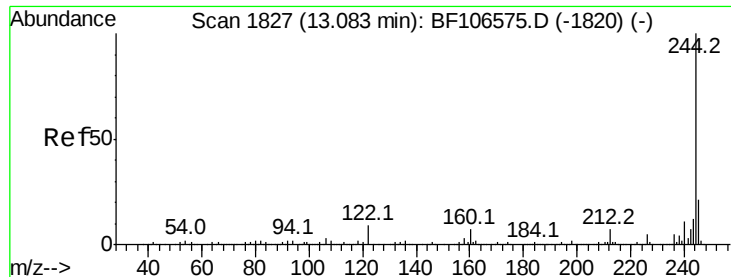

#78

Terphenyl-d14

Concen: 1.796 ng

RT: 13.07 min Scan# 1824

Delta R.T. -0.02 min

Lab File: BF107016.D

Acq: 30 Jun 2018 15:56

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 15277

Ion Ratio Lower Upper

244 100

212 5.7 5.4 8.0




122 9.2 11.0 16.4#

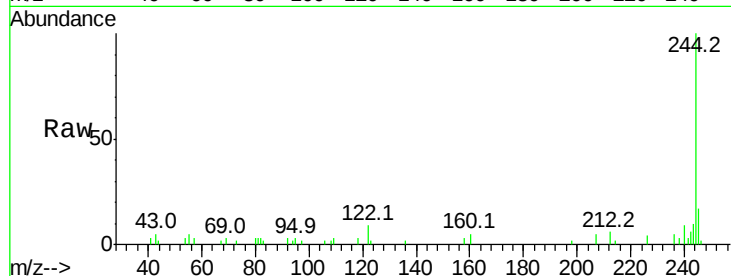

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

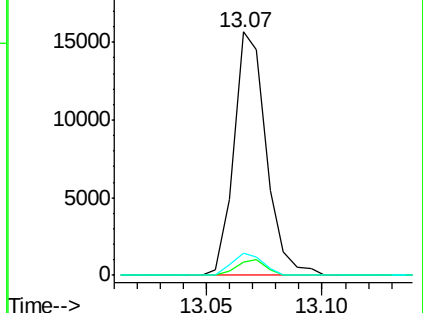

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.69 min Scan# 2270

Delta R.T. -0.03 min

Lab File: BF107016.D

Acq: 30 Jun 2018 15:56


Tgt Ion:264 Resp: 137604

Ion Ratio Lower Upper

264 100

260 24.2 19.2 28.8

265 22.4 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

