
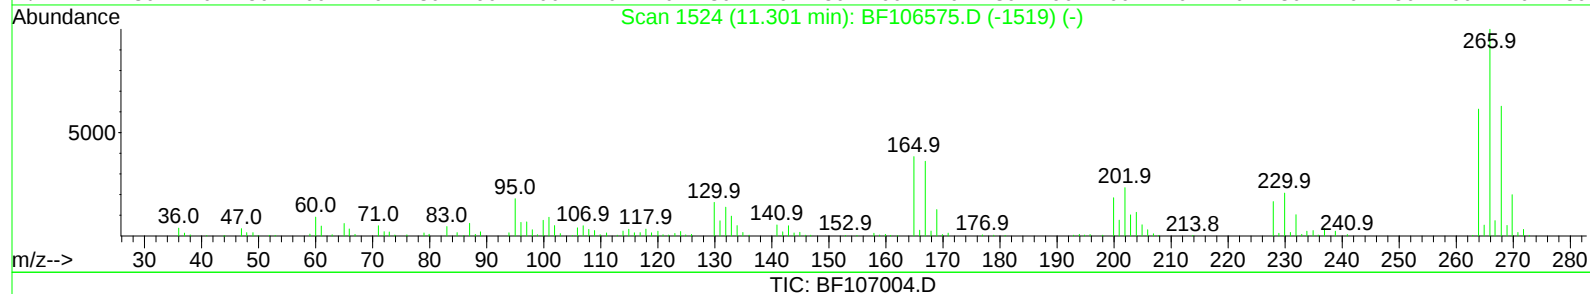
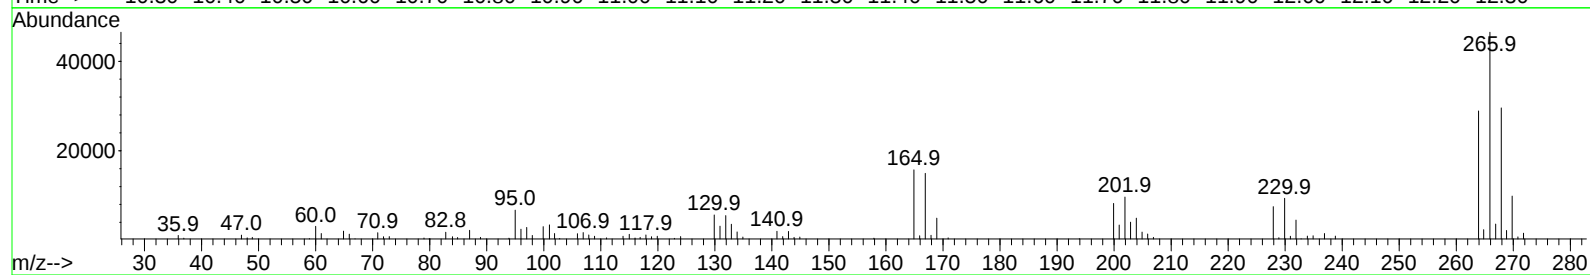


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF063018\
Data File : BF107004.D
Acq On : 30 Jun 2018 10:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:05:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

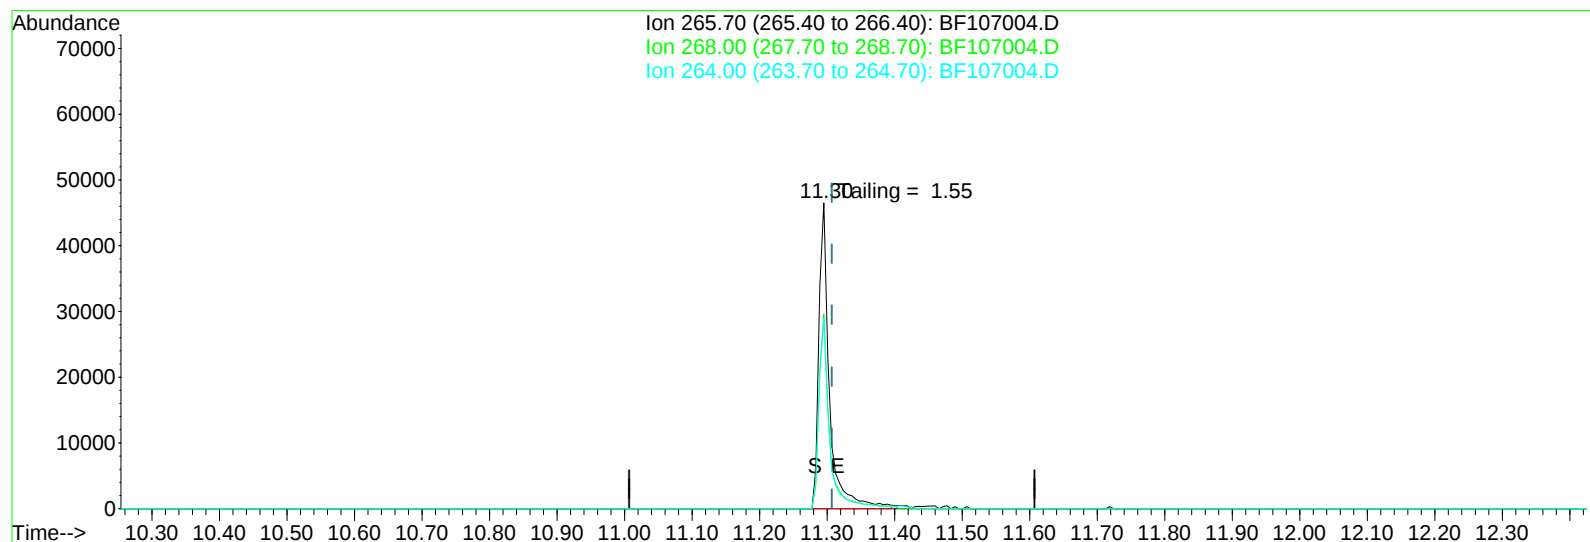

(69) Pentachlorophenol (C)




11.295min (-0.012) 60270.06ng m

response 50711

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.59
264.00	61.90	62.16
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF063018\
Data File : BF107004.D
Acq On : 30 Jun 2018 10:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:05:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

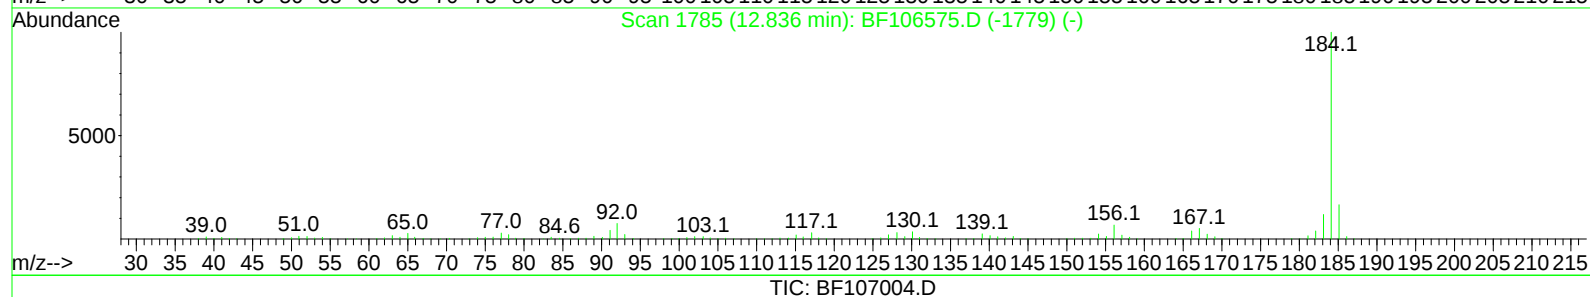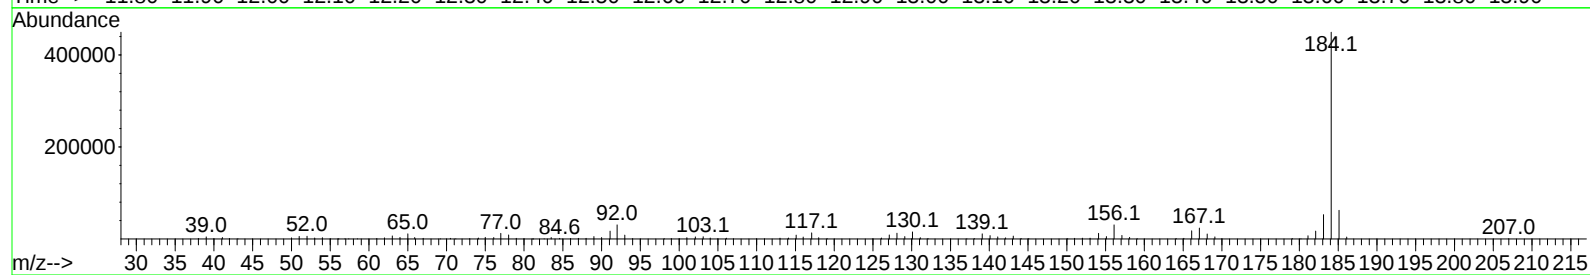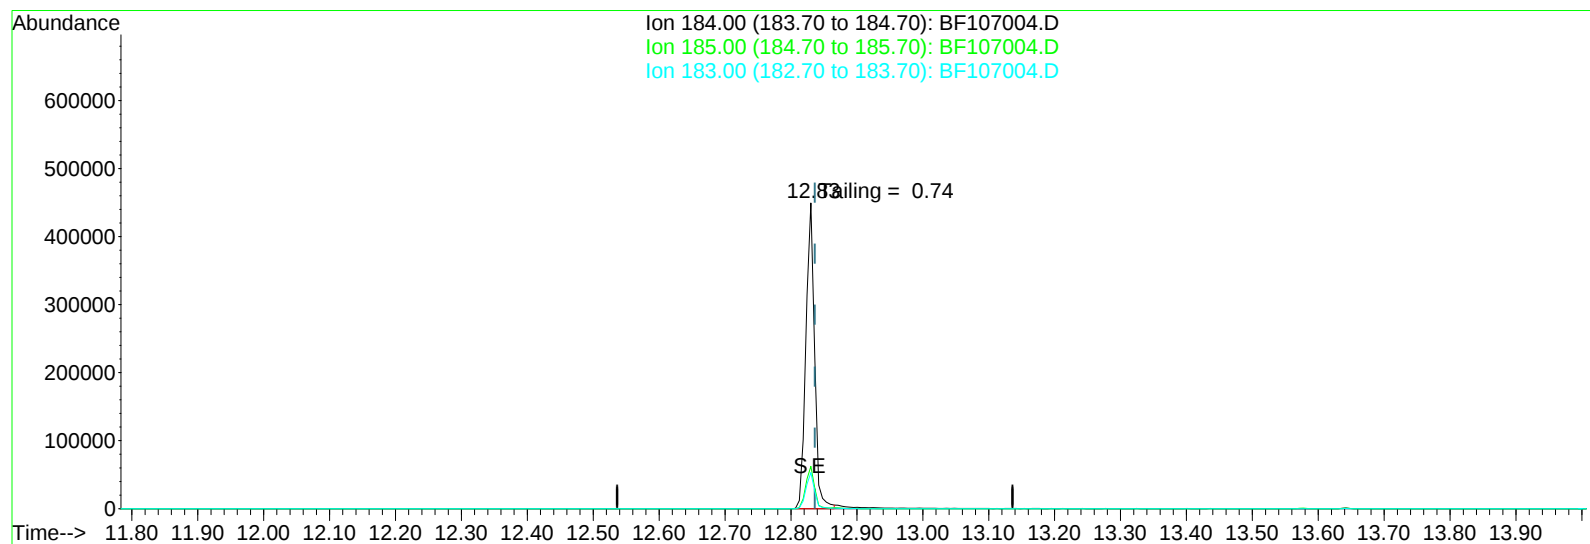

(76) Benzidine

12.830min (-0.006) 0.00ng

response 423971

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.87
183.00	11.60	11.79
0.00	0.00	0.00