

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF063018\
 Data File : BF107016.D
 Acq On : 30 Jun 2018 15:56
 Operator : JU/SJ
 Sample : J3629-07 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A0C10-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.601	552	555	564	rBB	11414	15442	2.81%	0.612%
2	6.607	723	726	739	rBB2	8953	14958	2.72%	0.593%
3	6.731	744	747	756	rBB	17543	18579	3.38%	0.737%
4	6.954	781	785	794	rBV	365132	327446	59.51%	12.986%
5	7.107	808	811	818	rBB	21854	19854	3.61%	0.787%
6	7.525	879	882	887	rBV	7180	8548	1.55%	0.339%
7	8.237	999	1003	1009	rBV	391926	363347	66.03%	14.410%
8	9.313	1183	1186	1197	rBB	15017	18602	3.38%	0.738%
9	9.925	1285	1290	1295	rBV2	4105	6685	1.21%	0.265%
10	9.995	1298	1302	1317	rVB	382890	372842	67.76%	14.787%
11	10.795	1435	1438	1441	rBB	7412	6640	1.21%	0.263%
12	11.489	1552	1556	1570	rBV	424190	402898	73.22%	15.979%
13	13.066	1822	1824	1828	rVB	34952	30586	5.56%	1.213%
14	13.577	1908	1911	1915	rBV6	4926	7526	1.37%	0.298%
15	13.736	1934	1938	1940	rBV5	5913	7978	1.45%	0.316%
16	14.142	2003	2007	2016	rBV	586236	550276	100.00%	21.824%
17	15.689	2265	2270	2278	rVB2	248846	349248	63.47%	13.851%


Sum of corrected areas: 2521455

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF063018\
Data File : BF107016.D
Acq On : 30 Jun 2018 15:56
Operator : JU/SJ
Sample : J3629-07 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C10-02

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

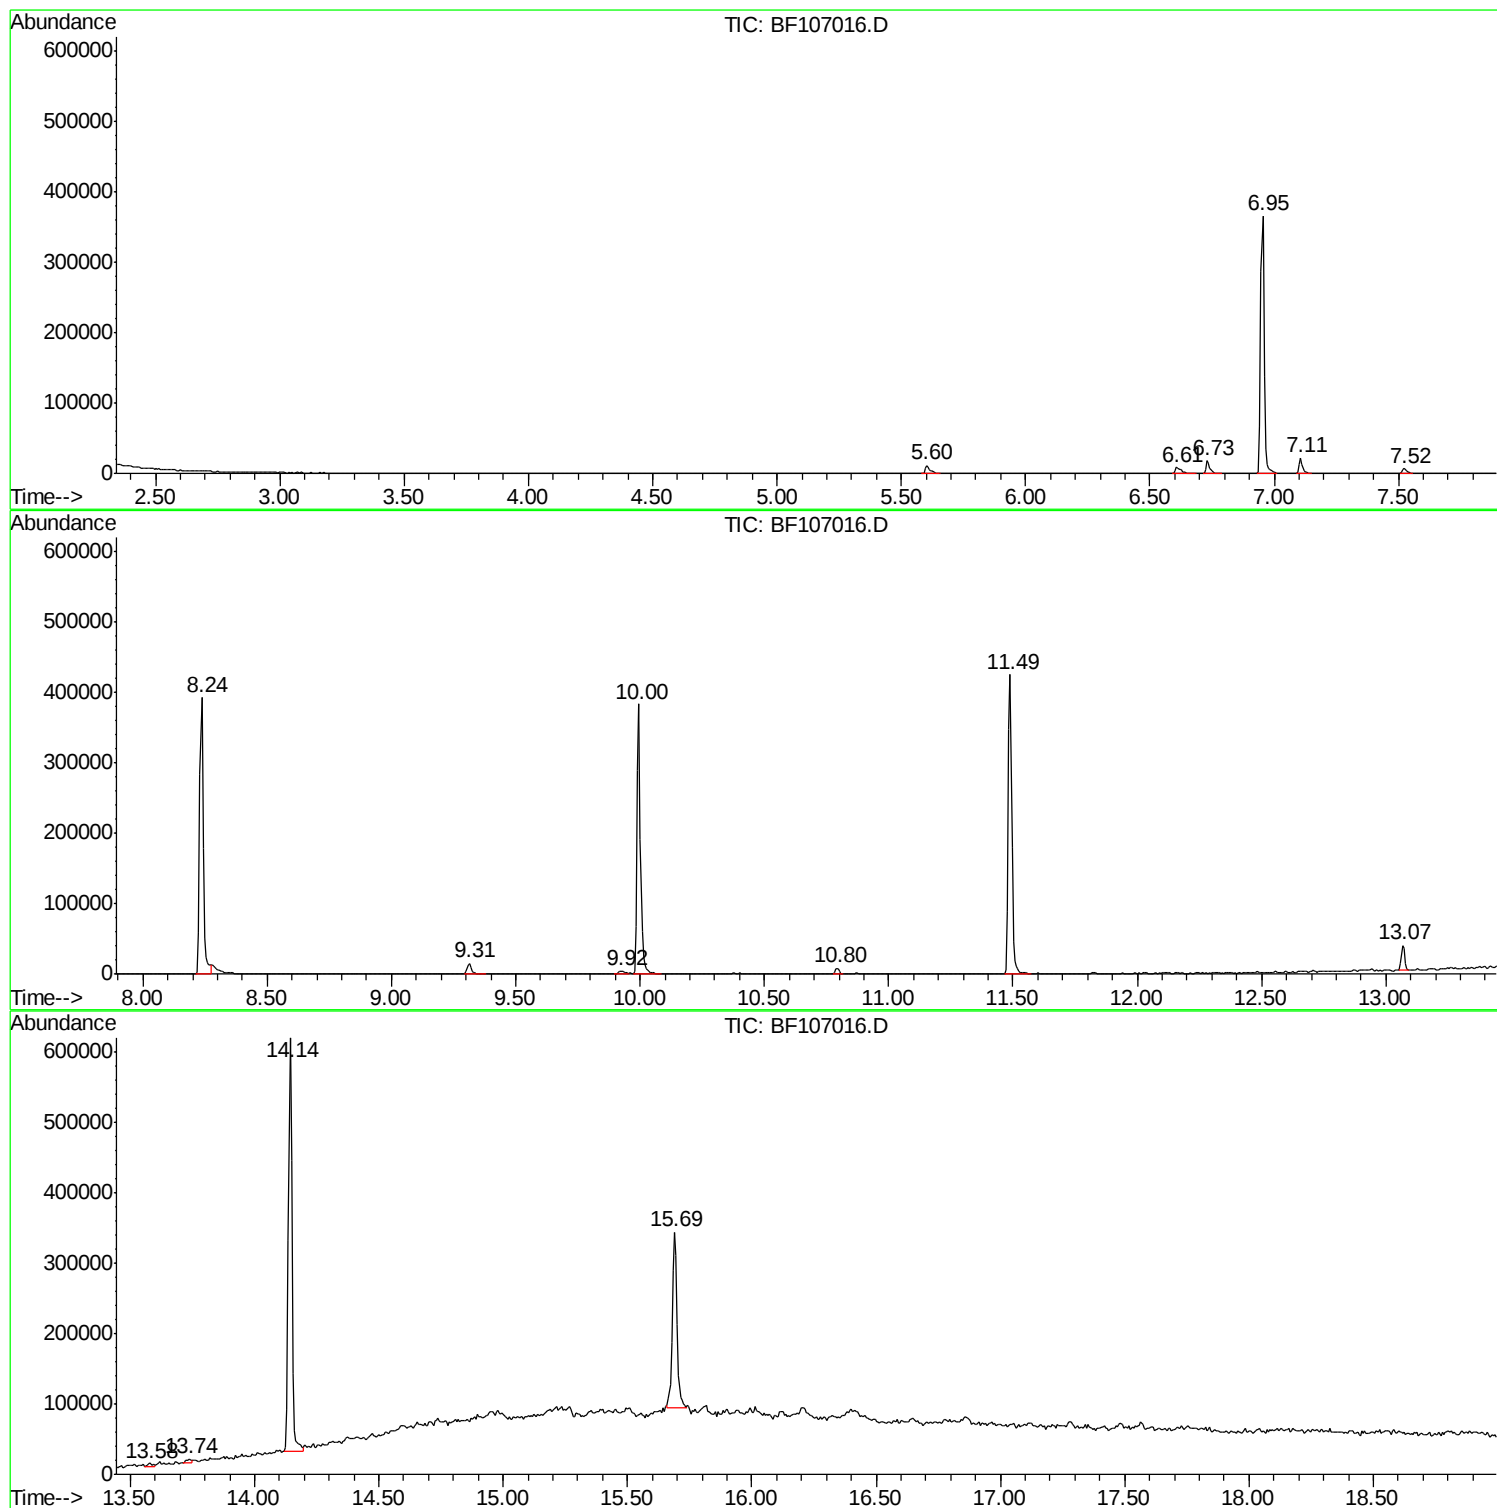

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF063018\
Data_File : BF107016.D
Acq_On : 30 Jun 2018 15:566
Operator : JU/SJJ
Sample : J3629-07.5XX
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
A0C10-02

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
