

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF063018\  
 Data File : BF107017.D  
 Acq On : 30 Jun 2018 16:22  
 Operator : JU/SJ  
 Sample : J3629-09 5X  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 A0C10-04

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.601       | 552           | 555         | 567          | rBB      | 13586          | 19388         | 3.81%           | 0.772%        |
| 2         | 6.607       | 723           | 726         | 739          | rBB      | 13642          | 19413         | 3.81%           | 0.773%        |
| 3         | 6.731       | 744           | 747         | 757          | rBB      | 24469          | 24193         | 4.75%           | 0.964%        |
| 4         | 6.954       | 781           | 785         | 798          | rBB      | 361861         | 324580        | 63.71%          | 12.930%       |
| 5         | 7.107       | 808           | 811         | 819          | rBB      | 27180          | 24662         | 4.84%           | 0.982%        |
| 6         | 7.525       | 879           | 882         | 888          | rBB      | 8950           | 11052         | 2.17%           | 0.440%        |
| 7         | 8.236       | 999           | 1003        | 1009         | rBV      | 385252         | 354463        | 69.57%          | 14.120%       |
| 8         | 9.313       | 1182          | 1186        | 1195         | rBV      | 23119          | 26598         | 5.22%           | 1.060%        |
| 9         | 9.925       | 1284          | 1290        | 1298         | rBV4     | 3937           | 8838          | 1.73%           | 0.352%        |
| 10        | 9.995       | 1298          | 1302        | 1315         | rVB      | 371093         | 366432        | 71.92%          | 14.597%       |
| 11        | 10.789      | 1435          | 1437        | 1442         | rBB      | 9952           | 9354          | 1.84%           | 0.373%        |
| 12        | 11.489      | 1552          | 1556        | 1563         | rBV      | 430384         | 401889        | 78.88%          | 16.009%       |
| 13        | 13.066      | 1822          | 1824        | 1830         | rBV      | 49460          | 45107         | 8.85%           | 1.797%        |
| 14        | 13.248      | 1850          | 1855        | 1858         | rBV5     | 6085           | 9326          | 1.83%           | 0.371%        |
| 15        | 13.589      | 1908          | 1913        | 1915         | rBV4     | 8219           | 15172         | 2.98%           | 0.604%        |
| 16        | 14.142      | 2003          | 2007        | 2012         | rBV      | 546885         | 509494        | 100.00%         | 20.296%       |
| 17        | 15.683      | 2265          | 2269        | 2279         | rVB      | 244660         | 340408        | 66.81%          | 13.560%       |


Sum of corrected areas: 2510369

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF063018\  
Data File : BF107017.D  
Acq On : 30 Jun 2018 16:22  
Operator : JU/SJ  
Sample : J3629-09 5X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
A0C10-04

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

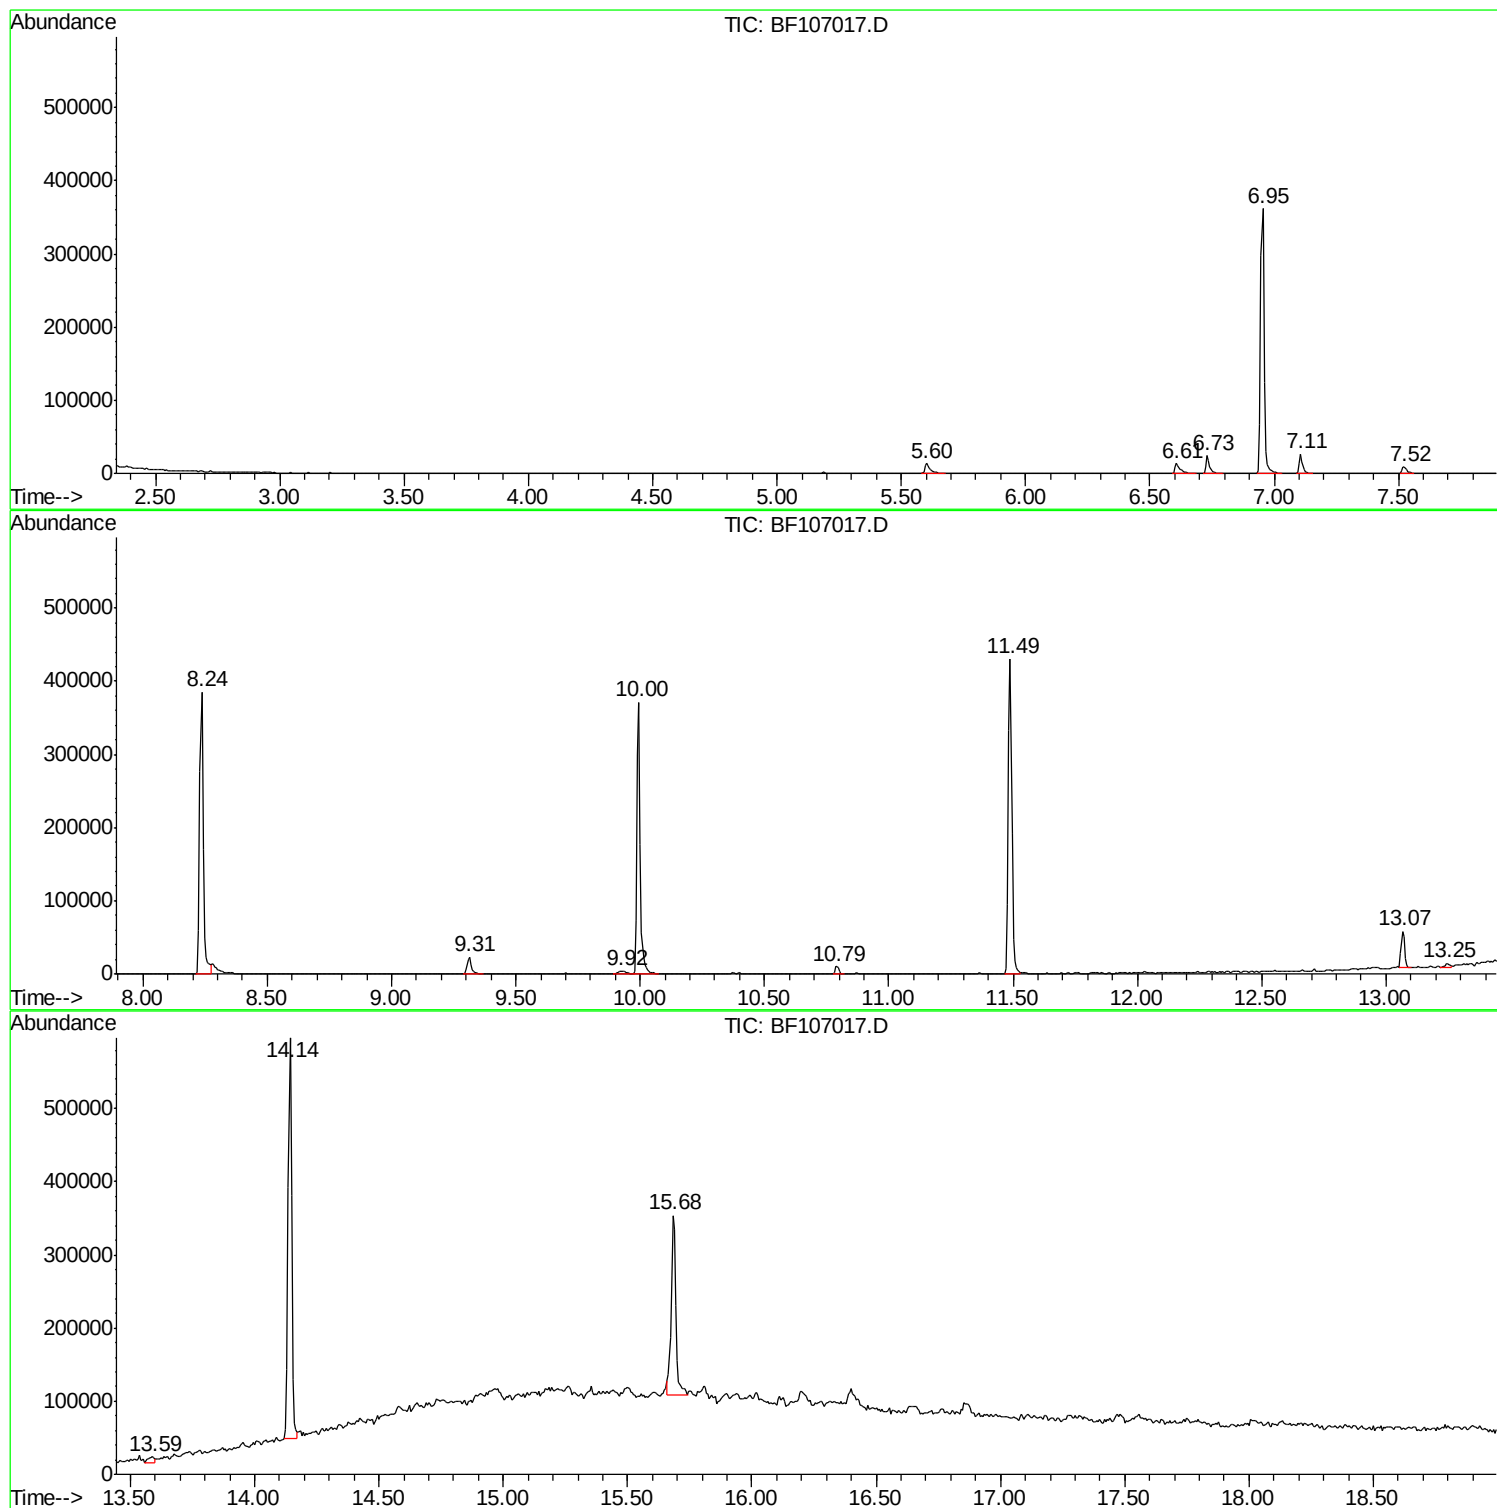

Data\_Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF063018\  
Data\_File : BF107017.D  
Acq\_On : 30 Jun 2018 16:222  
Operator : JU/SJJ  
Sample : J3629-09\_5XX  
Misc :  
ALS\_Vial : 14 Sample\_Multiplier: 11

Instrument :  
BNA\_F  
ClientSampleId :  
A0C10-04

Quant\_Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF061918.MM  
Quant\_Title : ASP\_BNA\_STANDARDS\_FOR\_5\_POINT\_CALIBRATIONN

TIC\_Library : C:\DATABASE\NIST11.LL  
TIC\_Integration Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | Internal Standard |
|------------------|----|---------|-------|----------|-------------------|
|                  |    |         |       | #        | RT Resp Conc      |

No Library Search Compounds Detected

\*\*\*\*\*