


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063018\
 Data File : BF107004.D
 Acq On : 30 Jun 2018 10:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

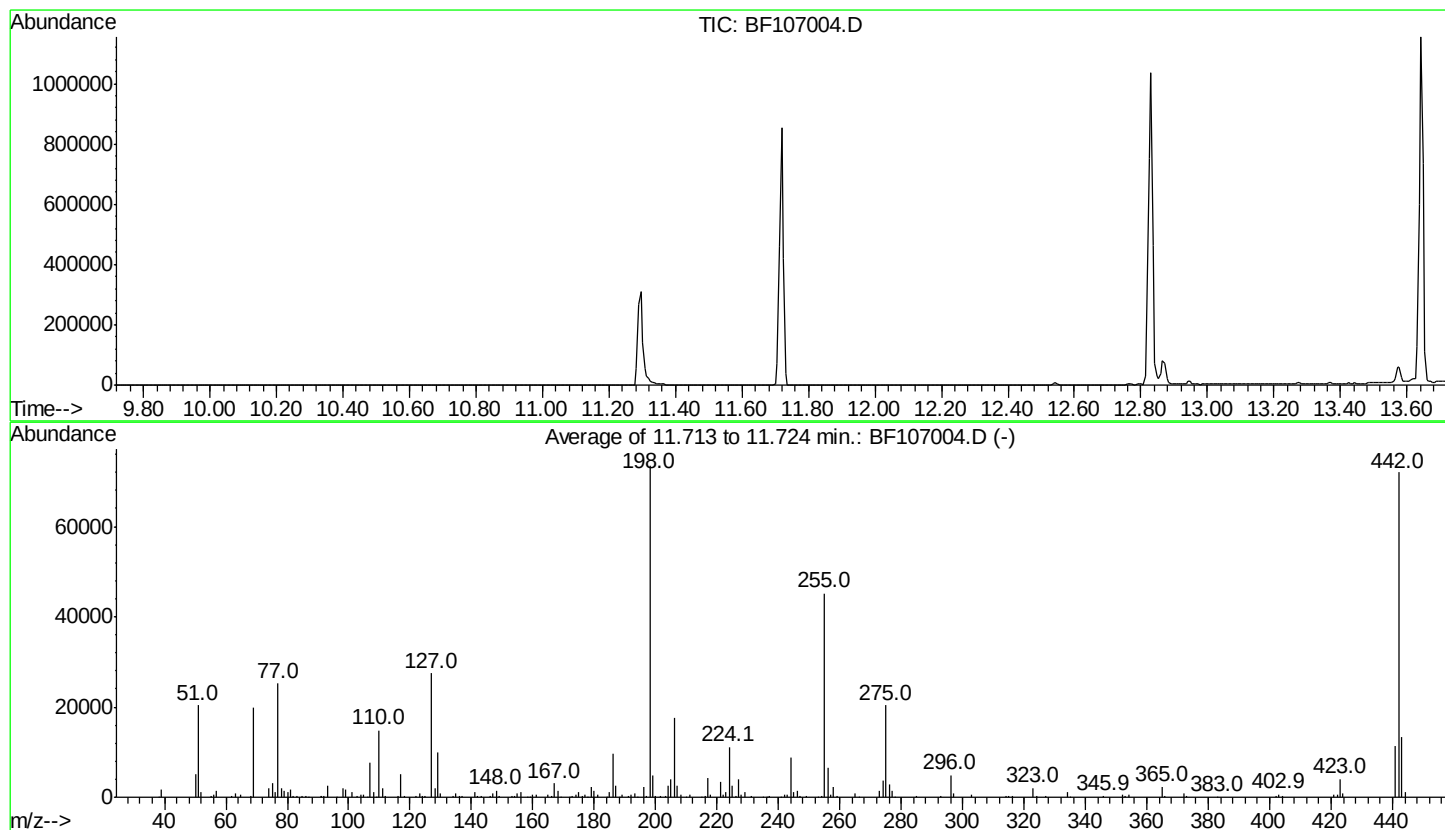

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	20430	PASS
68	69	0.00	2	2.0	396	PASS
69	198	0.00	100	26.9	19798	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.4	27465	PASS
197	198	0.00	2	0.6	419	PASS
198	198	100	100	100.0	73501	PASS
199	198	5	9	6.7	4920	PASS
275	198	10	60	27.7	20384	PASS
365	198	1	100	3.2	2368	PASS
441	443	0.01	100	85.9	11366	PASS
442	198	50	100	98.1	72104	PASS
443	442	15	24	18.3	13230	PASS