
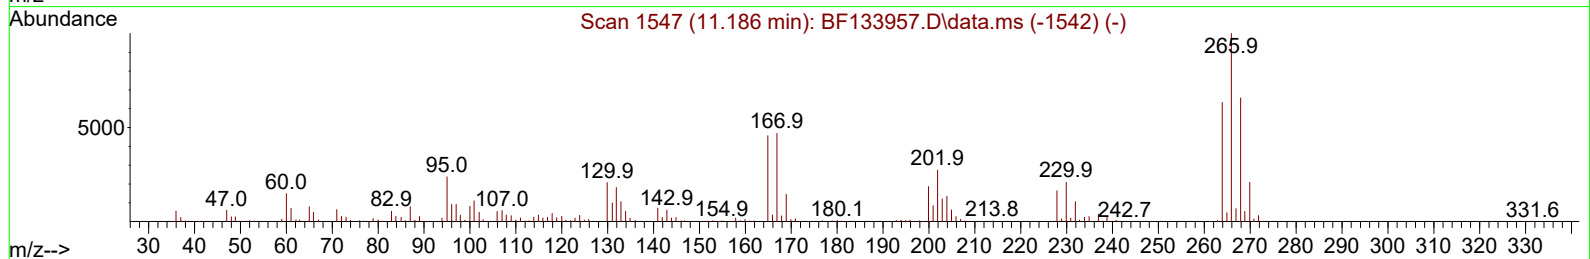
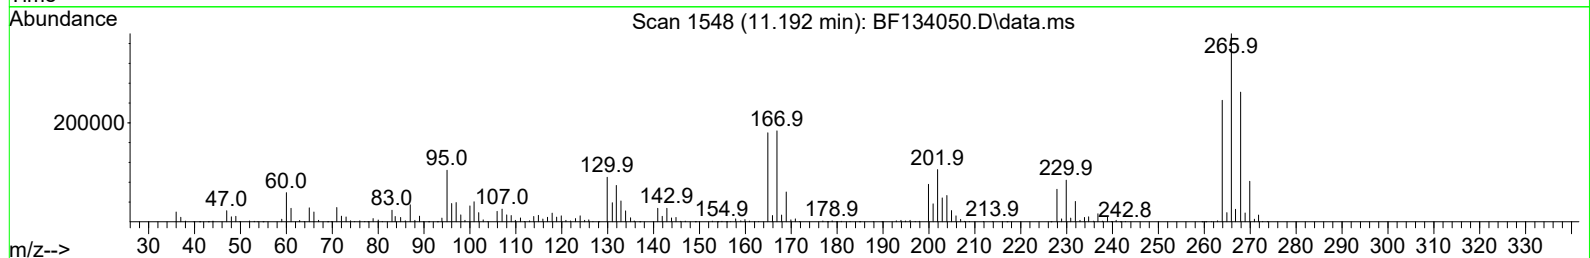


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063023\
Data File : BF134050.D
Acq On : 30 Jun 2023 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 16:26:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

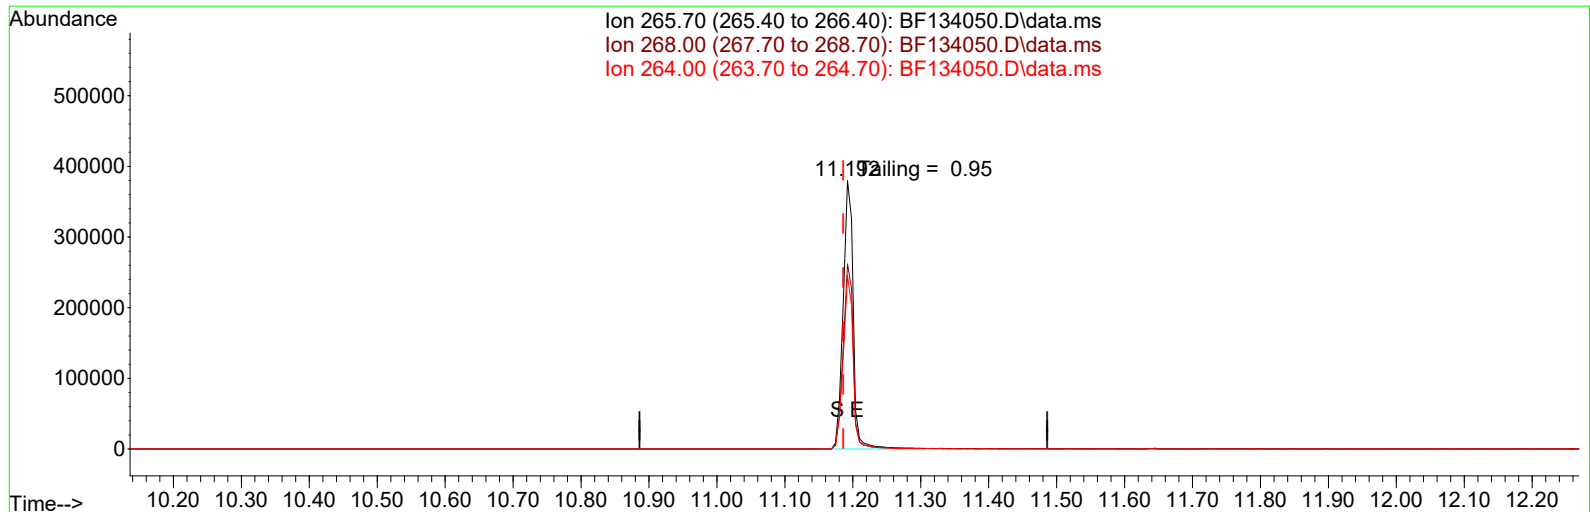

TIC: BF134050.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.006) 471783.51 ng

response 391563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.96
264.00	63.30	64.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063023\
Data File : BF134050.D
Acq On : 30 Jun 2023 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 16:26:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

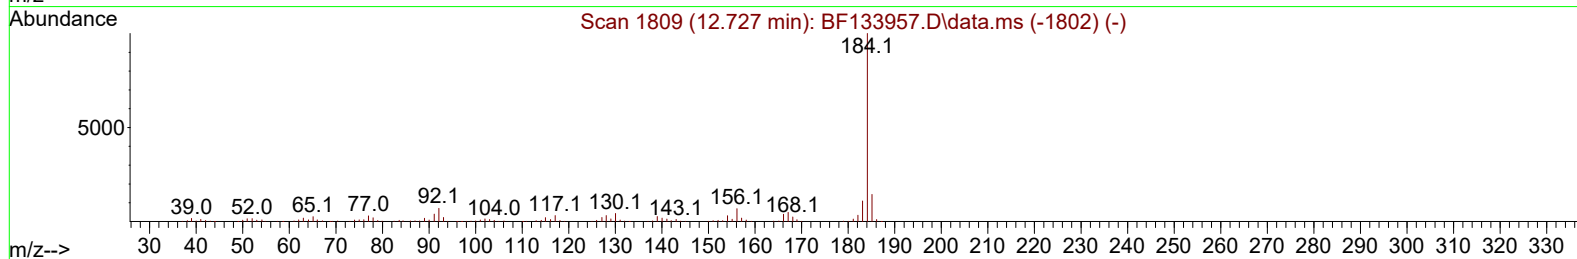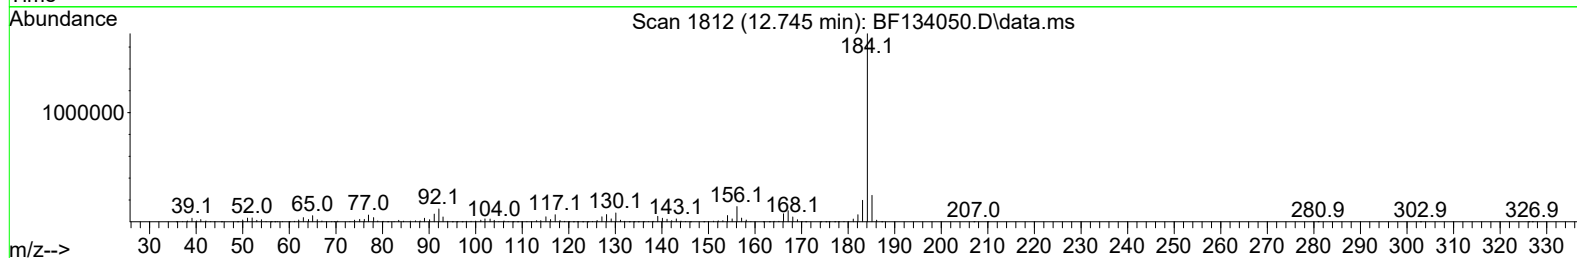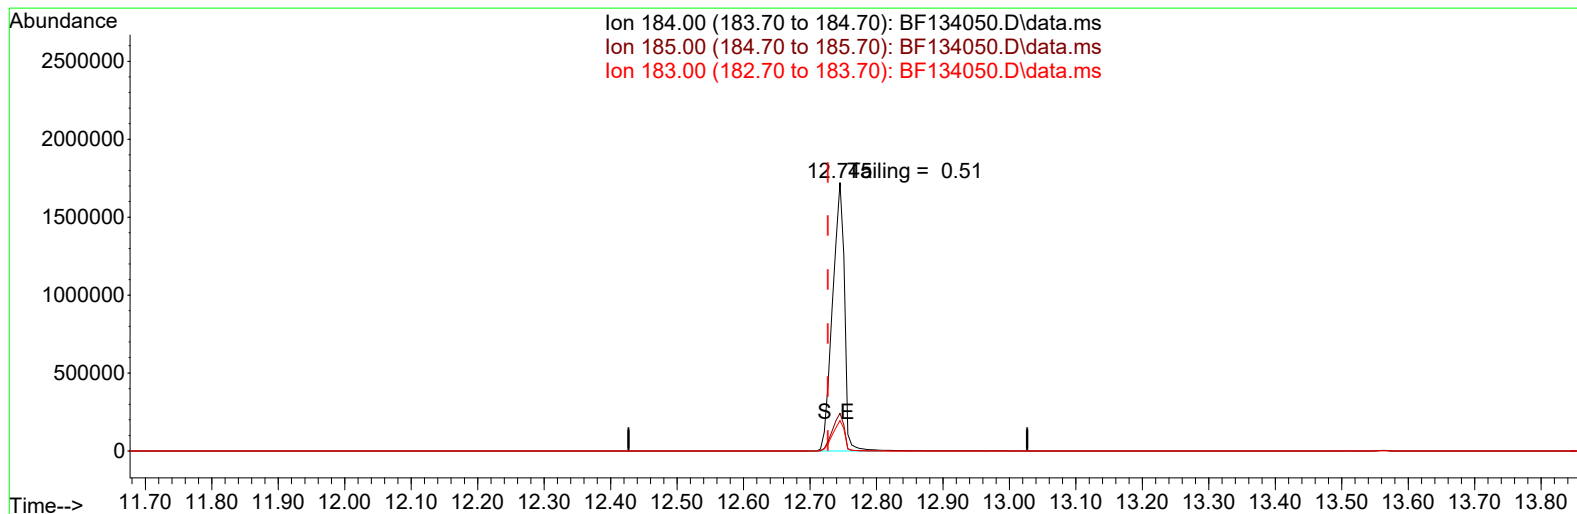

TIC: BF134050.D\data.ms

(77) Benzidine**12.745min (+ 0.018) 197245.87 ng****response 2144854**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.08
183.00	11.00	11.41
0.00	0.00	0.00