
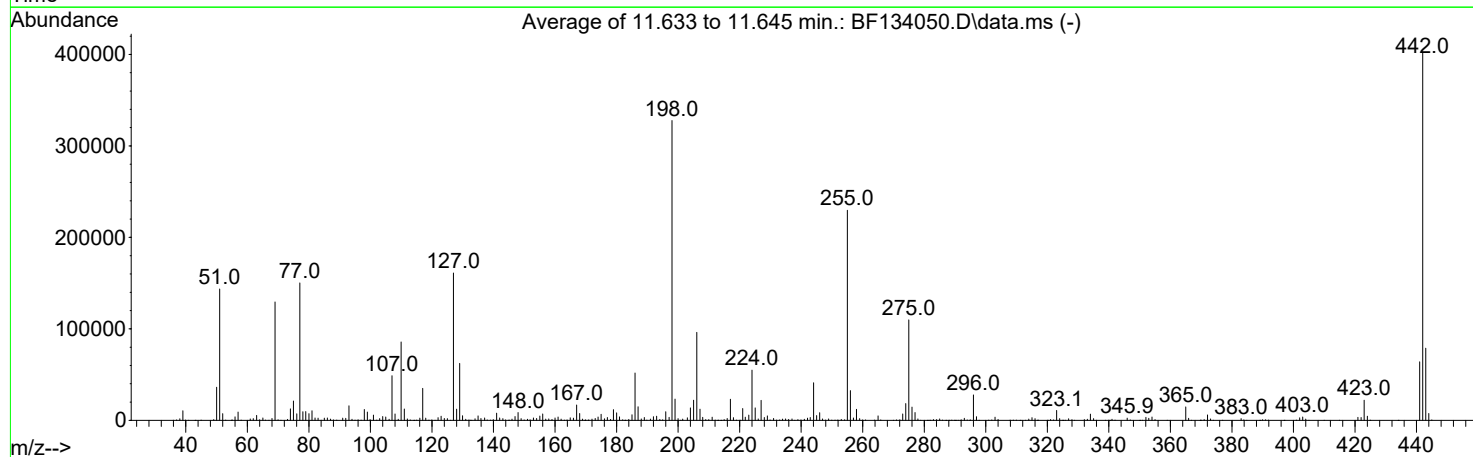


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063023\
 Data File : BF134050.D
 Acq On : 30 Jun 2023 13:39
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 30 18:35:29 2023

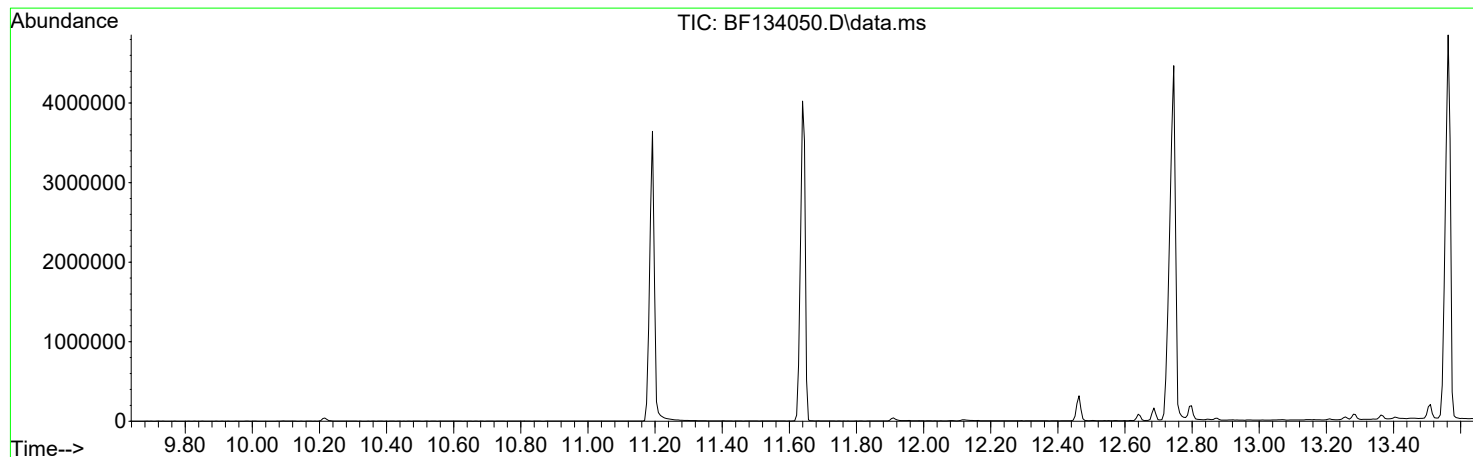




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	143579	PASS
68	69	0.00	2	1.6	2127	PASS
69	198	0.00	100	39.5	129397	PASS
70	69	0.00	2	0.5	689	PASS
127	198	10	80	49.1	161045	PASS
197	198	0.00	2	1.0	3330	PASS
198	198	100	100	100.0	327808	PASS
199	198	5	9	7.1	23208	PASS
275	198	10	60	33.5	109883	PASS
365	198	1	100	4.5	14682	PASS
441	198	0.01	100	19.5	64067	PASS
442	442	50	100	100.0	402091	PASS
443	442	15	24	19.6	78851	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063023\
Data File : BF134050.D
Acq On : 30 Jun 2023 13:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 30 16:26:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 26 23:12:04 2023
Response via : Initial Calibration

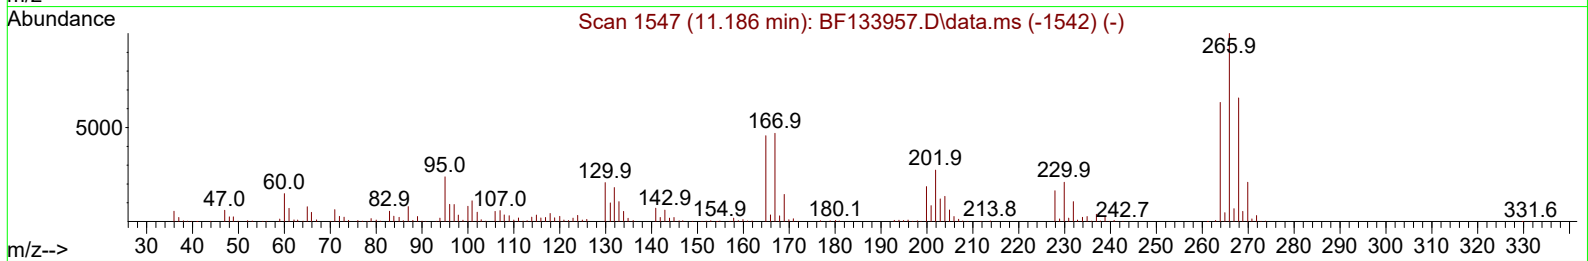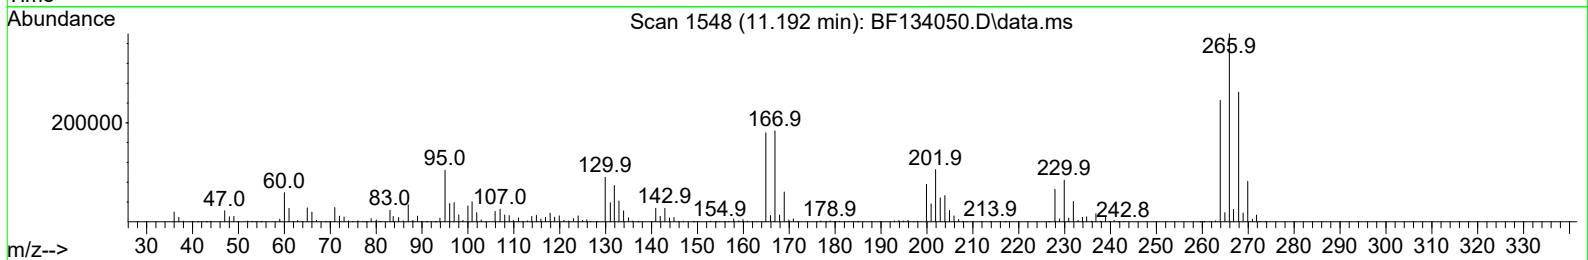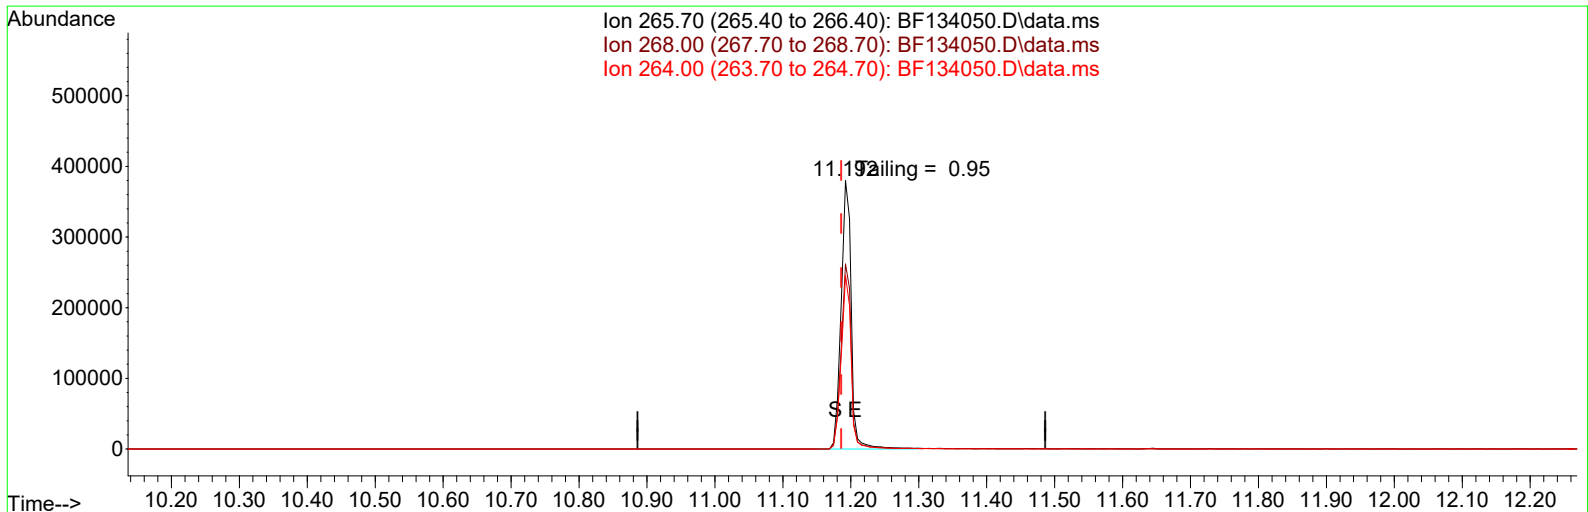

TIC: BF134050.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.006) 471783.51 ng




response 391563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.96
264.00	63.30	64.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF063023\
 Data File : BF134050.D
 Acq On : 30 Jun 2023 13:39
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 30 16:26:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 23:12:04 2023
 Response via : Initial Calibration

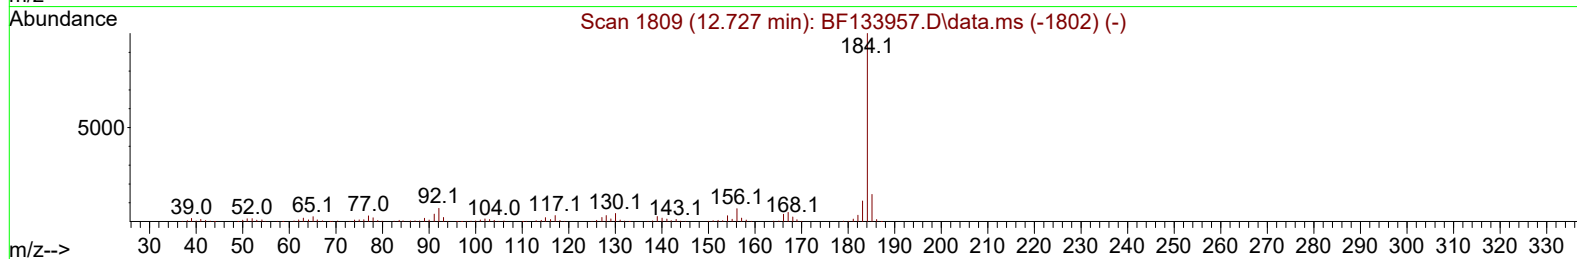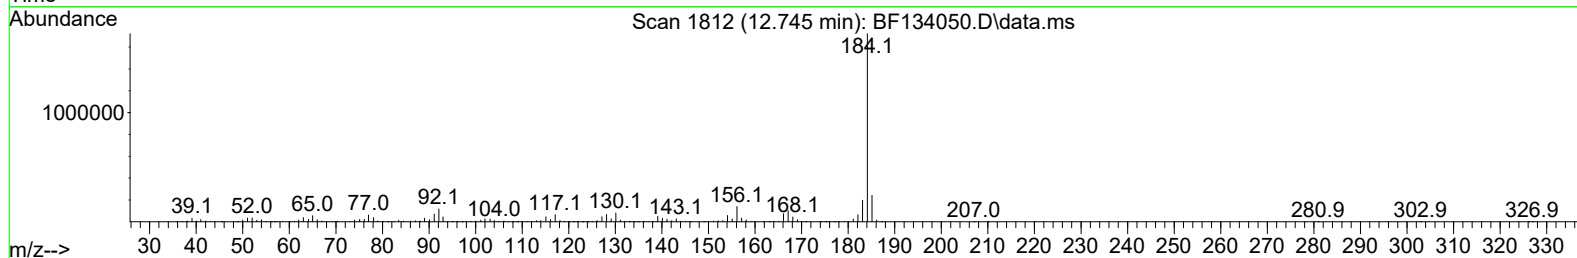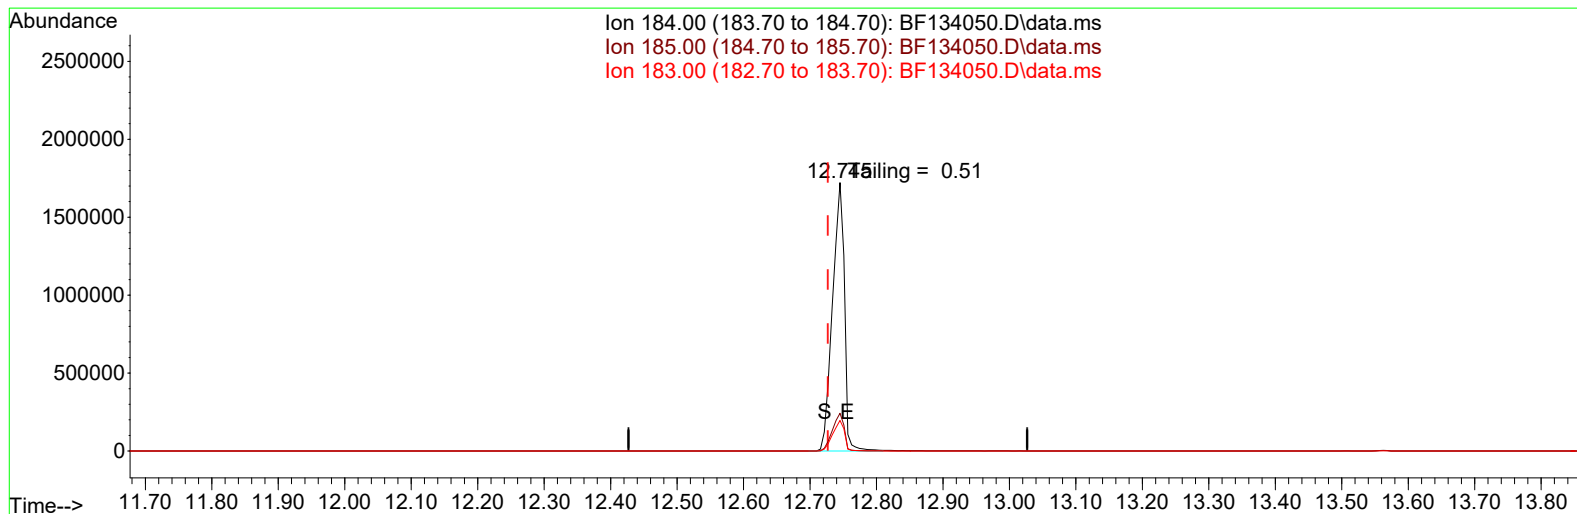

TIC: BF134050.D\data.ms

(77) Benzidine

12.745min (+ 0.018) 197245.87 ng

response 2144854

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.08
183.00	11.00	11.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/29/2023	BNA_F	BF134050.D
Compound Name	Response	Retention Time
DDT	937165	13.563
DDD	13985	13.286
DDE	9404	11.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23389	960554	2.43

Instrument :
BNA_F
ClientSampleId :
DFTPP