
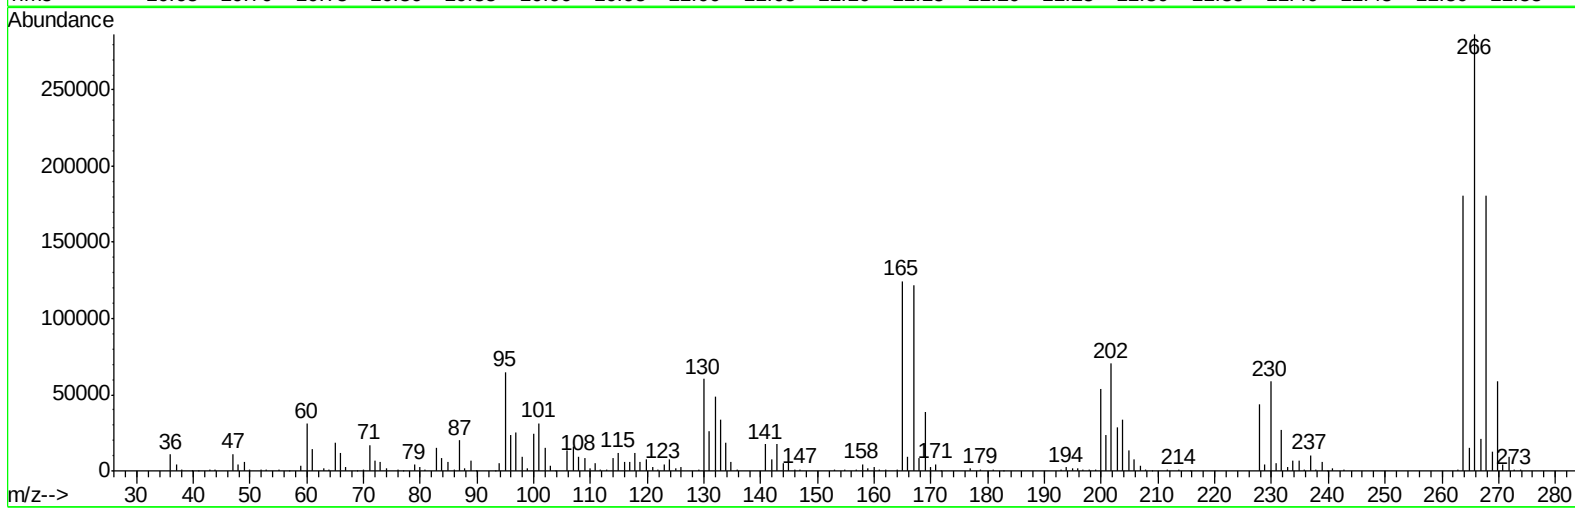


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070119\
Data File : BF115327.D
Acq On : 1 Jul 2019 9:02
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:14:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

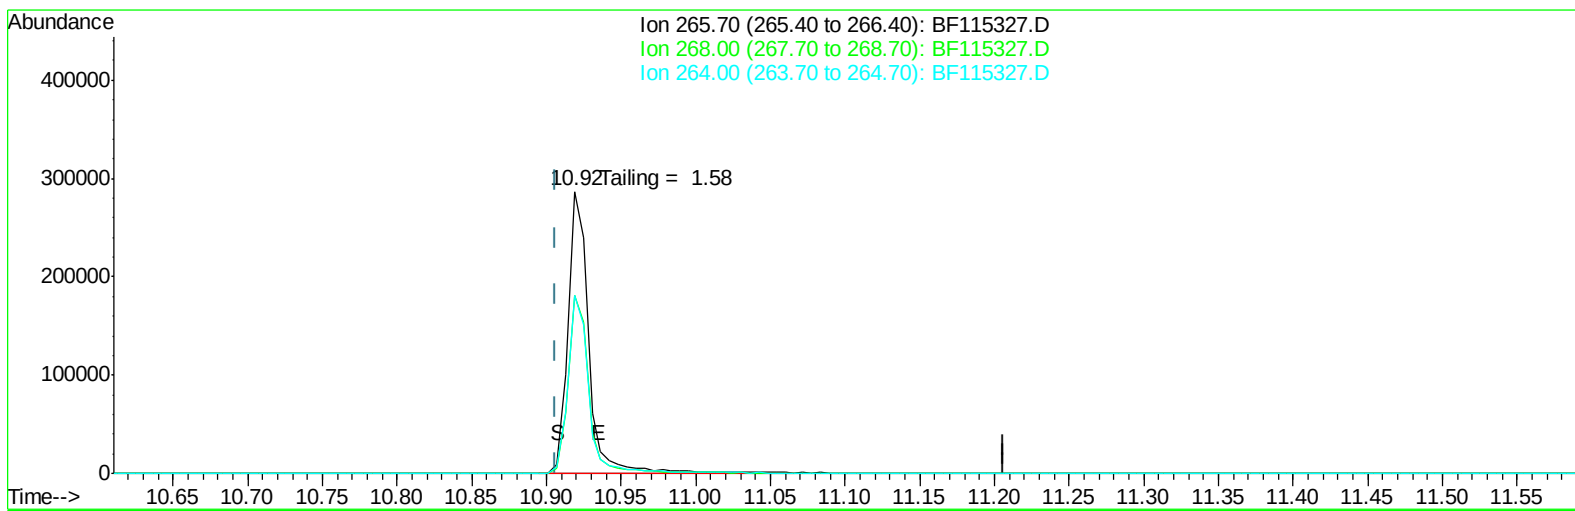

TIC: BF115327.D

(70) Pentachlorophenol (C)



10.919min (+0.012) 6244.80ng

response 275905

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	63.11
264.00	61.60	63.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070119\
Data File : BF115327.D
Acq On : 1 Jul 2019 9:02
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:14:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

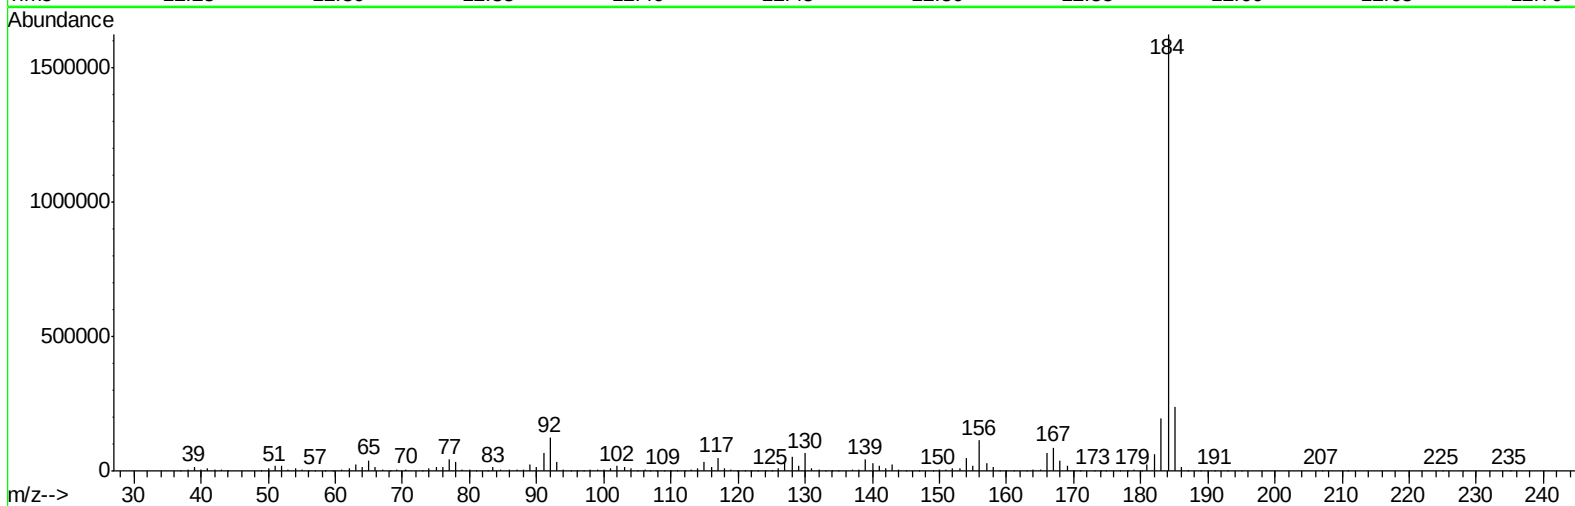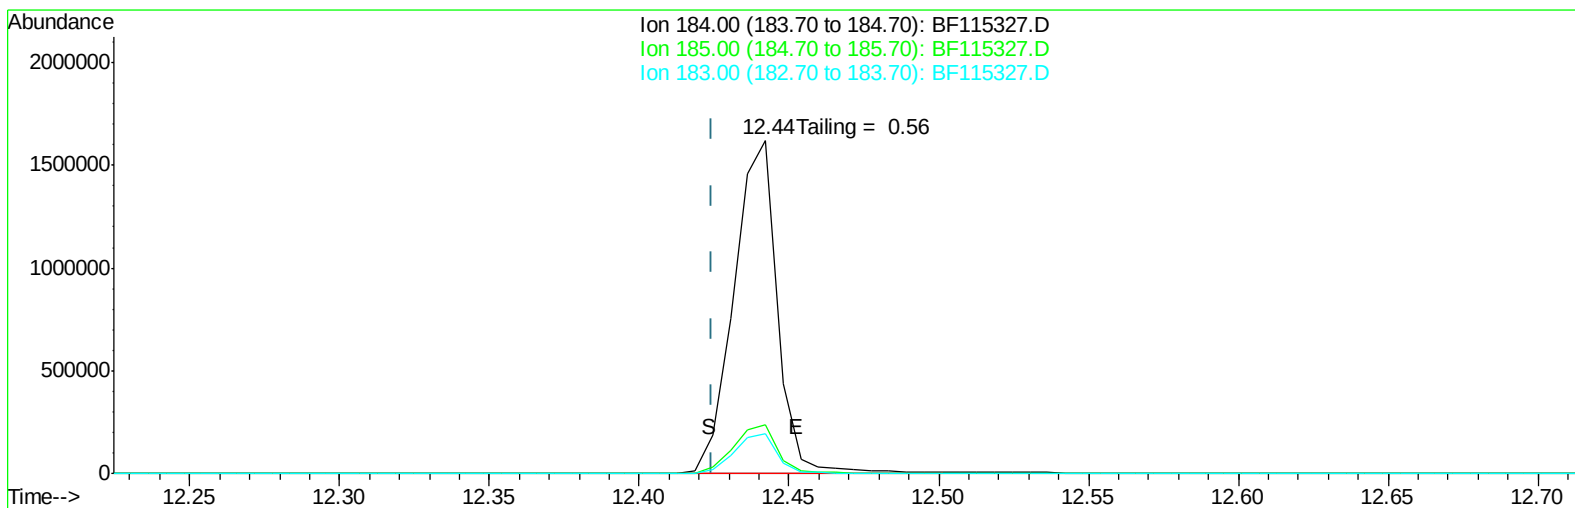

TIC: BF115327.D

(77) Benzidine

12.442min (+0.018) 3379.14ng

response 1661775

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.59
183.00	12.00	12.06
0.00	0.00	0.00