

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070119\
 Data File : BF115331.D
 Acq On : 1 Jul 2019 11:31
 Operator : HP/JU
 Sample : PB121019BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121019BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.213	551	557	560	rBV	5003073	5240214	76.25%	9.650%
2	6.248	727	733	736	rBV	4824154	5345696	77.79%	9.844%
3	6.372	749	754	757	rBV	5327690	5597158	81.45%	10.307%
4	6.601	789	793	797	rBV	1767539	1426091	20.75%	2.626%
5	6.760	815	820	823	rBV	5090230	4624236	67.29%	8.515%
6	7.166	883	889	892	rBV	3341924	3564653	51.87%	6.564%
7	7.884	1006	1011	1015	rBV	2060565	1815599	26.42%	3.343%
8	8.960	1188	1194	1198	rBV	5963226	6574934	95.68%	12.108%
9	9.630	1302	1308	1323	rBV	2387598	2092596	30.45%	3.853%
10	10.413	1436	1441	1445	rBV	3719861	3980033	57.92%	7.329%
11	11.107	1555	1559	1562	rBV	2587310	2218162	32.28%	4.085%
12	12.695	1823	1829	1832	rBV	6583430	6872113	100.00%	12.655%
13	13.724	2000	2004	2008	rBV	2282123	2162786	31.47%	3.983%
14	14.530	2138	2141	2145	rBV	68525	70126	1.02%	0.129%
15	14.830	2189	2192	2196	rVB	93370	90403	1.32%	0.166%
16	15.101	2233	2238	2243	rBV	1823675	2094207	30.47%	3.856%
17	15.165	2246	2249	2253	rVB	140274	156817	2.28%	0.289%
18	15.548	2310	2314	2320	rVB	139712	203381	2.96%	0.375%
19	15.989	2385	2389	2395	rVB	110565	174733	2.54%	0.322%


Sum of corrected areas: 54303938

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070119\
Data File : BF115331.D
Acq On : 1 Jul 2019 11:31
Operator : HP/JU
Sample : PB121019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121019BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

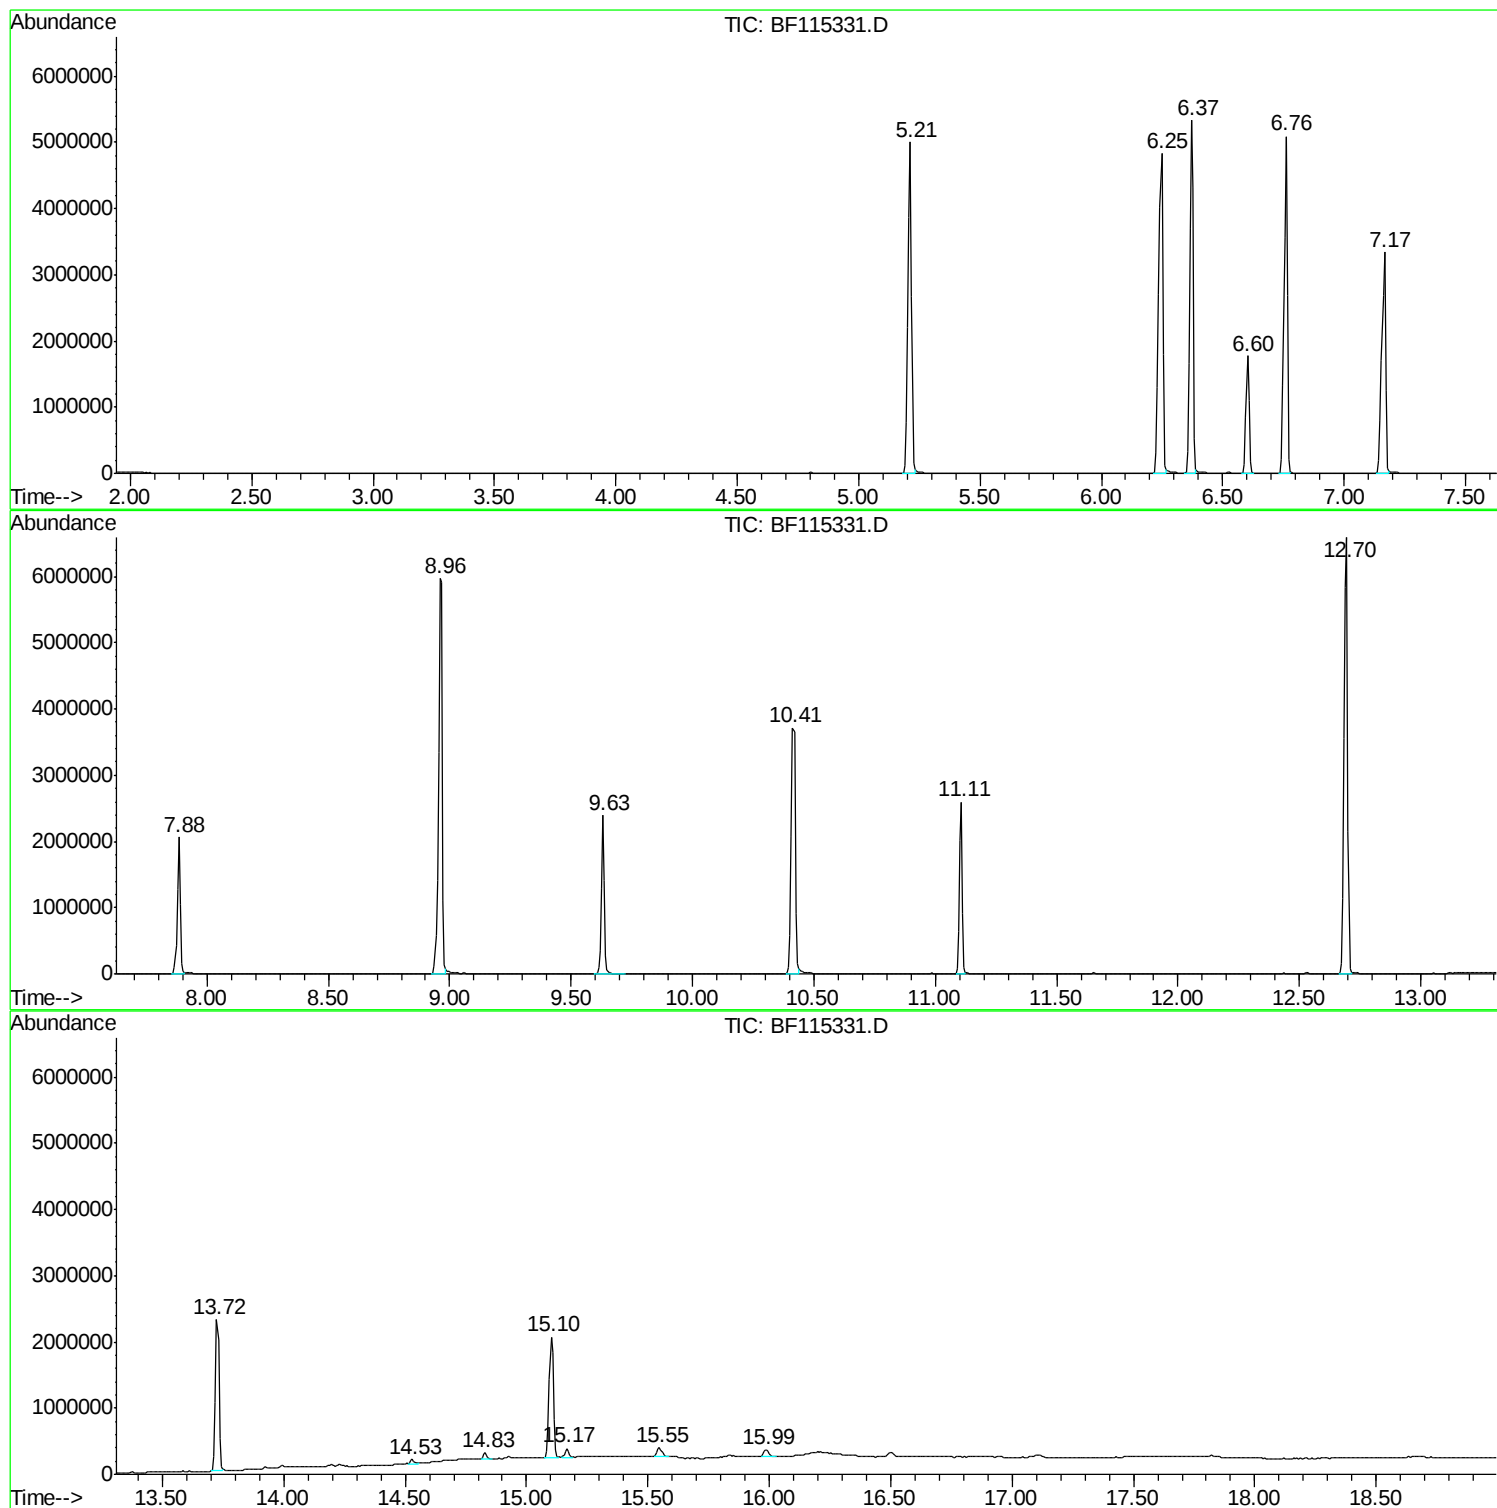

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070119\
Data File : BF115331.D
Acq On : 1 Jul 2019 11:31
Operator : HP/JU
Sample : PB121019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121019BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	78.50 ng	5597160	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

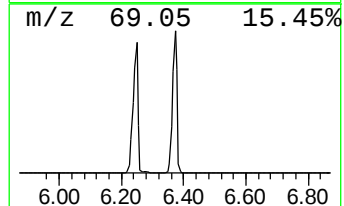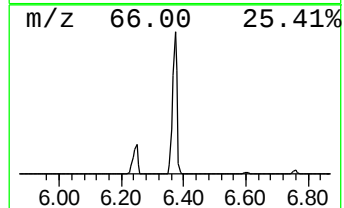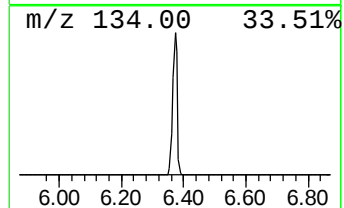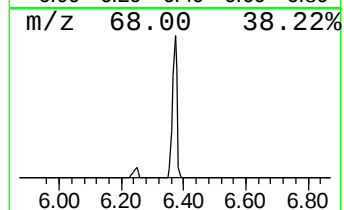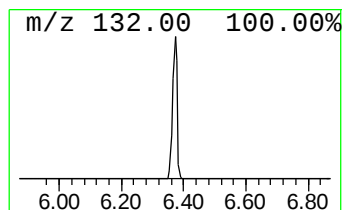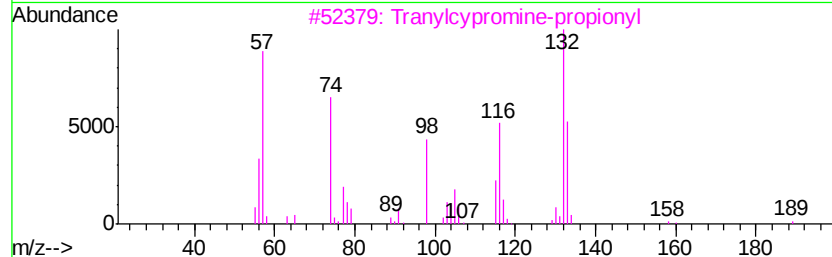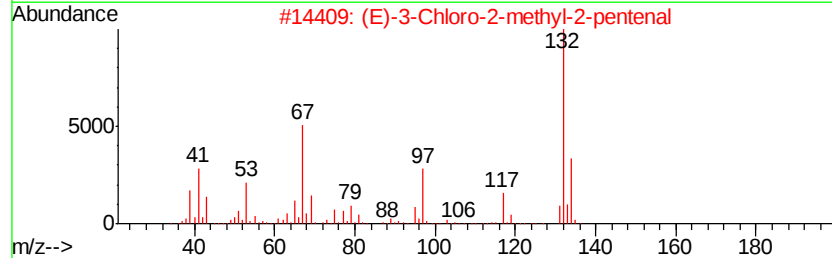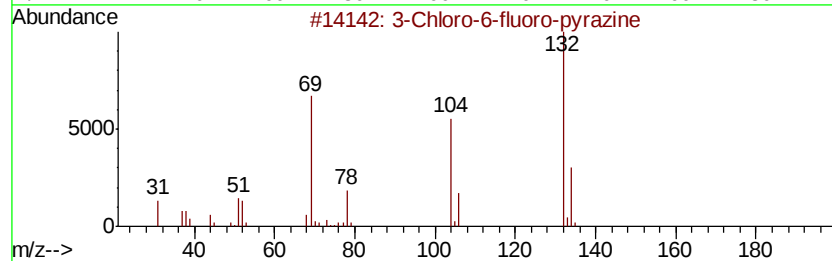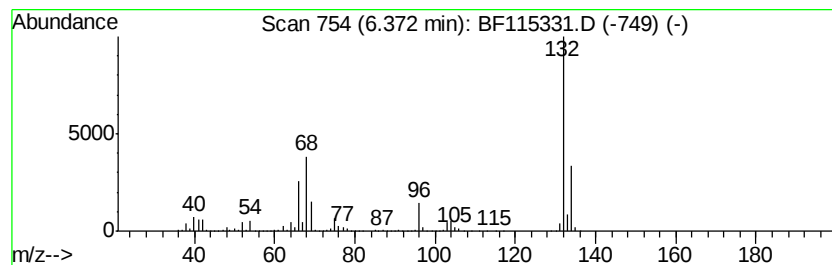

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070119\
Data File : BF115331.D
Acq On : 1 Jul 2019 11:31
Operator : HP/JU
Sample : PB121019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121019BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.37	6.37	78.5	ng	5597160	1	6.60	1426090	20.0