


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070119\
 Data File : BF115327.D
 Acq On : 1 Jul 2019 9:02
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:26:43 2019

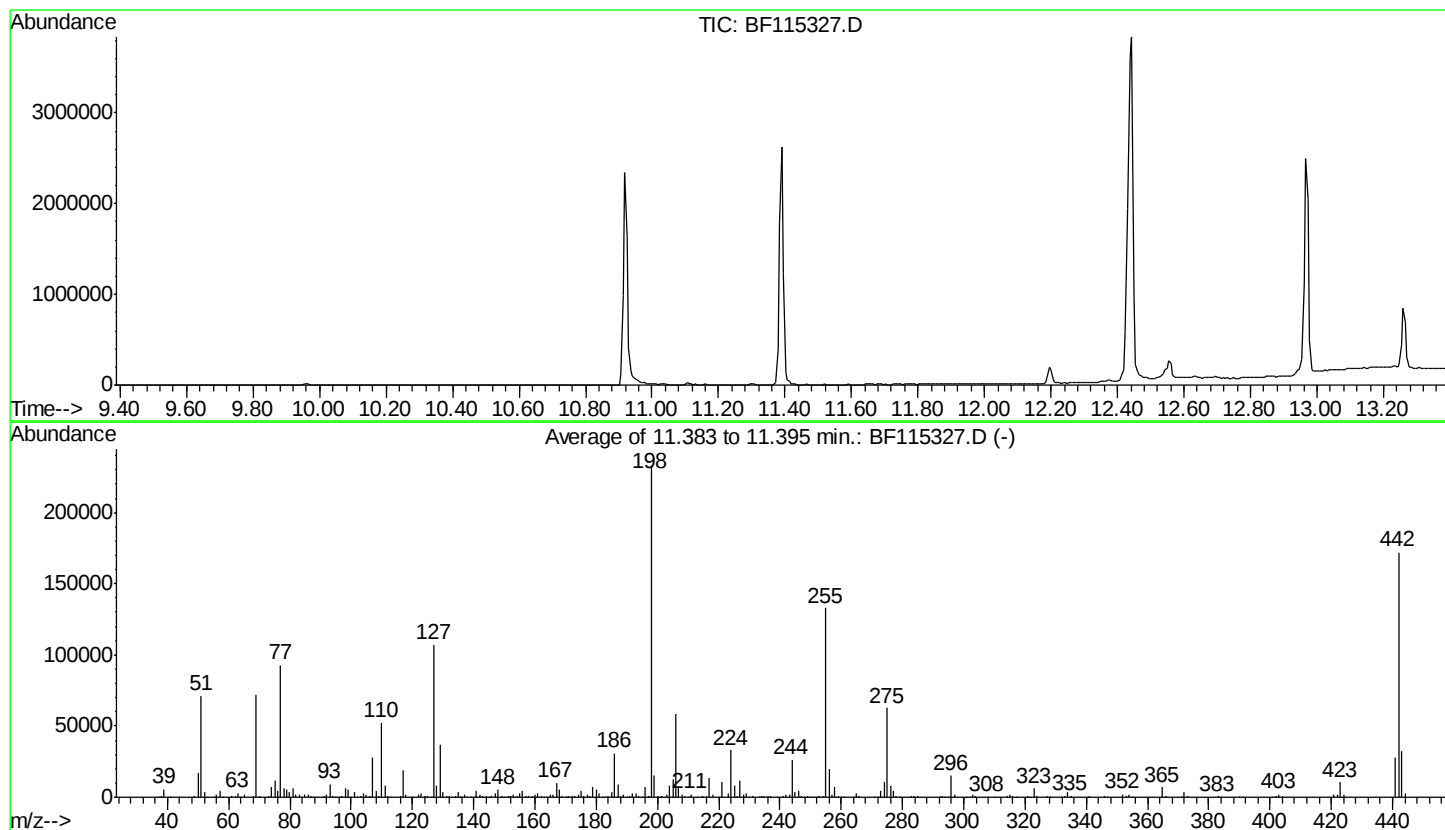

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	71442	PASS
68	69	0.00	2	1.8	1287	PASS
69	198	0.00	100	30.8	71799	PASS
70	69	0.00	2	0.8	603	PASS
127	198	10	80	46.0	107120	PASS
197	198	0.00	2	0.4	943	PASS
198	198	100	100	100.0	233002	PASS
199	198	5	9	6.6	15417	PASS
275	198	10	60	26.9	62594	PASS
365	198	1	100	3.0	7009	PASS
441	198	0.01	100	11.8	27492	PASS
442	198	50	100	73.9	172112	PASS
443	442	15	24	19.0	32704	PASS