
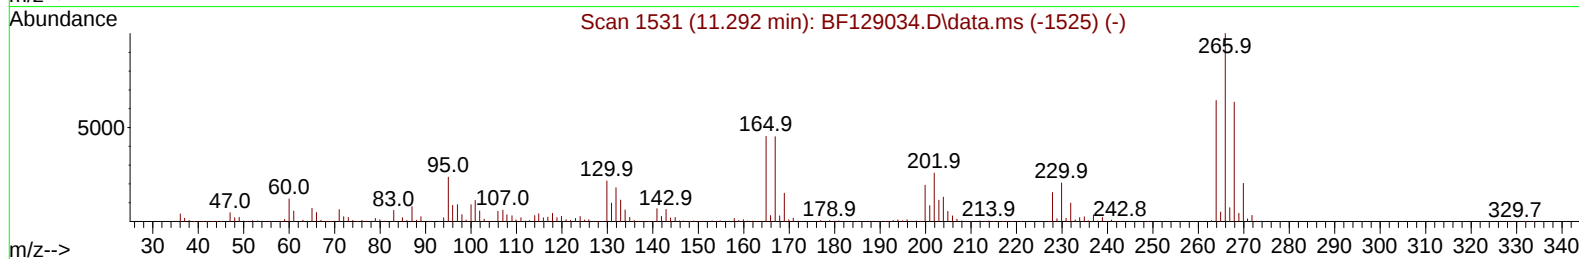
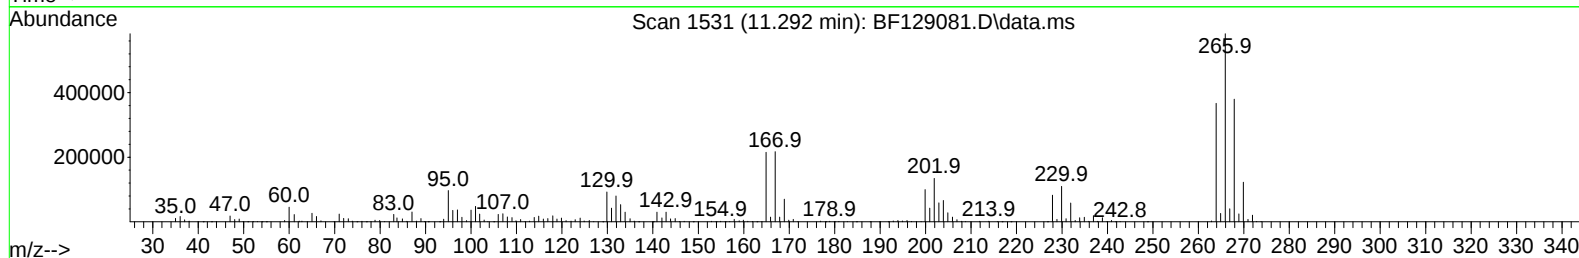


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129081.D
Acq On : 01 Jul 2022 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 03:59:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

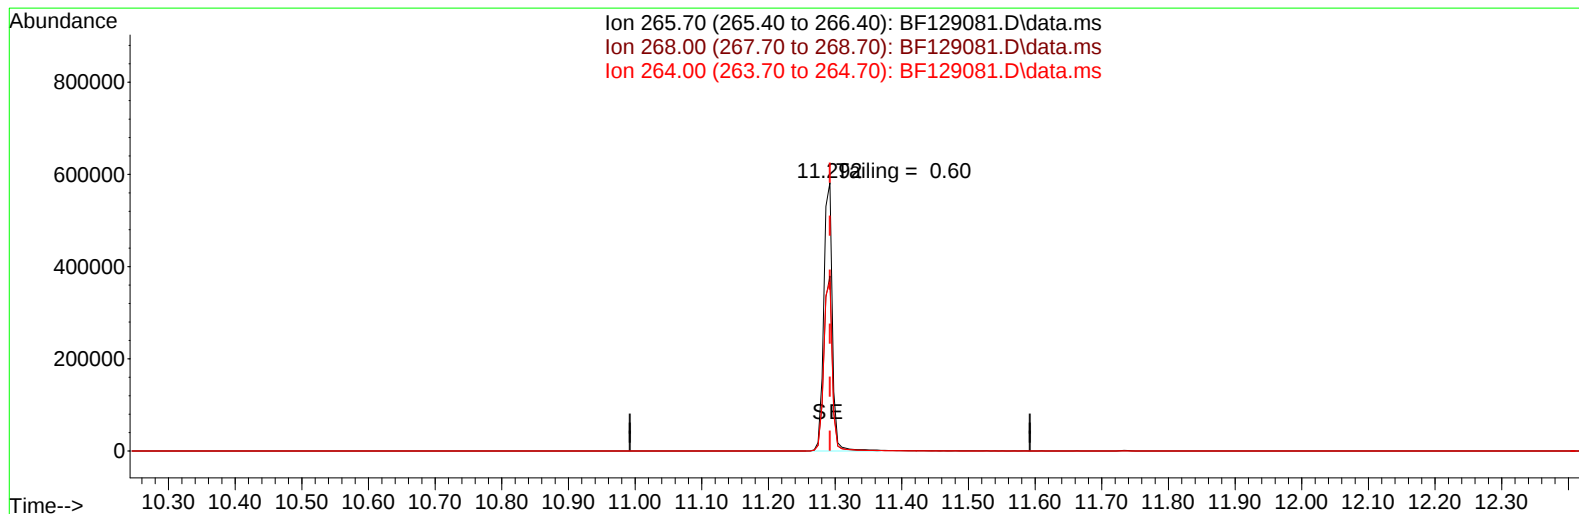

TIC: BF129081.D\data.ms




(70) Pentachlorophenol (C)

11.292min (-0.000) 183959.80 ng

response 524329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.18
264.00	61.80	62.97
0.00	0.00	0.00

Quant Time: Jul 02 03:59:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

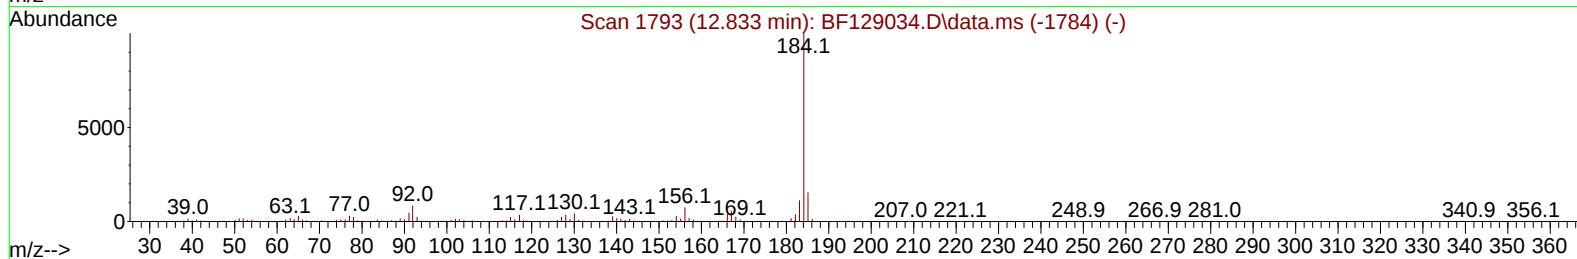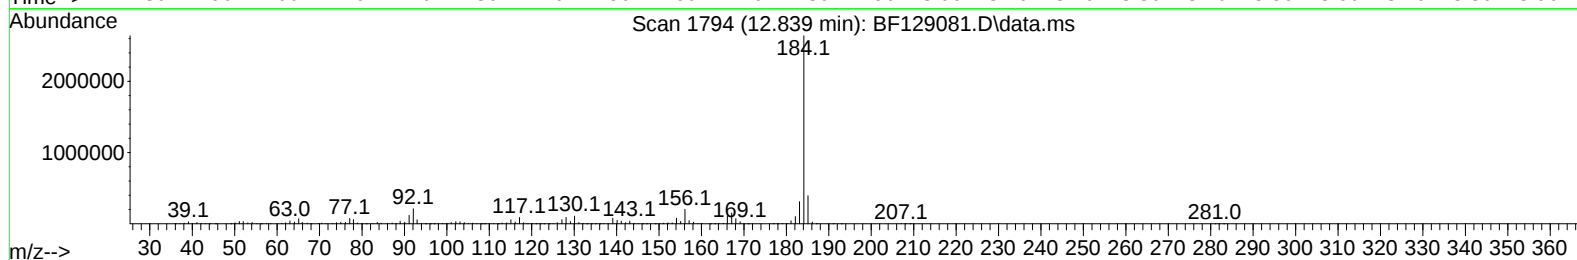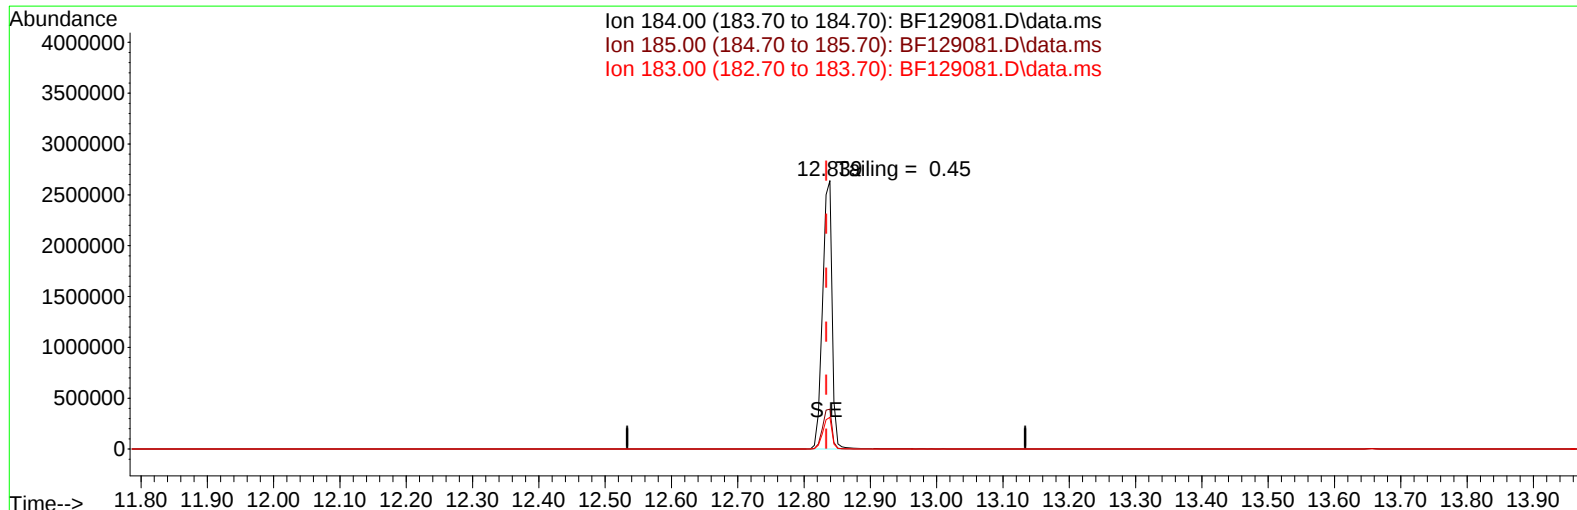

TIC: BF129081.D\data.ms

(77) Benzidine

12.839min (+ 0.006) 238953.64 ng

response 2646541

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	14.89
--------	-------	-------

183.00	11.60	11.79
--------	-------	-------

0.00 0.00 0.00