

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129087.D
 Acq On : 01 Jul 2022 12:16
 Operator : CG\JU
 Sample : PB145957BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145957BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.393	8	18	24	rVB	224898	324595	2.57%	0.423%
2	5.593	556	562	565	rBV	8908646	9544138	75.48%	12.425%
3	6.581	723	730	733	rBV	7769839	9344302	73.90%	12.165%
4	6.951	790	793	797	rVB	2535059	2271859	17.97%	2.958%
5	7.516	883	889	892	rBV	5622570	6445934	50.98%	8.391%
6	8.239	1006	1012	1015	rBV	3052947	3076540	24.33%	4.005%
7	9.316	1188	1195	1198	rBV	11291337	11805846	93.37%	15.369%
8	9.998	1305	1311	1314	rBV	3933015	3448480	27.27%	4.489%
9	10.792	1439	1446	1449	rBV	7740872	7580047	59.95%	9.868%
10	11.486	1558	1564	1568	rBV	3812528	3600697	28.48%	4.687%
11	13.080	1830	1835	1839	rBV	11527480	12644522	100.00%	16.461%
12	14.139	2011	2015	2018	rBV	3713342	3194770	25.27%	4.159%
13	14.233	2025	2031	2038	rBV	203076	253852	2.01%	0.330%
14	15.663	2268	2274	2283	rBV	2221094	2908241	23.00%	3.786%
15	16.133	2350	2354	2361	rVB	123744	192506	1.52%	0.251%
16	16.674	2441	2446	2455	rBV3	99643	179518	1.42%	0.234%




Sum of corrected areas: 76815847

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129087.D
Acq On : 01 Jul 2022 12:16
Operator : CG\JU
Sample : PB145957BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

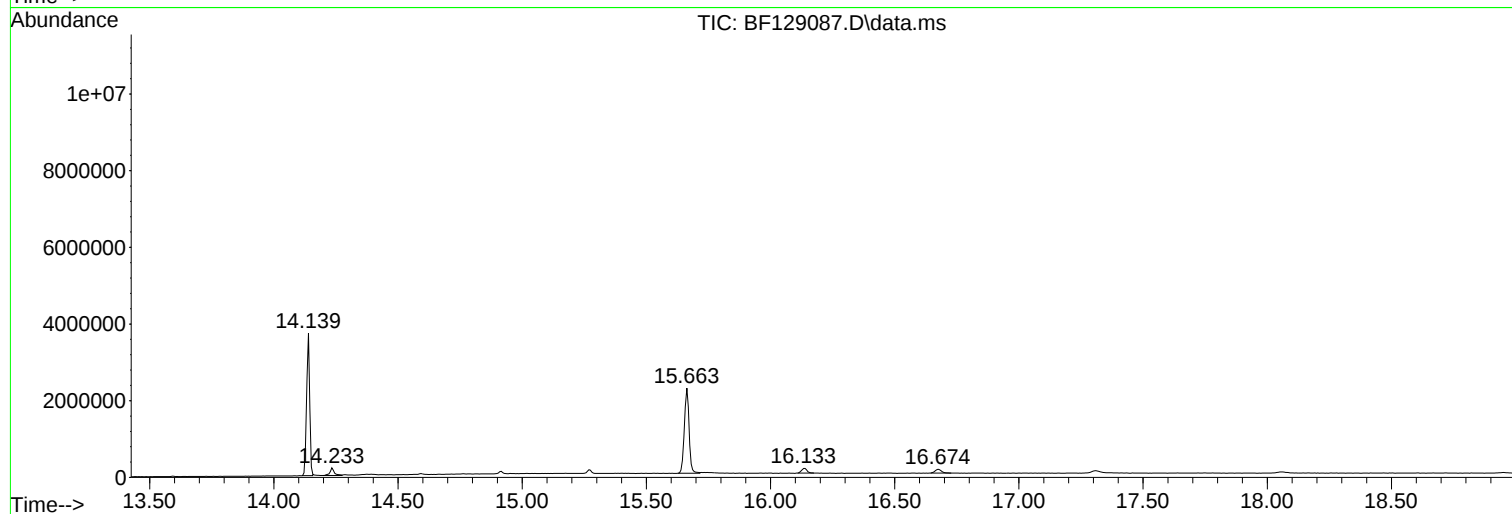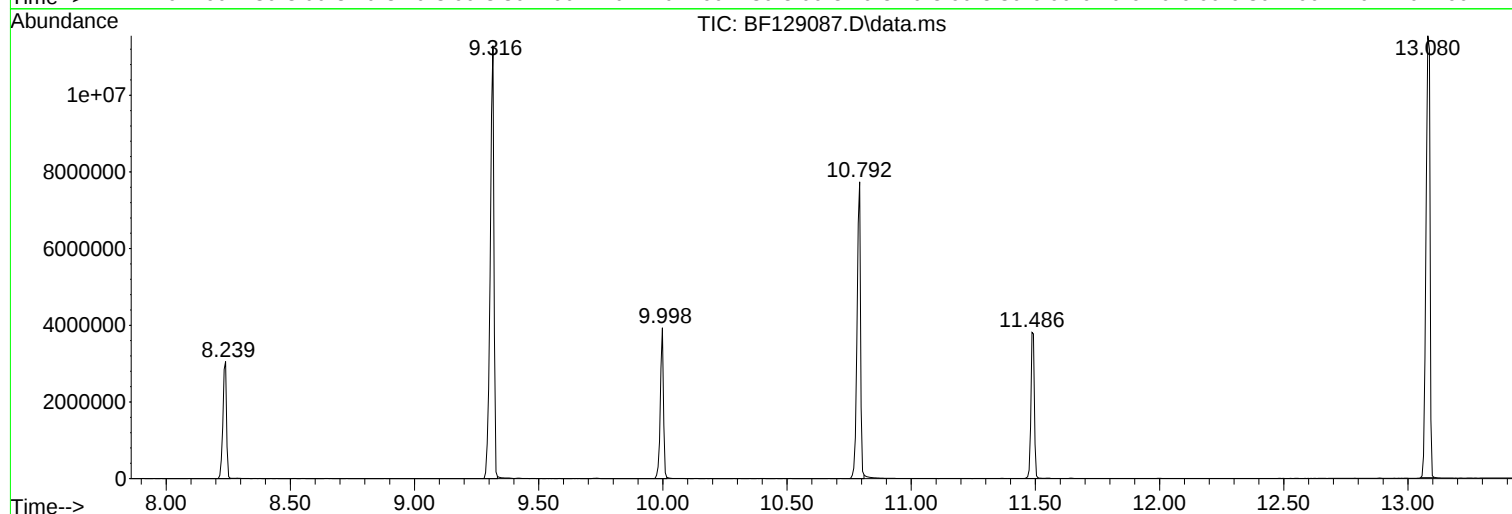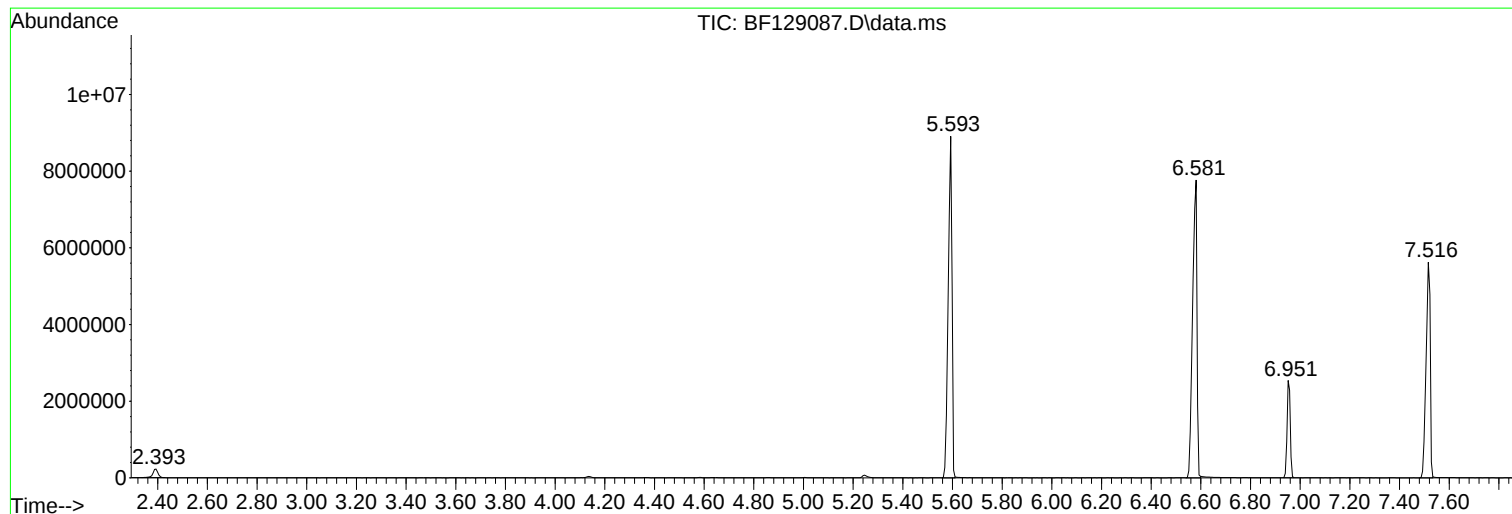

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129087.D
Acq On : 01 Jul 2022 12:16
Operator : CG\JU
Sample : PB145957BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145957BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.393	2.86 ng	324595	1,4-Dichlorobenzene-d4	6.951

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

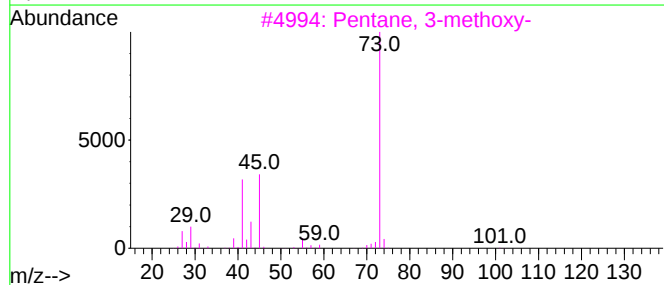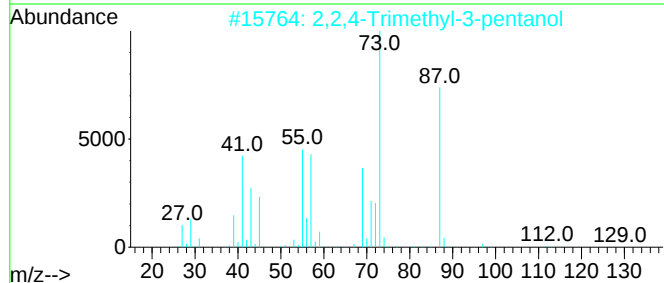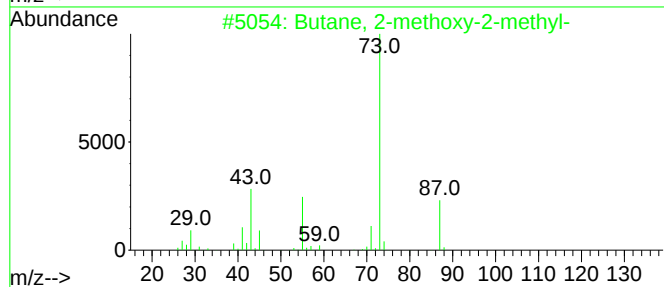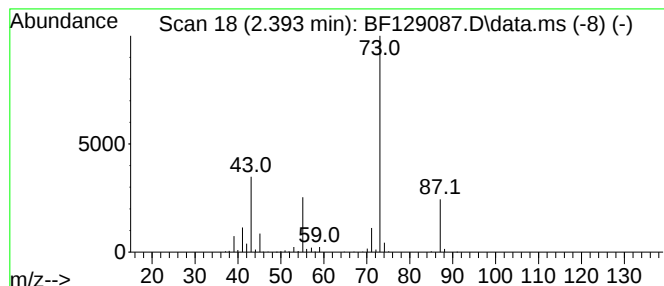

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129087.D
Acq On : 01 Jul 2022 12:16
Operator : CG\JU
Sample : PB145957BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145957BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.393	2.9	ng	324595	1	6.951	2271860	20.0