

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129100.D
 Acq On : 01 Jul 2022 19:27
 Operator : CG\JU
 Sample : N3561-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.204	493	496	506	rVB	77793	94681	1.31%	0.200%
2	5.575	555	559	563	rBV	5470000	5569160	76.91%	11.746%
3	6.575	723	729	732	rBV	5725441	5557645	76.75%	11.721%
4	6.957	790	794	797	rBV	1928615	1730317	23.90%	3.649%
5	7.516	884	889	892	rBV	4336072	3771916	52.09%	7.955%
6	8.239	1007	1012	1015	rBV	2563027	2327213	32.14%	4.908%
7	9.310	1190	1194	1198	rBV	7762977	7241027	100.00%	15.272%
8	9.998	1306	1311	1314	rBV	2902872	2641385	36.48%	5.571%
9	10.786	1441	1445	1448	rBV	5231909	4388188	60.60%	9.255%
10	11.486	1560	1564	1568	rBV	3182629	2725461	37.64%	5.748%
11	11.868	1626	1629	1635	rVB	217352	161513	2.23%	0.341%
12	11.998	1647	1651	1656	rBV	99106	99284	1.37%	0.209%
13	13.080	1830	1835	1838	rBV	7318014	7118091	98.30%	15.012%
14	14.133	2011	2014	2018	rBV	1981696	1890902	26.11%	3.988%
15	14.233	2026	2031	2037	rBV	329359	354458	4.90%	0.748%
16	14.762	2117	2121	2124	rBV	104417	102194	1.41%	0.216%
17	14.909	2143	2146	2151	rBV	68607	76680	1.06%	0.162%
18	15.656	2268	2273	2283	rBV2	1156925	1564616	21.61%	3.300%




Sum of corrected areas: 47414731

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129100.D
Acq On : 01 Jul 2022 19:27
Operator : CG\JU
Sample : N3561-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

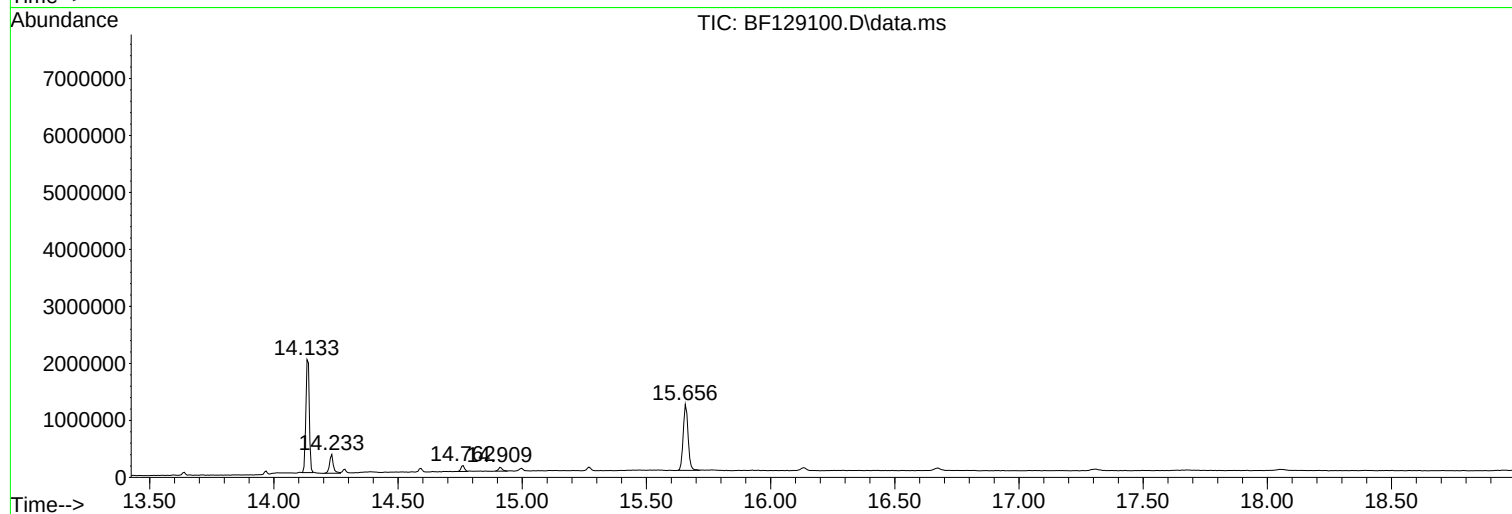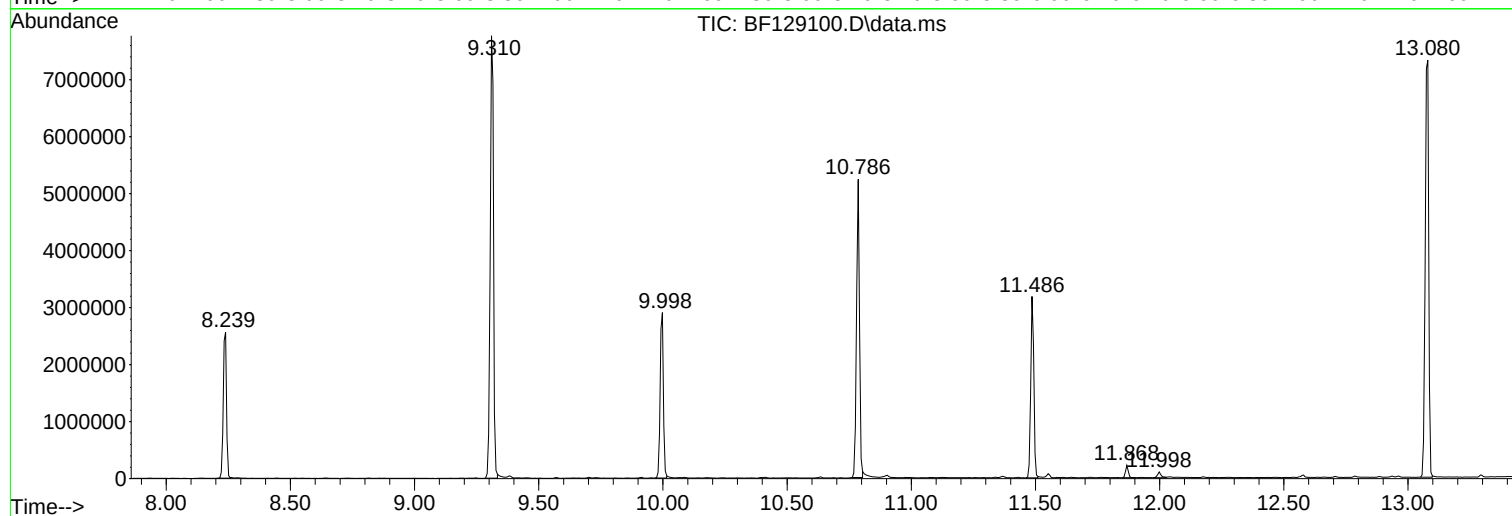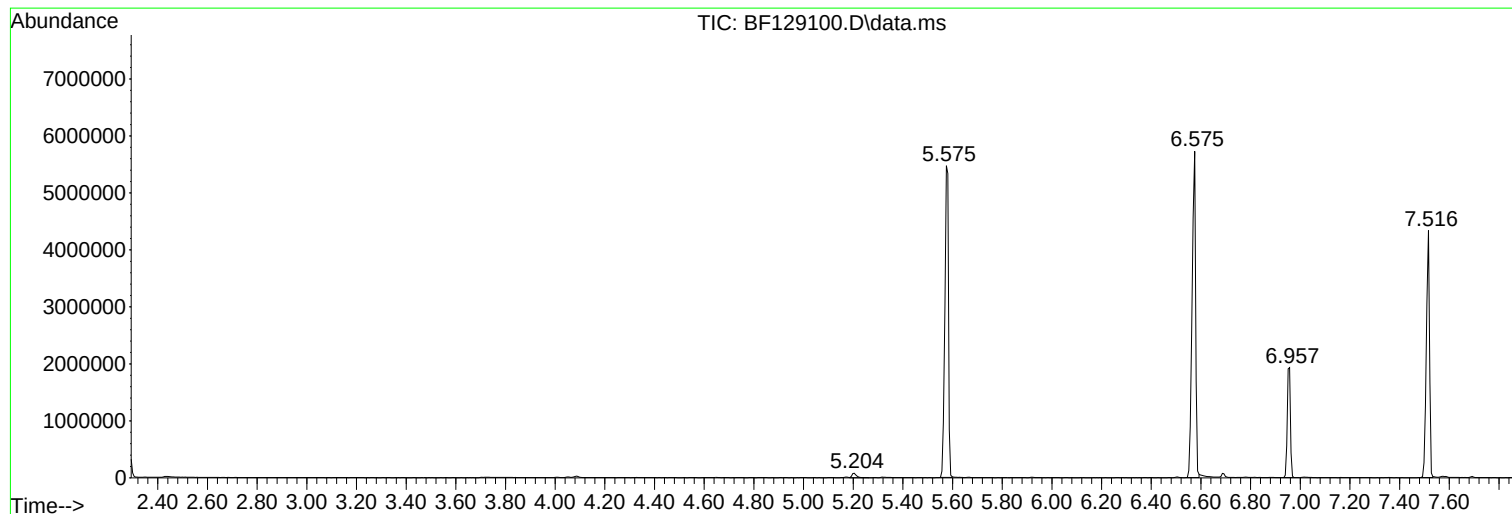

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129100.D
Acq On : 01 Jul 2022 19:27
Operator : CG\JU
Sample : N3561-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.233	3.75 ng	354458	Chrysene-d12	14.133

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	38
4			1H-Indol-4-ol, 2TMS derivative	277	C14H23NOSi2	1000485-28-1	33
5			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28

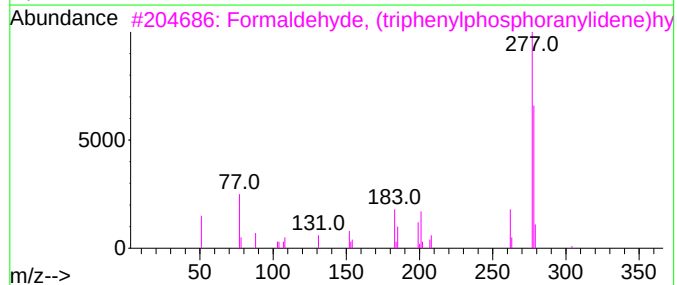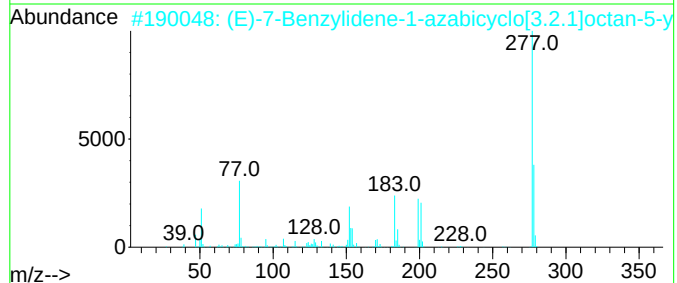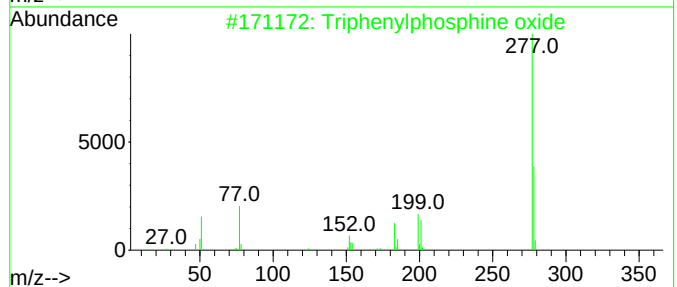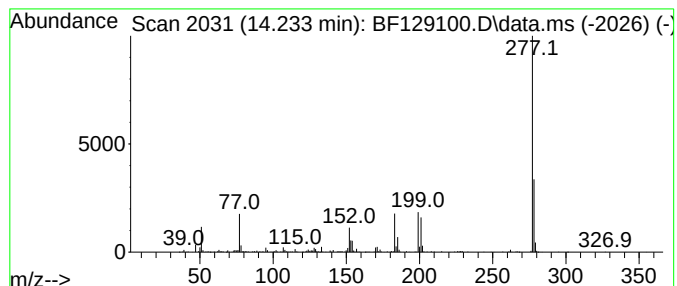

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129100.D
Acq On : 01 Jul 2022 19:27
Operator : CG\JU
Sample : N3561-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.233	3.8	ng	354458	5	14.133	1890900	20.0