

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129101.D
 Acq On : 01 Jul 2022 19:57
 Operator : CG\JU
 Sample : N3562-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-17

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129101.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.581	555	560	563	rBV	5680698	5671154	74.79%	11.132%
2	6.575	723	729	732	rBV	5813813	5668551	74.75%	11.127%
3	6.951	790	793	797	rBV	2270712	2018921	26.62%	3.963%
4	7.516	884	889	892	rBV	4410607	3829582	50.50%	7.517%
5	8.239	1007	1012	1015	rBV	3052878	2739998	36.13%	5.378%
6	9.310	1189	1194	1198	rBV	8037301	7583269	100.00%	14.885%
7	9.998	1307	1311	1314	rBV	3548495	3028589	39.94%	5.945%
8	10.786	1441	1445	1448	rBV	5184484	4354842	57.43%	8.548%
9	11.486	1560	1564	1567	rBV	3707825	3113220	41.05%	6.111%
10	11.510	1567	1568	1572	rVB	173889	105820	1.40%	0.208%
11	11.998	1646	1651	1657	rBV2	174389	227413	3.00%	0.446%
12	12.704	1767	1771	1776	rBV	317016	269275	3.55%	0.529%
13	12.933	1808	1810	1813	rVB	291127	227037	2.99%	0.446%
14	13.074	1830	1834	1838	rBV	7308183	6831121	90.08%	13.409%
15	14.133	2010	2014	2017	rBV	2014904	2033394	26.81%	3.991%
16	14.162	2017	2019	2024	rVB	145201	133456	1.76%	0.262%
17	14.233	2026	2031	2036	rBV	384544	419056	5.53%	0.823%
18	15.204	2192	2196	2199	rBV	107090	158265	2.09%	0.311%
19	15.268	2204	2207	2212	rVB	94096	105414	1.39%	0.207%
20	15.521	2248	2250	2257	rVB	73552	93890	1.24%	0.184%
21	15.586	2258	2261	2267	rVV	83864	113423	1.50%	0.223%
22	15.656	2268	2273	2287	rVB	1413403	1963086	25.89%	3.853%
23	16.133	2350	2354	2361	rVB2	94545	143443	1.89%	0.282%
24	16.668	2442	2445	2452	rVB2	69143	113380	1.50%	0.223%




Sum of corrected areas: 50945599

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129101.D
Acq On : 01 Jul 2022 19:57
Operator : CG\JU
Sample : N3562-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

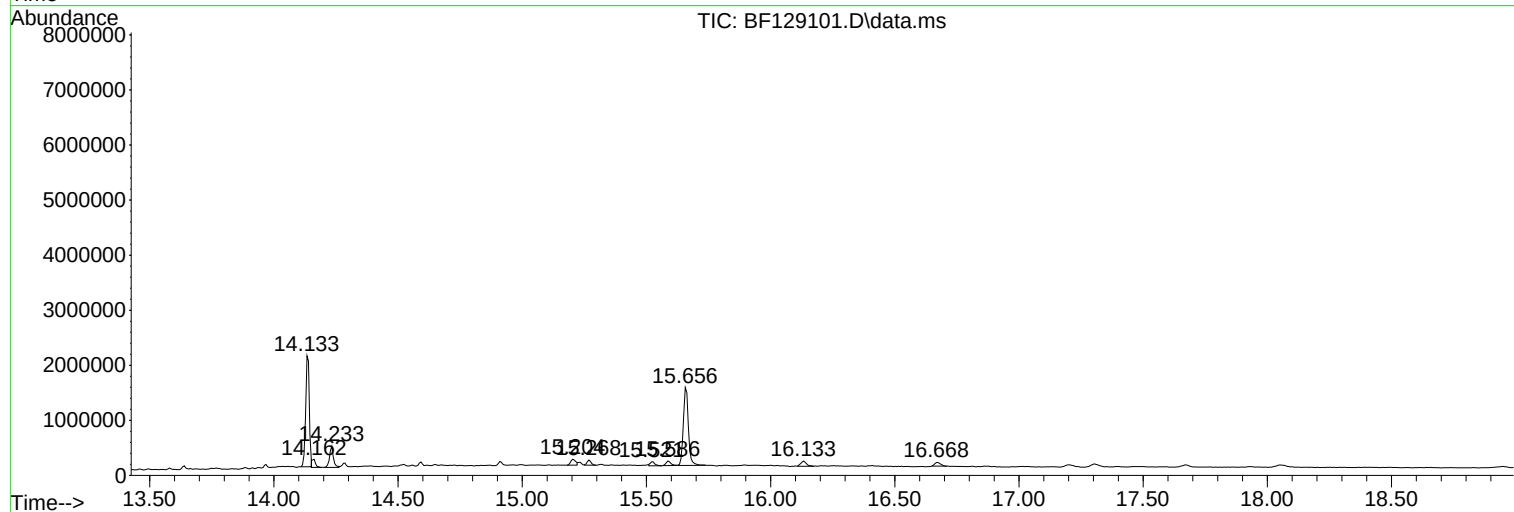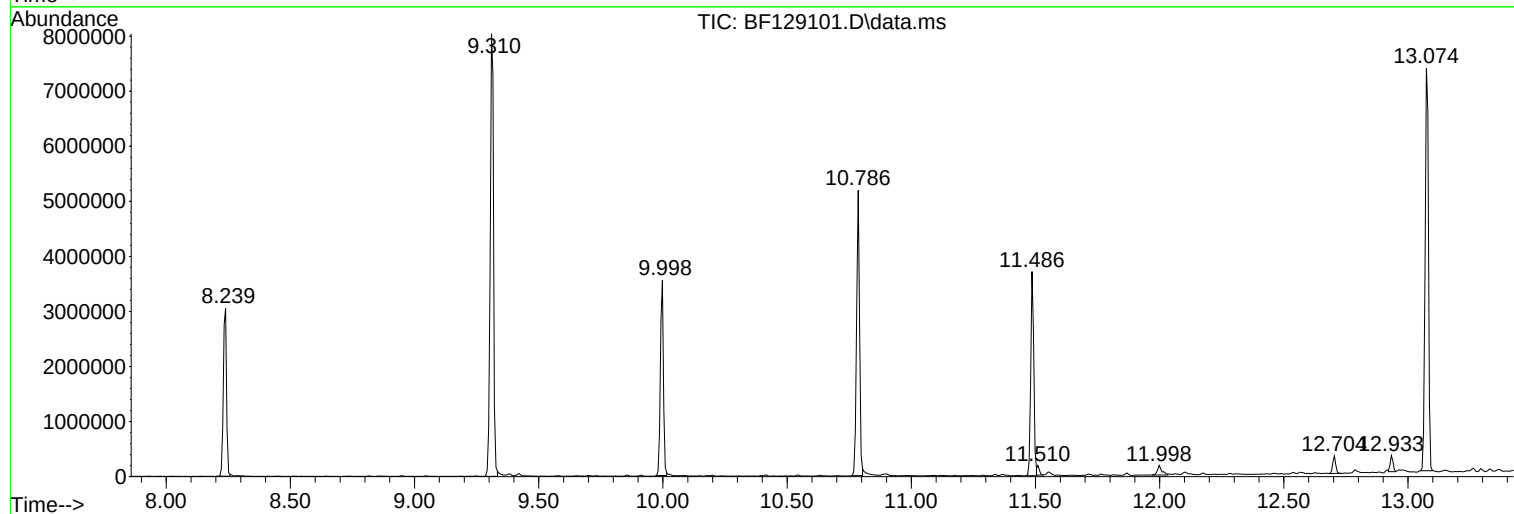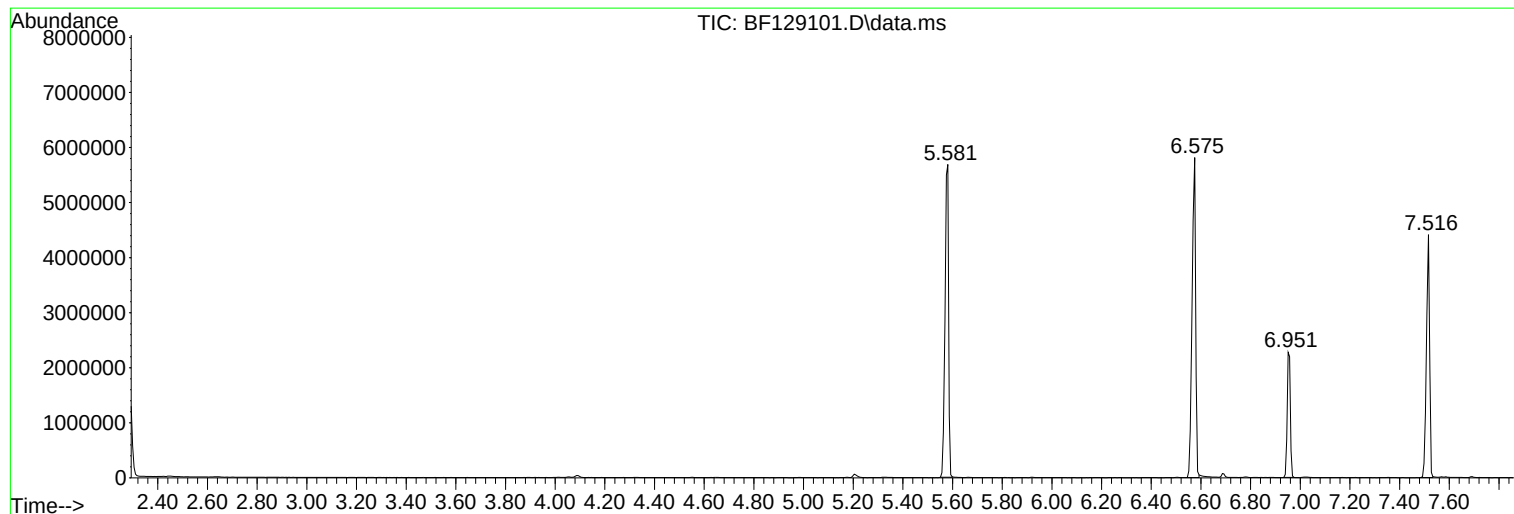

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129101.D
Acq On : 01 Jul 2022 19:57
Operator : CG\JU
Sample : N3562-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-17










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.233	4.12 ng	419056	Chrysene-d12	14.139

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	94
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	59
4			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	53
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	42

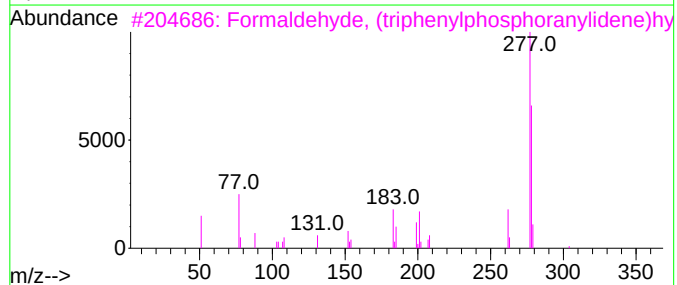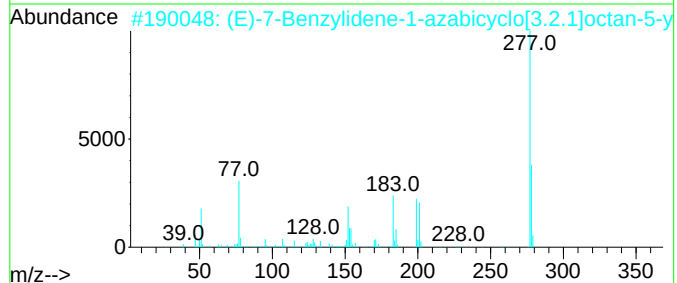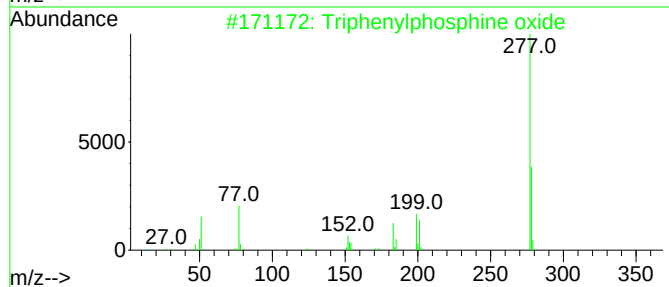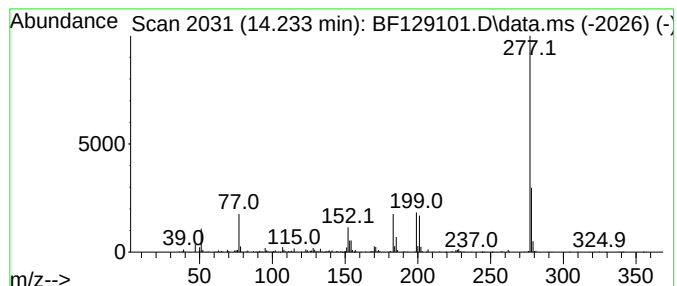

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129101.D
Acq On : 01 Jul 2022 19:57
Operator : CG\JU
Sample : N3562-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.233	4.1	ng	419056	5	14.139	2033390	20.0