

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129109.D
 Acq On : 01 Jul 2022 23:59
 Operator : CG\JU
 Sample : N3562-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-8A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129109.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.581	555	560	563	rBV	6520107	6088088	87.27%	11.495%
2	6.575	724	729	732	rBV	5448664	5987756	85.83%	11.305%
3	6.957	790	794	797	rBV	2358962	1873825	26.86%	3.538%
4	7.516	884	889	892	rBV	4267951	3984549	57.12%	7.523%
5	8.239	1008	1012	1015	rBV	3002331	2427764	34.80%	4.584%
6	9.316	1190	1195	1198	rBV	8117770	6975969	100.00%	13.171%
7	9.998	1307	1311	1314	rBV	2927049	2293762	32.88%	4.331%
8	10.027	1314	1316	1320	rVB	171771	143917	2.06%	0.272%
9	10.545	1400	1404	1409	rBV	148866	128436	1.84%	0.242%
10	10.786	1441	1445	1456	rBV	4009762	3464371	49.66%	6.541%
11	11.345	1535	1540	1543	rBV3	53625	84852	1.22%	0.160%
12	11.492	1561	1565	1567	rBV	2210262	2099834	30.10%	3.965%
13	11.516	1567	1569	1572	rVV	1366021	1089252	15.61%	2.057%
14	11.563	1573	1577	1580	rVB	364304	310552	4.45%	0.586%
15	11.716	1599	1603	1609	rBV2	77175	105064	1.51%	0.198%
16	12.004	1647	1652	1653	rBV2	363859	424943	6.09%	0.802%
17	12.021	1653	1655	1658	rVB	182010	158376	2.27%	0.299%
18	12.104	1666	1669	1672	rBV2	210938	238294	3.42%	0.450%
19	12.286	1697	1700	1702	rBV	111745	93952	1.35%	0.177%
20	12.710	1768	1772	1775	rBV	1643946	1496894	21.46%	2.826%
21	12.792	1783	1786	1790	rBV2	150359	154368	2.21%	0.291%
22	12.939	1808	1811	1814	rVB	1442220	1146112	16.43%	2.164%
23	13.080	1828	1835	1838	rBV	5641084	5470603	78.42%	10.329%
24	13.263	1864	1866	1869	rVB	219053	196895	2.82%	0.372%
25	13.333	1875	1878	1880	rBV	170810	135724	1.95%	0.256%
26	14.139	2010	2015	2018	rBV2	2271421	2629752	37.70%	4.965%
27	14.162	2018	2019	2025	rVB	553354	497048	7.13%	0.938%
28	14.239	2029	2032	2036	rVB2	395977	482585	6.92%	0.911%
29	15.215	2195	2198	2201	rBV	342451	487934	6.99%	0.921%
30	15.598	2261	2263	2268	rVB	329249	400539	5.74%	0.756%
31	15.668	2271	2275	2284	rVB	1265945	1892987	27.14%	3.574%




Sum of corrected areas: 52964997

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129109.D
Acq On : 01 Jul 2022 23:59
Operator : CG\JU
Sample : N3562-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

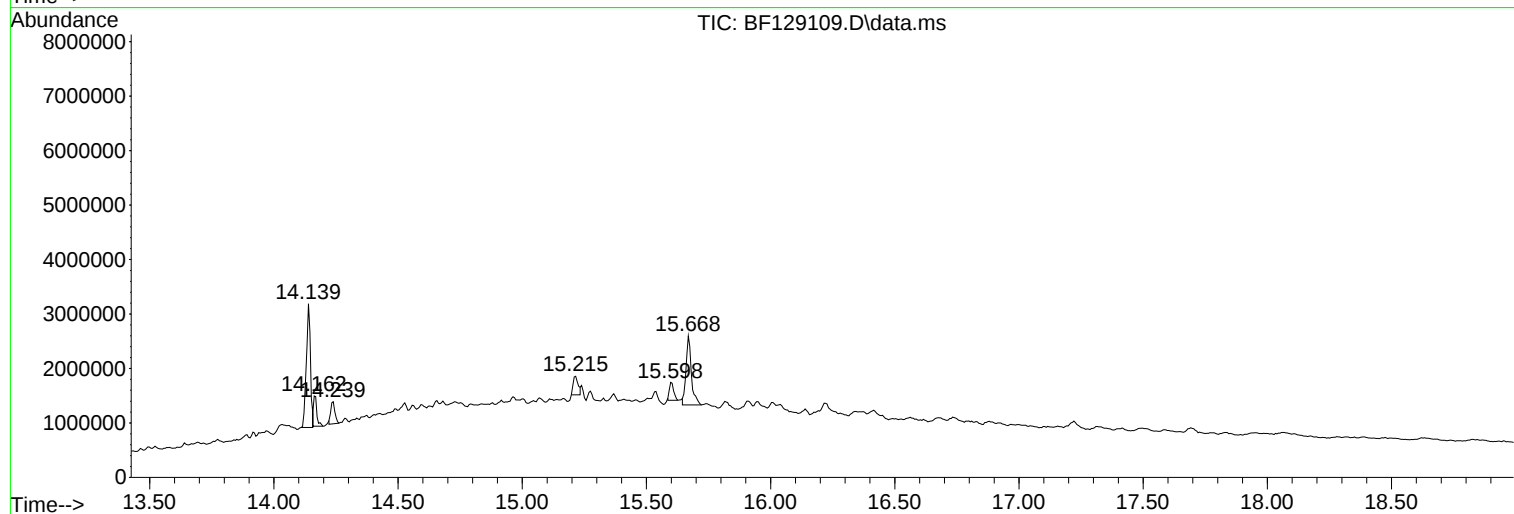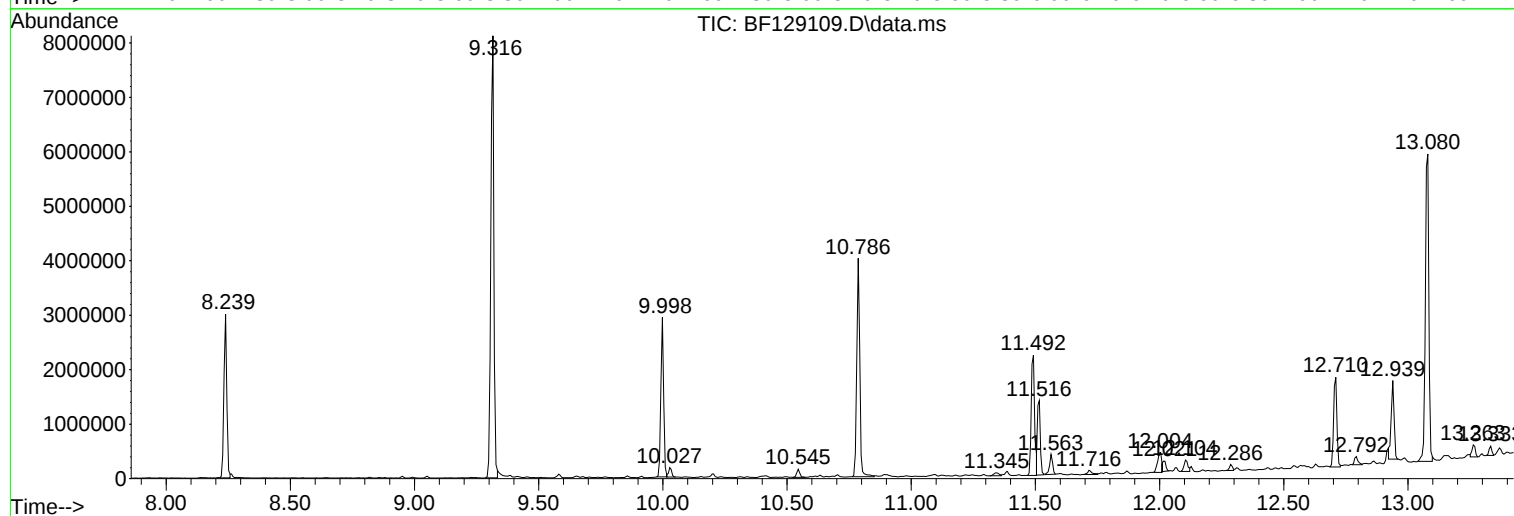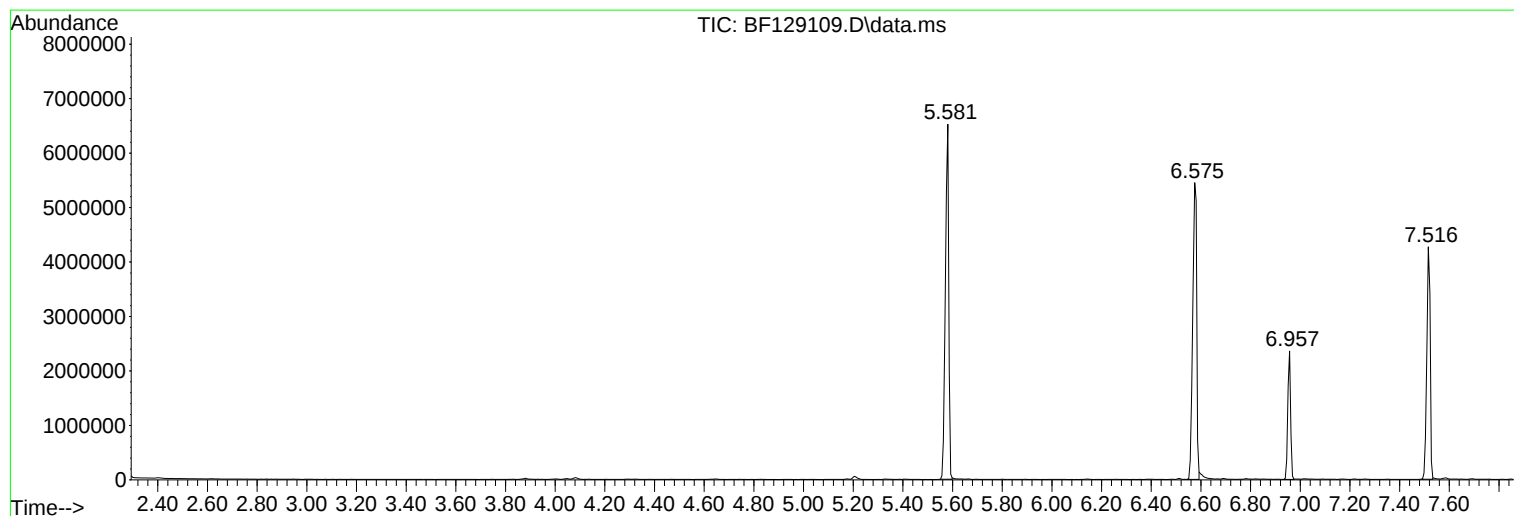

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129109.D
Acq On : 01 Jul 2022 23:59
Operator : CG\JU
Sample : N3562-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129109.D
Acq On : 01 Jul 2022 23:59
Operator : CG\JU
Sample : N3562-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-8A

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc